

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014530.D
 Acq On : 04 Apr 2023 16:19
 Operator : CG/JU
 Sample : 02123-01
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9A0

Quant Time: Apr 04 23:45:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 04 23:43:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.005	152	113173	20.000	ng/u1	0.00
20) Naphthalene-d8	10.822	136	476869	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.657	164	320971	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.416	188	753171	20.000	ng/u1	0.00
79) Chrysene-d12	21.504	240	783259	20.000	ng/u1	0.00
88) Perylene-d12	24.021	264	879207	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	15704	5.381	ng/uL	0.00
4) Pyridine-d5	3.822	84	112678	15.066	ng/u1	0.01
7) Phenol-d5	7.175	99	102900	9.859	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.328	67	207773	31.026	ng/u1	0.00
11) 2-Chlorophenol-d4	7.534	132	202665	26.865	ng/u1	0.00
15) 4-Methylphenol-d8	8.728	113	190196	22.591	ng/u1	0.00
21) Nitrobenzene-d5	9.181	128	120995	31.430	ng/u1	0.00
24) 2-Nitrophenol-d4	9.904	143	133421	30.267	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	252227	31.418	ng/u1	0.00
31) 4-Chloroaniline-d4	10.975	131	204382	19.328	ng/u1	0.00
46) Dimethylphthalate-d6	14.063	166	928730	35.686	ng/u1	0.00
49) Acenaphthylene-d8	14.351	160	1028134	35.603	ng/u1	0.00
54) 4-Nitrophenol-d4	14.910	143	40175	10.218	ng/u1	0.02
60) Fluorene-d10	15.651	176	800470	36.883	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.781	200	158203	28.546	ng/u1	0.00
73) Anthracene-d10	17.516	188	1318998	36.186	ng/u1	0.00
81) Pyrene-d10	19.745	212	1649587	31.354	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.857	264	1705236	36.505	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.417	88	51558	16.076	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014530.D
Acq On : 04 Apr 2023 16:19
Operator : CG/JU
Sample : 02123-01
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A0

Quant Time: Apr 04 23:45:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 04 23:43:56 2023
Response via : Initial Calibration

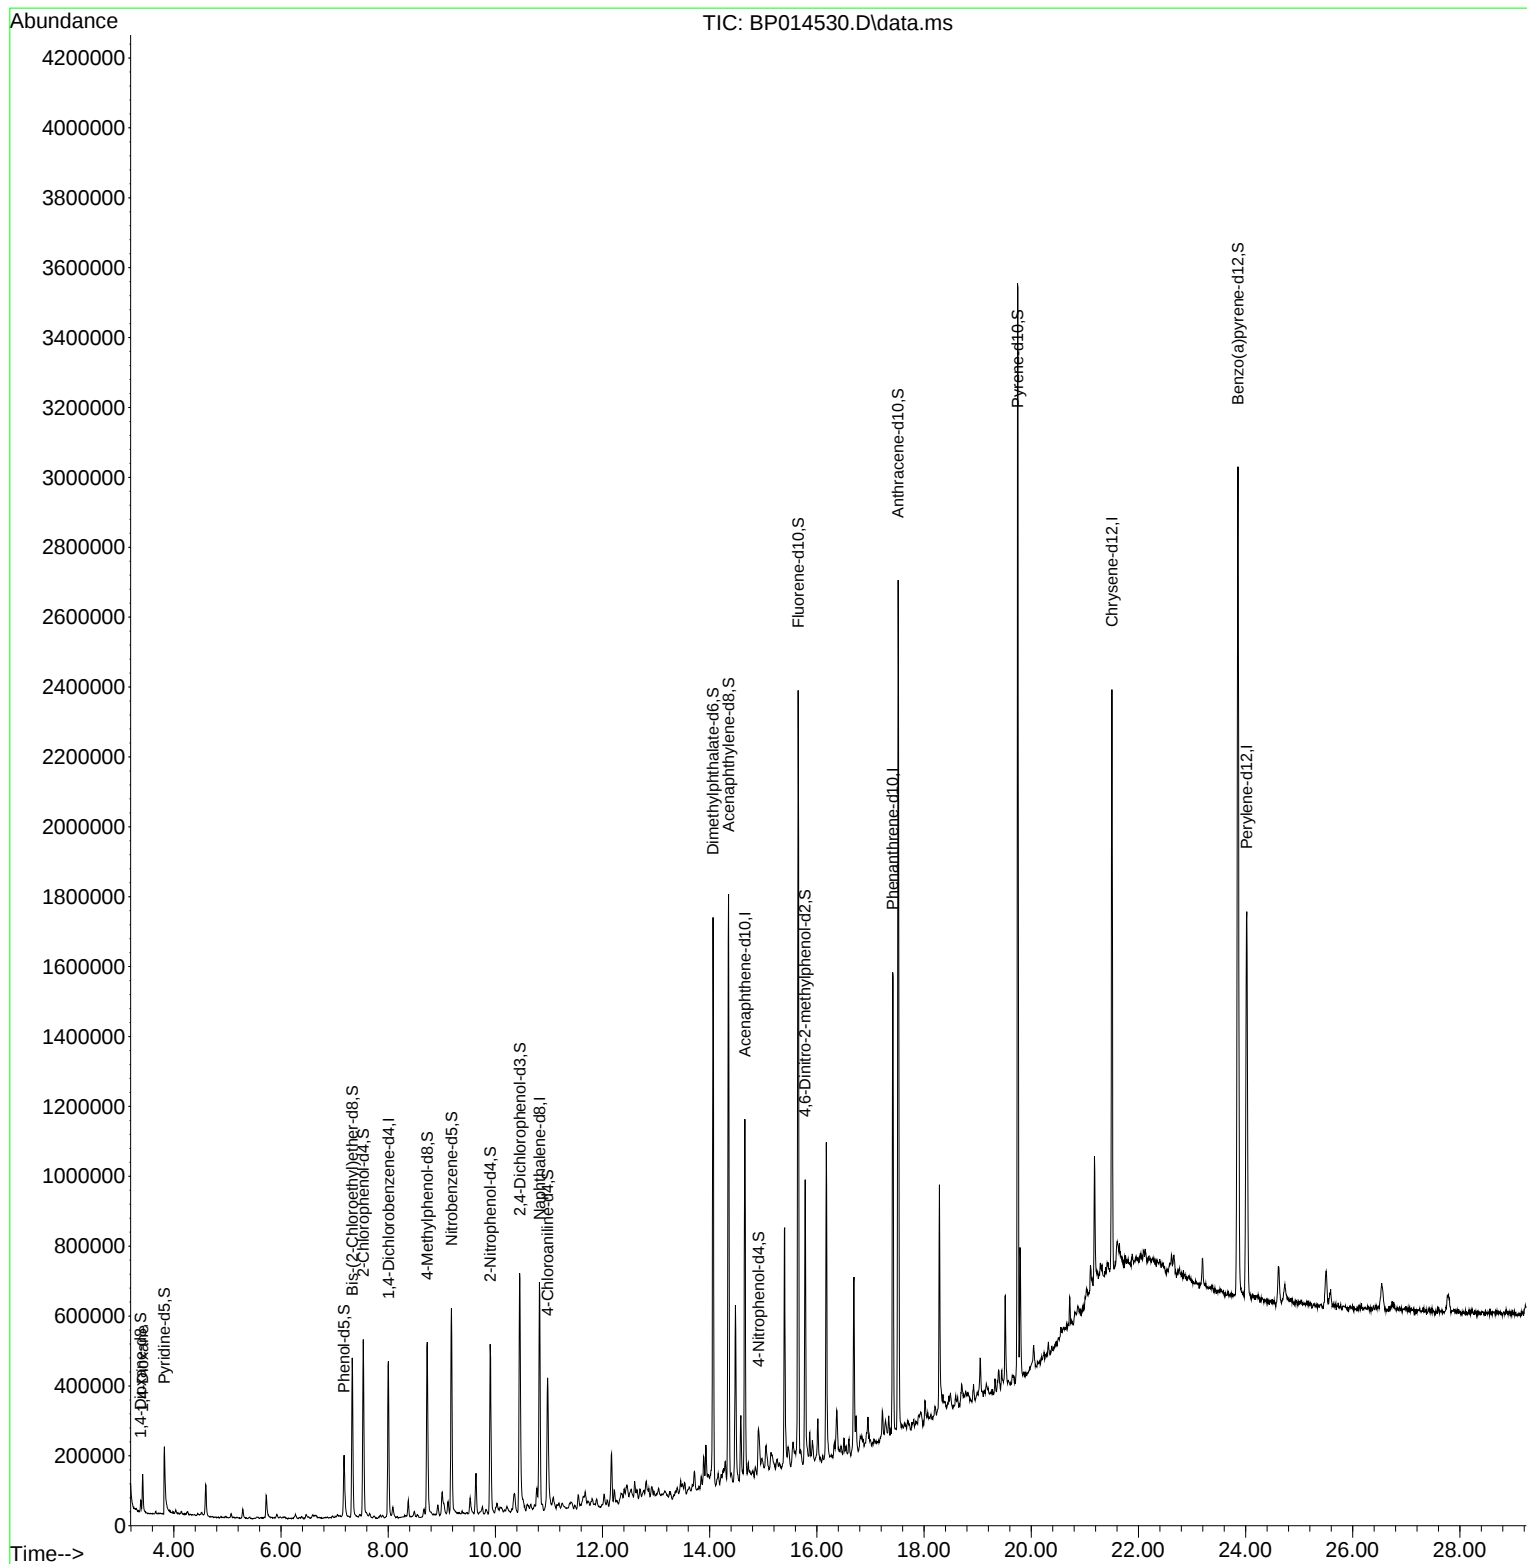

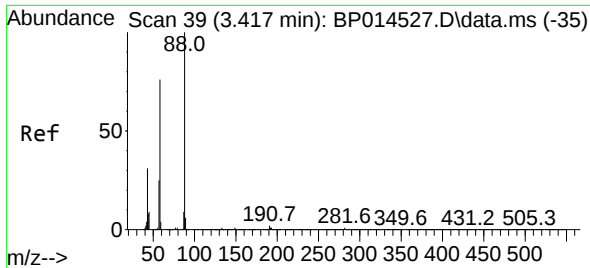

#2
 1,4-Dioxane
 Concen: 16.076 ng/uL
 RT: 3.417 min Scan# 39
 Delta R.T. -0.000 min
 Lab File: BP014530.D
 Acq: 04 Apr 2023 16:19

Instrument :
 BNA_P
 ClientSampleId :
 CB9A0

Tgt Ion:	88	Resp:	51558
Ion	Ratio	Lower	Upper
88	100		
43	30.6	24.4	36.6
58	76.8	57.4	86.0

