

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014482.D
 Acq On : 03 Apr 2023 12:25
 Operator : CG/JU
 Sample : 02093-04DL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB971DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.423	35	40	46	rVB	111780	158116	5.52%	0.889%
2	3.670	78	82	87	rBV2	13370	19727	0.69%	0.111%
3	3.770	97	99	105	rVB6	3513	4638	0.16%	0.026%
4	3.876	114	117	123	rBV5	8842	14750	0.51%	0.083%
5	4.140	158	162	168	rBV2	10993	19465	0.68%	0.109%
6	4.217	171	175	178	rBV	22636	28485	0.99%	0.160%
7	4.599	234	240	249	rVB2	20518	36888	1.29%	0.207%
8	5.075	316	321	325	rVB6	2145	3819	0.13%	0.021%
9	5.346	364	367	371	rBV5	2134	3344	0.12%	0.019%
10	5.552	396	402	404	rBV6	2559	3833	0.13%	0.022%
11	5.987	472	476	478	rBV4	2773	3630	0.13%	0.020%
12	6.270	517	524	531	rVB	4256	8970	0.31%	0.050%
13	6.393	543	545	552	rVB8	2311	4763	0.17%	0.027%
14	6.517	560	566	570	rBV9	4964	7060	0.25%	0.040%
15	6.669	585	592	594	rBV8	2215	5122	0.18%	0.029%
16	6.711	594	599	606	rVV8	13237	21891	0.76%	0.123%
17	7.211	677	684	695	rVB4	10943	32910	1.15%	0.185%
18	7.340	701	706	714	rBV	56924	104570	3.65%	0.588%
19	7.546	735	741	751	rBV	51724	99787	3.48%	0.561%
20	7.846	786	792	798	rBV	2400	5308	0.19%	0.030%
21	8.005	813	819	829	rBV	618578	1039581	36.27%	5.847%
22	8.564	907	914	916	rBV8	2009	3615	0.13%	0.020%
23	8.752	938	946	956	rBV3	31692	85969	3.00%	0.484%
24	9.128	1006	1010	1014	rVB7	3745	5293	0.18%	0.030%
25	9.193	1015	1021	1033	rBV	62117	127413	4.45%	0.717%
26	9.534	1071	1079	1086	rBV	10529	23602	0.82%	0.133%
27	9.640	1092	1097	1101	rVB8	3103	5324	0.19%	0.030%
28	9.734	1109	1113	1114	rBV4	3416	3665	0.13%	0.021%
29	9.822	1125	1128	1130	rBV4	3251	4133	0.14%	0.023%
30	9.916	1138	1144	1158	rBV	50102	105599	3.68%	0.594%
31	10.093	1168	1174	1176	rBV6	1828	3331	0.12%	0.019%
32	10.246	1198	1200	1205	rVB6	2301	3108	0.11%	0.017%
33	10.375	1217	1222	1228	rVB3	18470	32833	1.15%	0.185%
34	10.487	1230	1241	1254	rBV2	48916	157008	5.48%	0.883%
35	10.834	1289	1300	1310	rBV	930936	1638962	57.19%	9.219%
36	10.957	1318	1321	1325	rBV6	5142	7002	0.24%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014482.D
 Acq On : 03 Apr 2023 12:25
 Operator : CG/JU
 Sample : 02093-04DL 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB971DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	11.016	1325	1331	1337	rVB6	7757	16153	0.56%	0.091%
38	11.310	1380	1381	1386	rVB5	3385	3726	0.13%	0.021%
39	11.416	1393	1399	1404	rBV9	5757	11583	0.40%	0.065%
40	11.546	1417	1421	1426	rVB7	2539	4034	0.14%	0.023%
41	11.652	1434	1439	1441	rBV6	3973	5480	0.19%	0.031%
42	11.687	1443	1445	1448	rVV4	3470	3899	0.14%	0.022%
43	11.810	1462	1466	1467	rBV4	4068	3972	0.14%	0.022%
44	11.969	1488	1493	1495	rBV6	2271	3467	0.12%	0.020%
45	12.040	1501	1505	1510	rVB6	9956	16702	0.58%	0.094%
46	12.187	1526	1530	1538	rVB7	7633	16419	0.57%	0.092%
47	12.357	1551	1559	1568	rBV9	12956	35494	1.24%	0.200%
48	12.475	1573	1579	1581	rBV6	6995	13008	0.45%	0.073%
49	12.652	1602	1609	1615	rVB2	26384	47271	1.65%	0.266%
50	12.704	1615	1618	1620	rBV4	2221	3056	0.11%	0.017%
51	12.752	1624	1626	1628	rBV3	3565	3814	0.13%	0.021%
52	12.899	1647	1651	1652	rBV4	3293	3477	0.12%	0.020%
53	13.016	1668	1671	1673	rBV4	2358	3184	0.11%	0.018%
54	13.222	1700	1706	1708	rBV7	7727	11383	0.40%	0.064%
55	13.399	1732	1736	1743	rBV10	5161	12112	0.42%	0.068%
56	13.551	1756	1762	1765	rBV7	6599	13150	0.46%	0.074%
57	13.716	1785	1790	1793	rBV4	8938	15139	0.53%	0.085%
58	13.846	1810	1812	1815	rBV4	2789	3557	0.12%	0.020%
59	13.899	1815	1821	1827	rBV2	20524	42688	1.49%	0.240%
60	14.069	1844	1850	1861	rVB	201534	303895	10.60%	1.709%
61	14.175	1864	1868	1873	rBV2	16587	29486	1.03%	0.166%
62	14.357	1893	1899	1908	rBV	205539	327896	11.44%	1.844%
63	14.469	1915	1918	1925	rVB5	11940	23565	0.82%	0.133%
64	14.587	1933	1938	1943	rBV3	44570	65623	2.29%	0.369%
65	14.663	1945	1951	1959	rVV	1588598	2306259	80.47%	12.972%
66	15.034	2011	2014	2019	rVB4	14258	19473	0.68%	0.110%
67	15.404	2073	2077	2082	rBV2	20384	32932	1.15%	0.185%
68	15.563	2102	2104	2108	rBV5	6230	9594	0.33%	0.054%
69	15.657	2115	2120	2127	rBV	290420	435567	15.20%	2.450%
70	15.793	2139	2143	2152	rVB3	45204	81416	2.84%	0.458%
71	16.028	2179	2183	2188	rBV3	16347	25593	0.89%	0.144%
72	16.181	2204	2209	2222	rVB2	177018	265275	9.26%	1.492%
73	16.357	2236	2239	2243	rBV6	14218	21652	0.76%	0.122%
74	16.698	2292	2297	2308	rVB	98108	167150	5.83%	0.940%
75	17.428	2414	2421	2431	rBV	1968706	2865995	100.00%	16.120%
76	17.528	2433	2438	2447	rVB	314946	473903	16.54%	2.666%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014482.D
Acq On : 03 Apr 2023 12:25
Operator : CG/JU
Sample : 02093-04DL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB971DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

77	17.775	2477	2480	2485	rBV2	20765	29488	1.03%	0.166%
78	18.292	2565	2568	2572	rBV5	28960	36569	1.28%	0.206%
79	19.757	2812	2817	2822	rVB	406671	518706	18.10%	2.918%
80	21.516	3111	3116	3124	rBV	1949058	2713169	94.67%	15.261%
81	23.863	3512	3515	3522	rVB2	305027	548385	19.13%	3.084%
82	24.027	3537	3543	3552	rVB2	1141992	2350990	82.03%	13.224%




Sum of corrected areas: 17778863

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014482.D
Acq On : 03 Apr 2023 12:25
Operator : CG/JU
Sample : 02093-04DL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB971DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

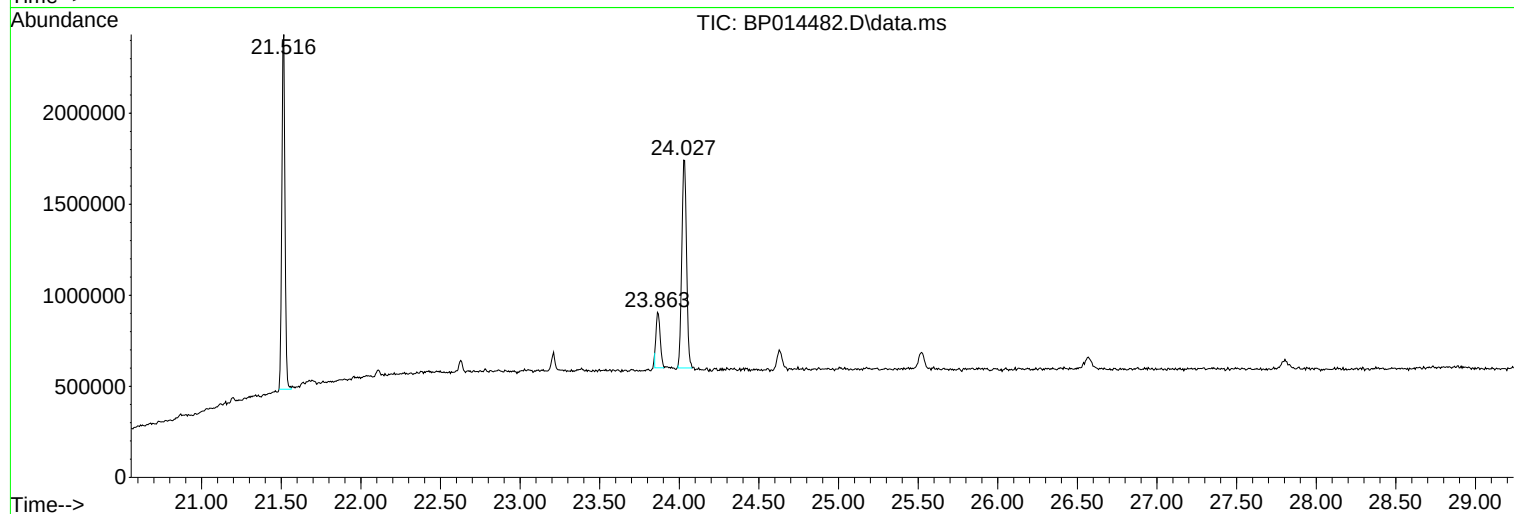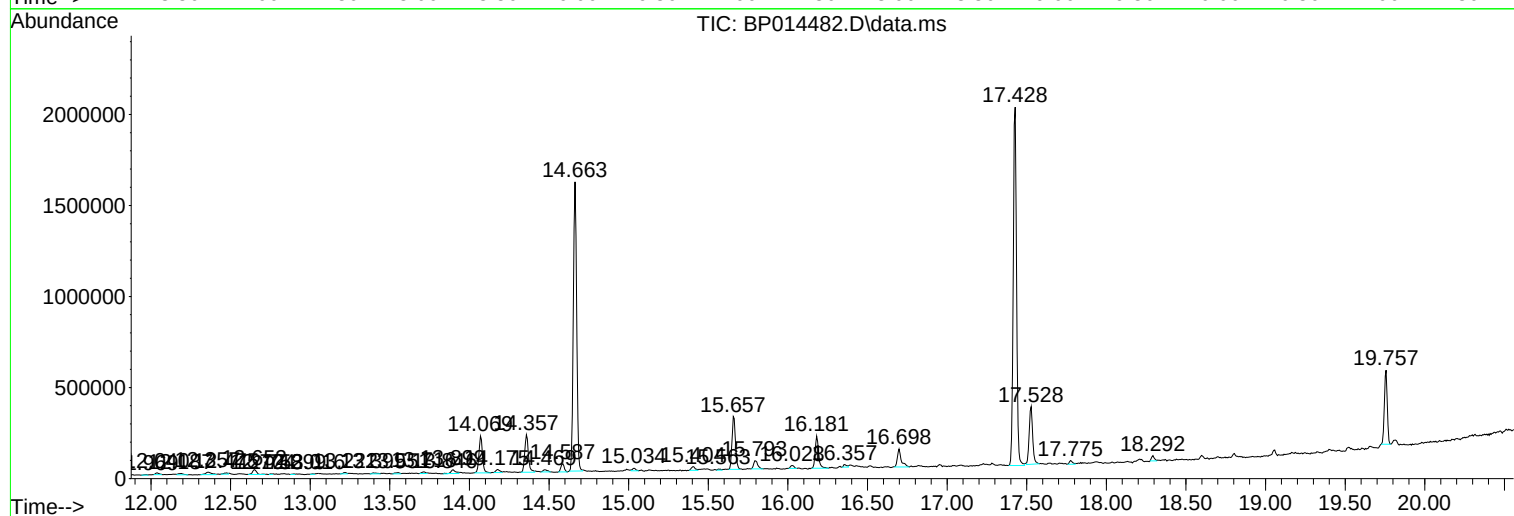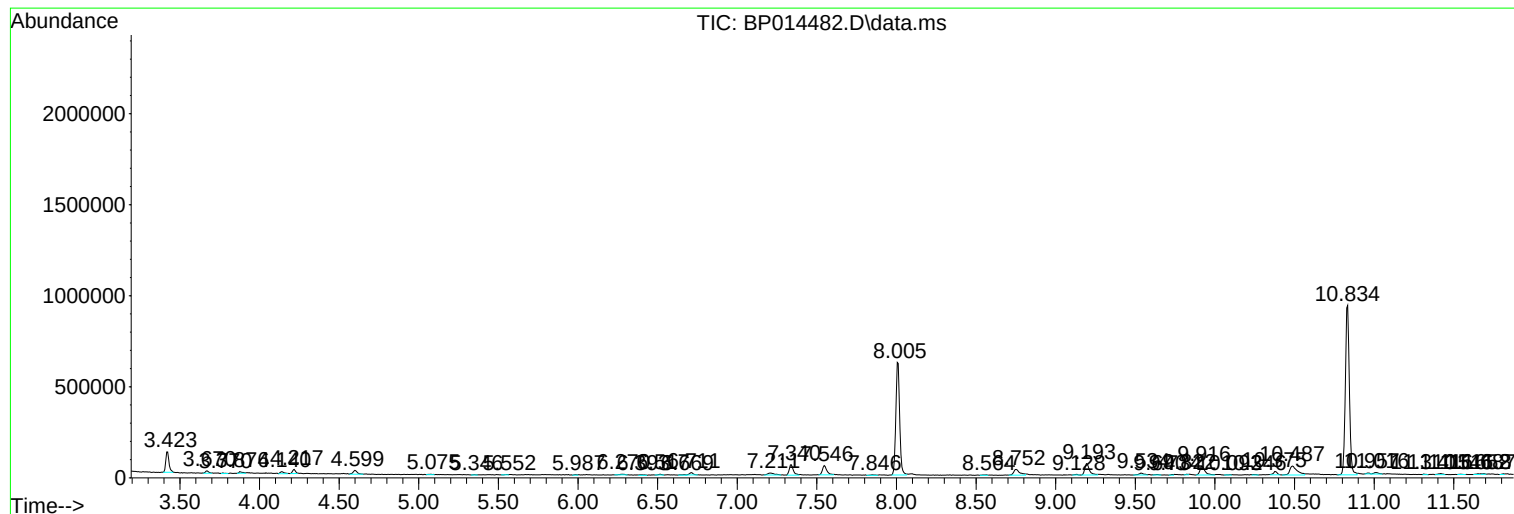

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014482.D
Acq On : 03 Apr 2023 12:25
Operator : CG/JU
Sample : 02093-04DL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB971DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014482.D
Acq On : 03 Apr 2023 12:25
Operator : CG/JU
Sample : 02093-04DL 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB971DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc