

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014484.D
 Acq On : 03 Apr 2023 13:33
 Operator : CG/JU
 Sample : 02093-08DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB978DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014484.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.422	35	40	50	rVB	142040	207964	7.88%	1.180%
2	3.869	114	116	120	rBV3	9289	15362	0.58%	0.087%
3	4.028	140	143	148	rBV6	3081	5650	0.21%	0.032%
4	4.140	158	162	168	rVB3	10947	14246	0.54%	0.081%
5	4.216	170	175	180	rVV	74657	98245	3.72%	0.558%
6	4.257	180	182	186	rVB5	5523	6764	0.26%	0.038%
7	4.599	234	240	248	rBV3	13171	26811	1.02%	0.152%
8	4.975	299	304	306	rBV6	2942	4108	0.16%	0.023%
9	5.069	318	320	323	rBV4	2904	2978	0.11%	0.017%
10	5.263	350	353	356	rBV5	1623	3022	0.11%	0.017%
11	6.275	521	525	529	rBV5	2668	4786	0.18%	0.027%
12	6.387	540	544	551	rVB9	2874	5878	0.22%	0.033%
13	6.840	618	621	622	rBV3	2230	2737	0.10%	0.016%
14	6.963	638	642	646	rBV7	3609	3547	0.13%	0.020%
15	7.104	661	666	670	rBV7	1878	3466	0.13%	0.020%
16	7.204	677	683	697	rVB3	17560	44707	1.69%	0.254%
17	7.334	700	705	715	rBV	62657	109872	4.16%	0.624%
18	7.475	725	729	731	rBV4	3033	4373	0.17%	0.025%
19	7.546	735	741	756	rVV2	57477	121521	4.61%	0.690%
20	7.663	757	761	768	rVB10	2982	6016	0.23%	0.034%
21	8.010	812	820	830	rBV	550779	938690	35.58%	5.327%
22	8.487	899	901	904	rBV4	1940	2986	0.11%	0.017%
23	8.745	939	945	961	rVV3	45317	114634	4.34%	0.651%
24	8.845	961	962	967	rVB5	2462	2639	0.10%	0.015%
25	8.945	972	979	984	rBV10	6346	11555	0.44%	0.066%
26	9.016	984	991	1001	rBV	101984	219608	8.32%	1.246%
27	9.128	1008	1010	1014	rVB5	6349	7293	0.28%	0.041%
28	9.192	1015	1021	1028	rBV	74321	135047	5.12%	0.766%
29	9.322	1041	1043	1046	rVV4	2731	2853	0.11%	0.016%
30	9.375	1048	1052	1058	rVB8	8885	15851	0.60%	0.090%
31	9.534	1075	1079	1086	rVB9	5866	11893	0.45%	0.067%
32	9.640	1092	1097	1108	rBV2	35018	62129	2.35%	0.353%
33	9.740	1108	1114	1122	rVB2	5991	13328	0.51%	0.076%
34	9.834	1125	1130	1135	rBV9	2995	6572	0.25%	0.037%
35	9.916	1138	1144	1155	rBV2	53361	116369	4.41%	0.660%
36	10.040	1158	1165	1171	rVV2	7463	13210	0.50%	0.075%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014484.D
 Acq On : 03 Apr 2023 13:33
 Operator : CG/JU
 Sample : 02093-08DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB978DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	10.098	1171	1175	1180	rVB7	5926	8793	0.33%	0.050%
38	10.234	1194	1198	1200	rBV5	2795	3922	0.15%	0.022%
39	10.310	1209	1211	1214	rBV4	2885	3644	0.14%	0.021%
40	10.375	1214	1222	1232	rVB10	15036	37397	1.42%	0.212%
41	10.487	1232	1241	1256	rBV2	57392	190636	7.23%	1.082%
42	10.604	1258	1261	1265	rVV6	4179	6556	0.25%	0.037%
43	10.745	1282	1285	1286	rBV3	2840	2650	0.10%	0.015%
44	10.834	1292	1300	1311	rBV	853126	1489889	56.47%	8.456%
45	10.963	1318	1322	1323	rBV4	6820	7360	0.28%	0.042%
46	11.004	1325	1329	1339	rVV4	18318	38304	1.45%	0.217%
47	11.092	1339	1344	1350	rVB9	6278	12409	0.47%	0.070%
48	11.187	1358	1360	1364	rVB5	2266	3206	0.12%	0.018%
49	11.257	1367	1372	1373	rBV5	3927	5879	0.22%	0.033%
50	11.281	1373	1376	1379	rVV5	2671	3209	0.12%	0.018%
51	11.439	1398	1403	1408	rVB8	5251	13137	0.50%	0.075%
52	11.504	1408	1414	1416	rBV7	3391	6388	0.24%	0.036%
53	11.639	1432	1437	1438	rBV5	6503	8027	0.30%	0.046%
54	11.669	1439	1442	1443	rVV3	3135	2977	0.11%	0.017%
55	11.734	1452	1453	1457	rBV4	2691	3431	0.13%	0.019%
56	11.810	1463	1466	1472	rVB8	5520	8468	0.32%	0.048%
57	11.869	1472	1476	1479	rBV6	3836	6071	0.23%	0.034%
58	12.045	1499	1506	1511	rVB10	5201	12563	0.48%	0.071%
59	12.181	1526	1529	1532	rBV5	4862	6016	0.23%	0.034%
60	12.357	1554	1559	1564	rBV2	26208	54568	2.07%	0.310%
61	12.463	1571	1577	1585	rVV9	8931	22014	0.83%	0.125%
62	12.545	1589	1591	1600	rVB9	6172	10366	0.39%	0.059%
63	12.704	1615	1618	1624	rBV7	4528	7509	0.28%	0.043%
64	12.745	1624	1625	1629	rVB4	3746	3555	0.13%	0.020%
65	12.828	1632	1639	1651	rVV8	13767	34908	1.32%	0.198%
66	13.045	1673	1676	1682	rVB6	9720	14461	0.55%	0.082%
67	13.222	1702	1706	1709	rVB5	3257	4451	0.17%	0.025%
68	13.404	1733	1737	1742	rVB8	4162	7395	0.28%	0.042%
69	13.445	1742	1744	1745	rBV2	4417	3765	0.14%	0.021%
70	13.463	1745	1747	1749	rVV3	3880	3552	0.13%	0.020%
71	13.545	1756	1761	1766	rBV3	18597	31303	1.19%	0.178%
72	13.716	1785	1790	1798	rVB3	7245	16942	0.64%	0.096%
73	14.069	1841	1850	1859	rBV	235923	366710	13.90%	2.081%
74	14.239	1877	1879	1880	rBV2	3931	3108	0.12%	0.018%
75	14.357	1893	1899	1908	rBV2	248236	379533	14.38%	2.154%
76	14.469	1914	1918	1928	rBV	22643	47690	1.81%	0.271%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014484.D
 Acq On : 03 Apr 2023 13:33
 Operator : CG/JU
 Sample : 02093-08DL 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB978DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

77	14.586	1933	1938	1943	rBV4	32704	46774	1.77%	0.265%
78	14.663	1944	1951	1960	rBV	1432689	2121241	80.40%	12.039%
79	14.980	2001	2005	2010	rBV8	7633	16961	0.64%	0.096%
80	15.410	2076	2078	2080	rBV3	5267	5336	0.20%	0.030%
81	15.657	2115	2120	2133	rVB	342284	505737	19.17%	2.870%
82	15.798	2139	2144	2156	rBV4	45171	94092	3.57%	0.534%
83	16.027	2179	2183	2188	rBV	34150	46542	1.76%	0.264%
84	16.186	2205	2210	2218	rVB	60444	95544	3.62%	0.542%
85	16.357	2236	2239	2245	rVB7	12198	19326	0.73%	0.110%
86	16.698	2293	2297	2301	rBV2	30159	47381	1.80%	0.269%
87	17.427	2414	2421	2431	rBV	1762250	2638449	100.00%	14.974%
88	17.527	2432	2438	2448	rVV	358715	558564	21.17%	3.170%
89	18.292	2564	2568	2574	rBV2	49450	76602	2.90%	0.435%
90	19.051	2695	2697	2701	rVB3	31780	31765	1.20%	0.180%
91	19.521	2774	2777	2781	rBV5	27832	36316	1.38%	0.206%
92	19.757	2812	2817	2822	rVB	469730	637510	24.16%	3.618%
93	21.515	3111	3116	3123	rBV	1851018	2517265	95.41%	14.286%
94	23.868	3511	3516	3524	rVB	314745	627439	23.78%	3.561%
95	24.033	3537	3544	3554	rVB2	1053743	2237784	84.81%	12.700%




Sum of corrected areas: 17620100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014484.D
Acq On : 03 Apr 2023 13:33
Operator : CG/JU
Sample : 02093-08DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB978DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

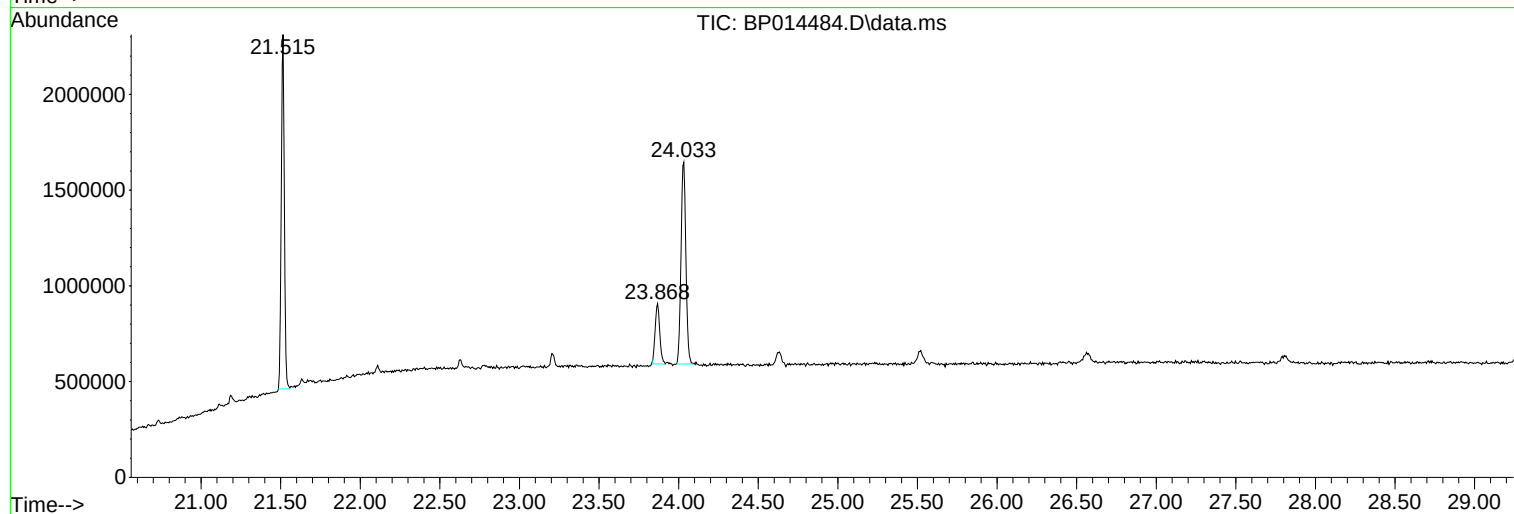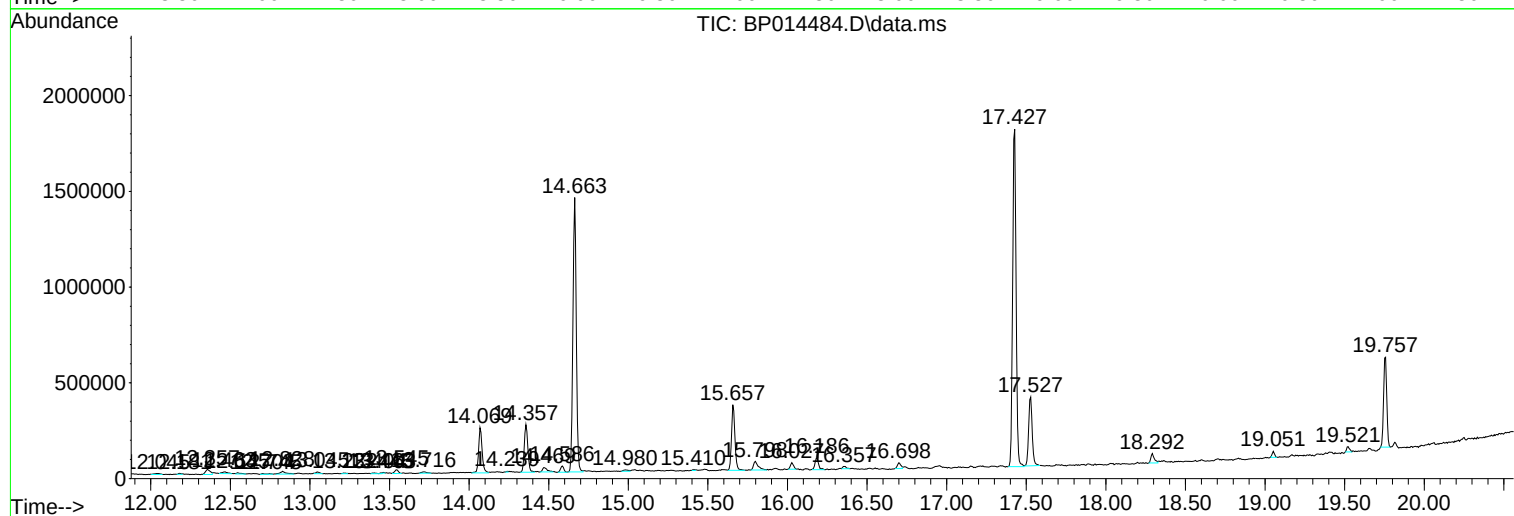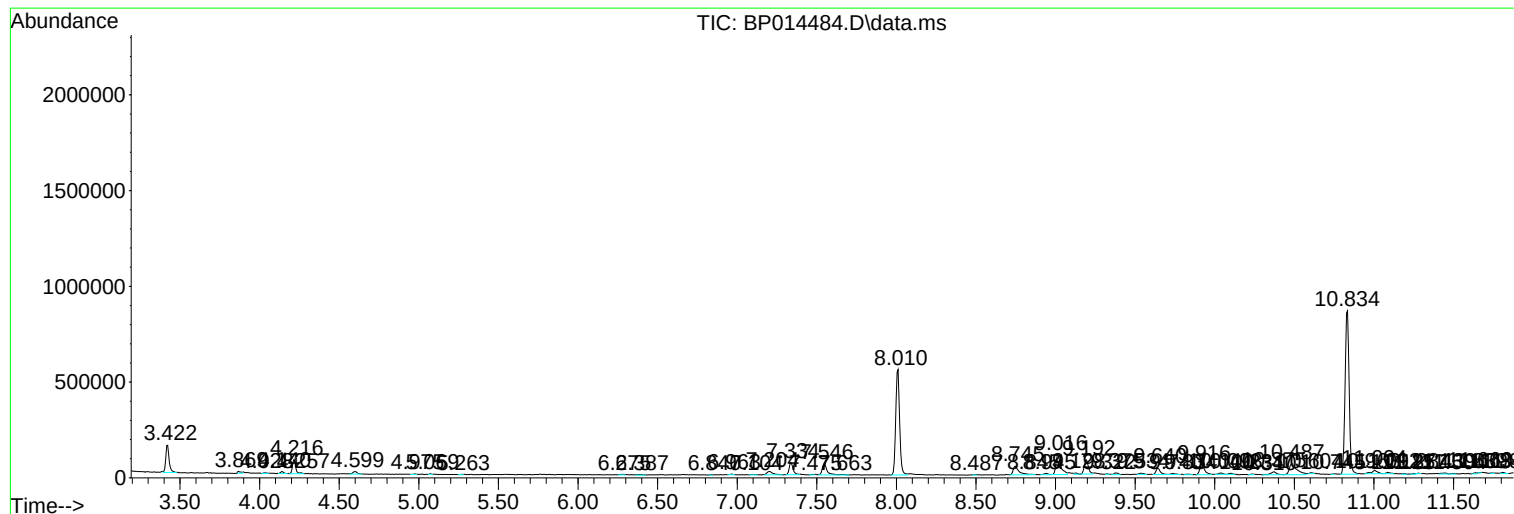

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014484.D
Acq On : 03 Apr 2023 13:33
Operator : CG/JU
Sample : 02093-08DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB978DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Paraldehyde Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.216	2.09 ng/ul	98245	1,4-Dichlorobenzene-d4	8.010

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Paraldehyde			132	C6H12O3	000123-63-7	83
2	Paraldehyde			132	C6H12O3	000123-63-7	83
3	Paraldehyde			132	C6H12O3	000123-63-7	78
4	Paraldehyde			132	C6H12O3	000123-63-7	56
5	Ethanol, 2-[2-(2-butoxyethoxy)et...			206	C10H22O4	000143-22-6	40

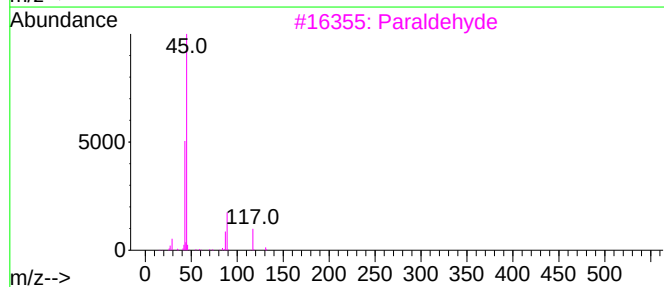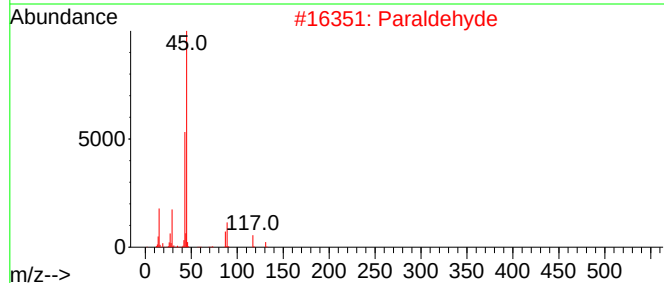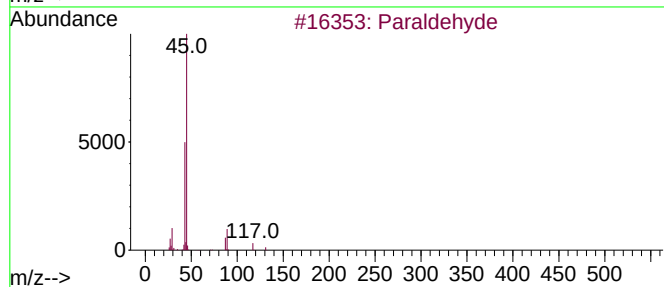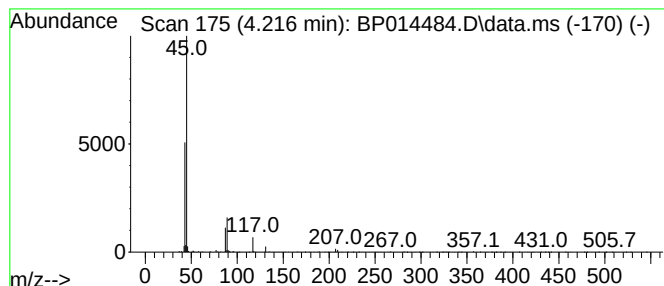

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014484.D
Acq On : 03 Apr 2023 13:33
Operator : CG/JU
Sample : 02093-08DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB978DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzenamine, 3-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.016	4.68 ng/ul	219608	1,4-Dichlorobenzene-d4	8.010

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzenamine, 3-methyl-	107	C7H9N	000108-44-1	97
2			Benzenamine, 3-methyl-	107	C7H9N	000108-44-1	96
3			Benzenamine, 3-methyl-	107	C7H9N	000108-44-1	96
4			Benzenamine, 3-methyl-	107	C7H9N	000108-44-1	95
5			o-Toluidine	107	C7H9N	000095-53-4	94

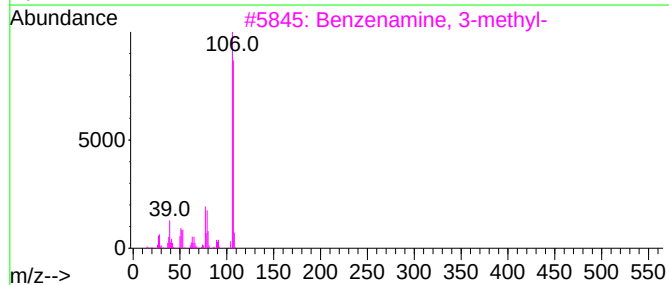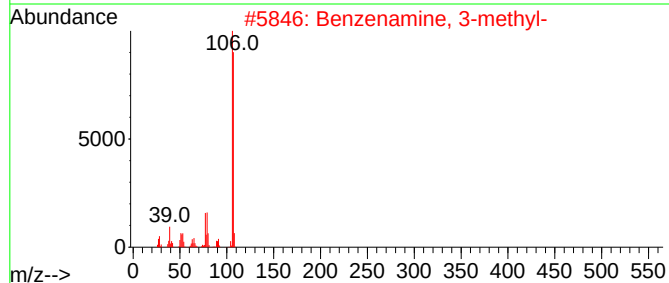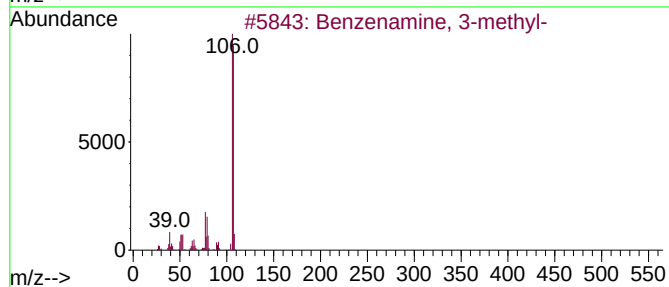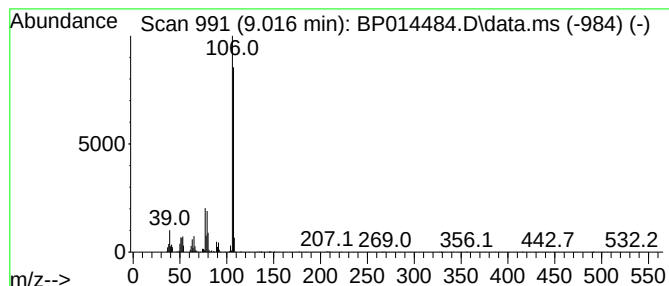

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014484.D
Acq On : 03 Apr 2023 13:33
Operator : CG/JU
Sample : 02093-08DL 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB978DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Paraldehyde	4.216	2.1	ng/ul	98245	1	8.010	938690	20.0
Benzenamine, 3-...	9.016	4.7	ng/ul	219608	1	8.010	938690	20.0