

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014488.D
 Acq On : 03 Apr 2023 15:49
 Operator : CG/JU
 Sample : PB151780BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK780

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	29	34	39	rBV	23207	34112	0.93%	0.099%
2	3.828	107	109	127	rBV	103174	218080	5.98%	0.630%
3	4.140	157	162	165	rBV3	9338	13787	0.38%	0.040%
4	4.940	296	298	302	rVB5	2654	3714	0.10%	0.011%
5	7.181	671	679	694	rBV	396601	749287	20.54%	2.165%
6	7.334	698	705	717	rVV	331725	544698	14.93%	1.574%
7	7.540	733	740	753	rBV	425753	721423	19.77%	2.085%
8	8.004	813	819	830	rBV	448738	753499	20.65%	2.178%
9	8.734	935	943	961	rBV	507748	940622	25.78%	2.718%
10	9.187	1011	1020	1037	rBV	434335	757448	20.76%	2.189%
11	9.910	1134	1143	1159	rBV	357831	660622	18.11%	1.909%
12	10.463	1230	1237	1260	rBV	362780	952950	26.12%	2.754%
13	10.834	1292	1300	1309	rBV	675367	1173079	32.15%	3.390%
14	11.016	1324	1331	1344	rBV5	14567	49277	1.35%	0.142%
15	12.440	1564	1573	1582	rBV5	7576	19625	0.54%	0.057%
16	13.545	1758	1761	1768	rVB8	5379	8392	0.23%	0.024%
17	14.069	1841	1850	1865	rBV	1074841	1577708	43.24%	4.559%
18	14.357	1890	1899	1916	rBV	1242668	1792262	49.12%	5.179%
19	14.663	1944	1951	1964	rBV	1161761	1727030	47.33%	4.991%
20	14.910	1986	1993	2010	rBV2	207469	667977	18.31%	1.930%
21	15.657	2114	2120	2133	rBV	1596174	2334019	63.97%	6.745%
22	15.786	2136	2142	2158	rVV	495580	793299	21.74%	2.293%
23	15.904	2159	2162	2166	rVB6	8308	12975	0.36%	0.037%
24	17.104	2363	2366	2369	rVB5	4029	4014	0.11%	0.012%
25	17.222	2381	2386	2390	rBV7	5080	9072	0.25%	0.026%
26	17.422	2412	2420	2428	rBV	1619930	2334608	63.98%	6.747%
27	17.528	2431	2438	2450	rVV	1805281	2746084	75.26%	7.936%
28	18.439	2591	2593	2596	rBV4	4707	5066	0.14%	0.015%
29	19.333	2742	2745	2749	rBV3	25338	31458	0.86%	0.091%
30	19.751	2811	2816	2826	rBV	2533161	3528472	96.70%	10.197%
31	21.516	3110	3116	3124	rBV	2020299	2968394	81.35%	8.578%
32	23.862	3509	3515	3526	rVB2	1782074	3648820	100.00%	10.545%
33	24.033	3537	3544	3555	rVB2	1308975	2821231	77.32%	8.153%




Sum of corrected areas: 34603104

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014488.D
Acq On : 03 Apr 2023 15:49
Operator : CG/JU
Sample : PB151780BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

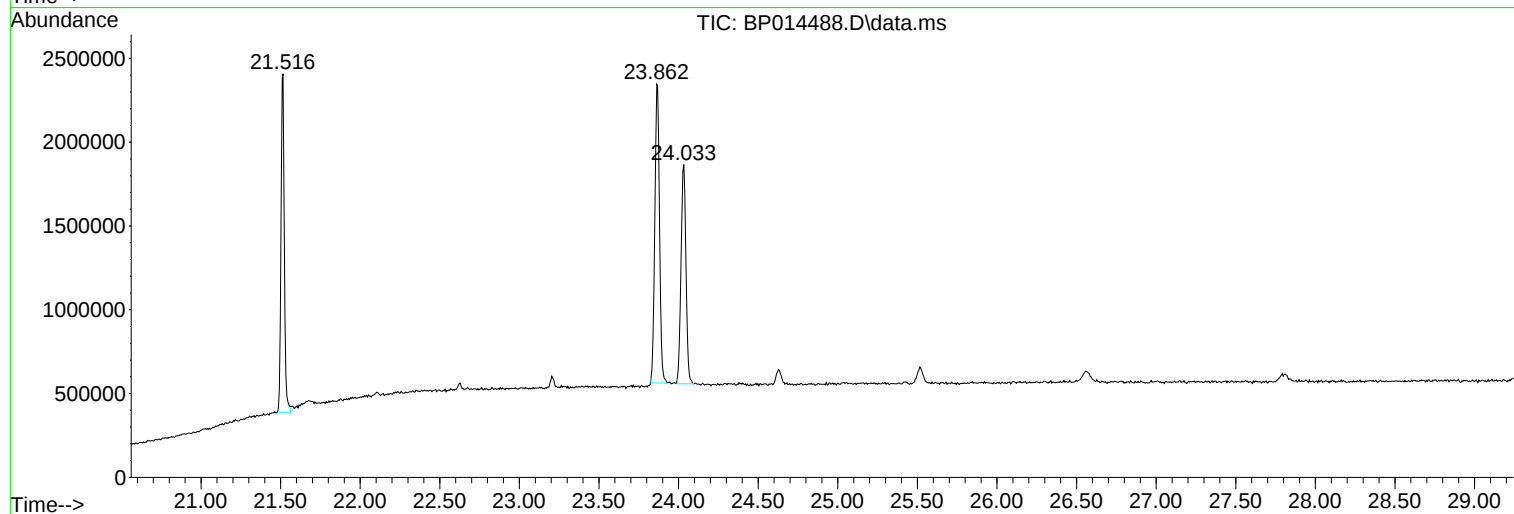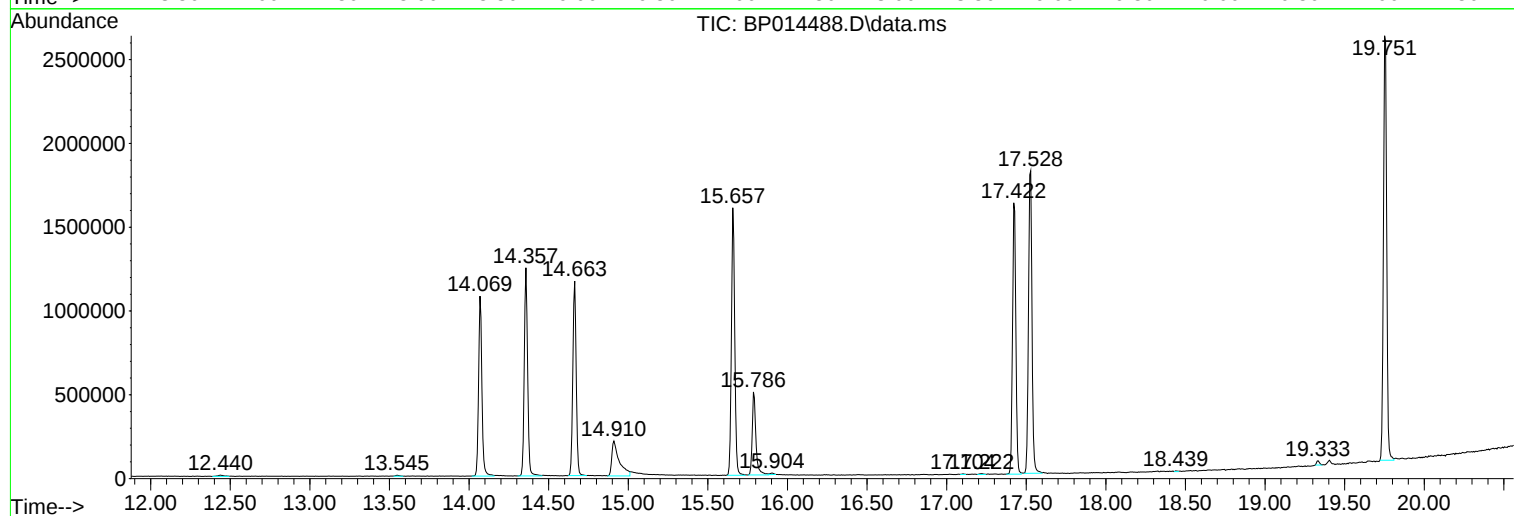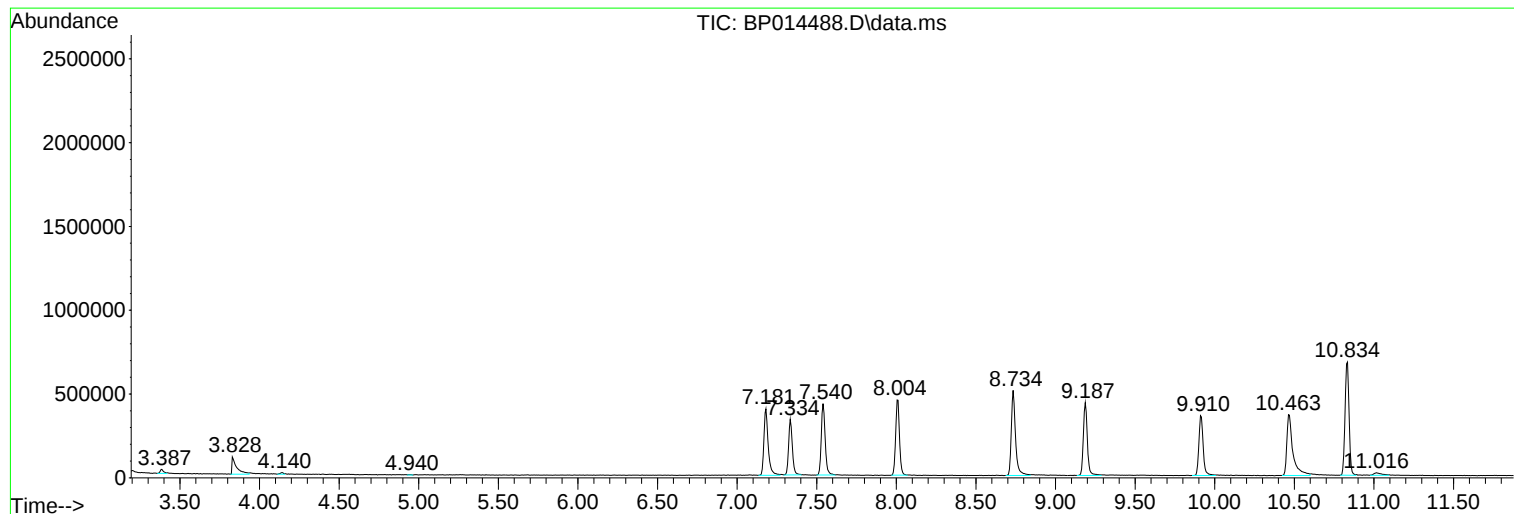

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014488.D
Acq On : 03 Apr 2023 15:49
Operator : CG/JU
Sample : PB151780BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014488.D
Acq On : 03 Apr 2023 15:49
Operator : CG/JU
Sample : PB151780BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK780

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc