

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014492.D
 Acq On : 03 Apr 2023 18:05
 Operator : CG/JU
 Sample : PB151858BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK858

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.387	29	34	46	rVB	31843	56543	1.51%	0.151%
2	3.728	88	92	95	rVB5	2874	4368	0.12%	0.012%
3	3.816	105	107	130	rBV	366208	687119	18.29%	1.841%
4	4.140	159	162	167	rVB3	7528	9928	0.26%	0.027%
5	7.175	670	678	694	rBV	487512	922006	24.55%	2.470%
6	7.334	699	705	719	rVB	424206	678029	18.05%	1.816%
7	7.540	732	740	753	rBV	547148	908997	24.20%	2.435%
8	8.004	813	819	831	rBV	438870	742463	19.77%	1.989%
9	8.734	934	943	959	rBV	626929	1159295	30.86%	3.105%
10	9.187	1011	1020	1034	rBV	540780	945007	25.16%	2.531%
11	9.910	1133	1143	1157	rBV	473281	836163	22.26%	2.240%
12	10.457	1229	1236	1256	rBV	531966	1181283	31.45%	3.164%
13	10.828	1291	1299	1316	rVB	659954	1154583	30.74%	3.093%
14	10.981	1316	1325	1356	rBV	555560	1224756	32.60%	3.281%
15	12.439	1567	1573	1577	rBV4	6974	13801	0.37%	0.037%
16	14.069	1843	1850	1867	rBV	1294838	1898895	50.55%	5.087%
17	14.357	1891	1899	1916	rBV	1500912	2185970	58.19%	5.856%
18	14.663	1944	1951	1964	rBV	1083220	1645957	43.82%	4.409%
19	14.904	1986	1992	2018	rBV	227562	774384	20.62%	2.074%
20	15.657	2113	2120	2130	rBV	1934736	2767384	73.67%	7.413%
21	15.786	2136	2142	2157	rBV	541327	850622	22.64%	2.279%
22	15.904	2157	2162	2169	rVB7	10812	22832	0.61%	0.061%
23	17.098	2362	2365	2369	rBV6	3598	5368	0.14%	0.014%
24	17.422	2414	2420	2431	rBV	1441834	2124798	56.57%	5.692%
25	17.522	2431	2437	2448	rBV2	2116506	3129890	83.32%	8.384%
26	19.333	2741	2745	2749	rBV3	31779	39900	1.06%	0.107%
27	19.404	2753	2757	2763	rBV2	22309	45311	1.21%	0.121%
28	19.751	2811	2816	2827	rBV	2713428	3756370	100.00%	10.062%
29	21.510	3110	3115	3126	rBV	1502103	2304337	61.34%	6.173%
30	23.862	3508	3515	3527	rBV2	1541327	3246502	86.43%	8.696%
31	24.027	3537	3543	3557	rVB2	900552	2008975	53.48%	5.381%




Sum of corrected areas: 37331836

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014492.D
Acq On : 03 Apr 2023 18:05
Operator : CG/JU
Sample : PB151858BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK858

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

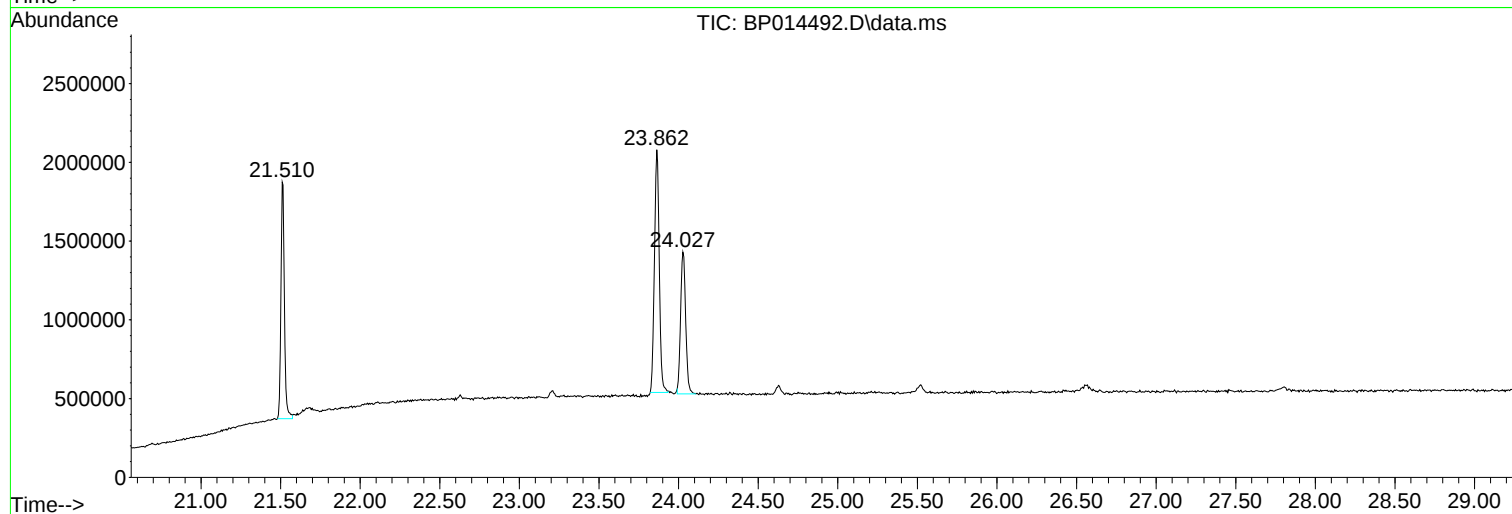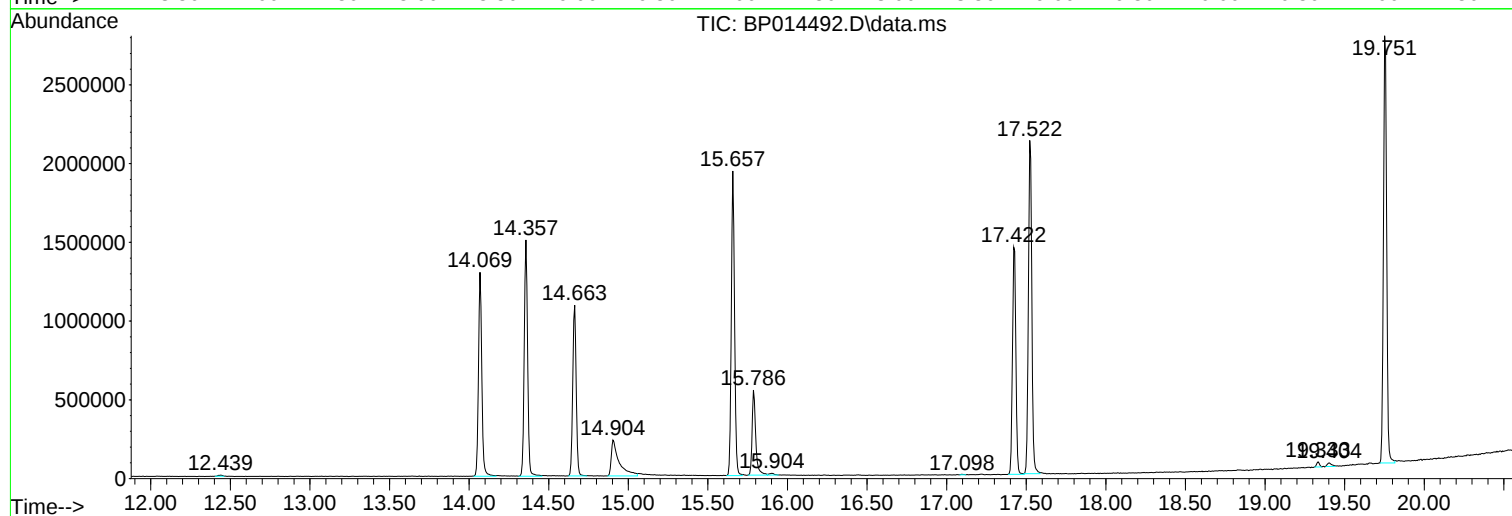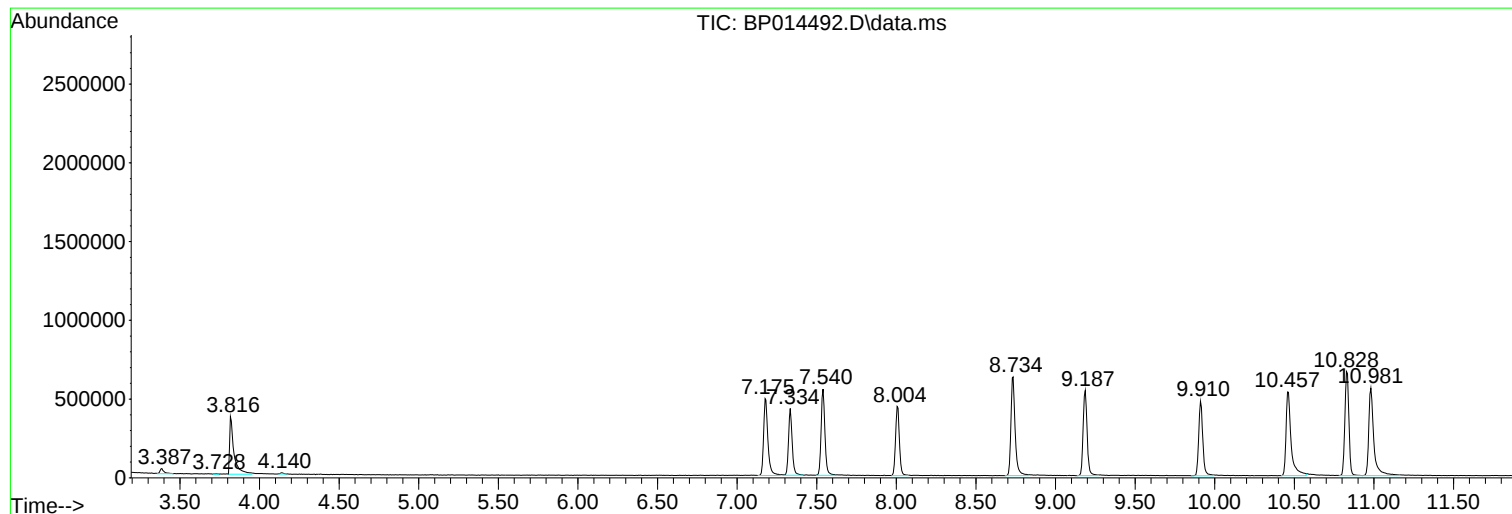

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014492.D
Acq On : 03 Apr 2023 18:05
Operator : CG/JU
Sample : PB151858BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK858

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014492.D
Acq On : 03 Apr 2023 18:05
Operator : CG/JU
Sample : PB151858BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK858

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc