

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014511.D
 Acq On : 04 Apr 2023 05:20
 Operator : CG/JU
 Sample : PB151859BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK859

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014511.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	30	33	40	rVB	44512	54807	1.65%	0.168%
2	3.811	104	106	129	rBV	436936	754686	22.67%	2.320%
3	4.134	156	161	167	rBV2	9414	14814	0.44%	0.046%
4	7.175	671	678	692	rBV	551561	1028741	30.90%	3.163%
5	7.328	698	704	715	rBV	491255	776558	23.32%	2.387%
6	7.534	732	739	758	rBV	633195	1046754	31.44%	3.218%
7	8.005	811	819	833	rBV	473917	783031	23.52%	2.407%
8	8.458	894	896	903	rVB8	1763	3374	0.10%	0.010%
9	8.728	934	942	957	rBV	662866	1231019	36.97%	3.784%
10	9.181	1012	1019	1036	rVV	595569	1016779	30.54%	3.126%
11	9.905	1135	1142	1159	rBV	495515	877940	26.37%	2.699%
12	10.457	1229	1236	1262	rBV	518674	1200836	36.07%	3.692%
13	10.822	1290	1298	1311	rBV	625996	1066723	32.04%	3.279%
14	10.975	1317	1324	1349	rBV	518796	1156299	34.73%	3.555%
15	12.422	1563	1570	1579	rVB9	8515	21370	0.64%	0.066%
16	13.540	1758	1760	1765	rVB6	2828	4380	0.13%	0.013%
17	14.063	1838	1849	1864	rBV	1035644	1570381	47.17%	4.828%
18	14.351	1891	1898	1913	rBV2	1278731	1890803	56.79%	5.813%
19	14.657	1942	1950	1964	rBV	863224	1289331	38.73%	3.964%
20	14.910	1986	1993	2017	rBV	170048	628331	18.87%	1.932%
21	15.587	2104	2108	2112	rBV7	3433	5539	0.17%	0.017%
22	15.651	2112	2119	2133	rBV	1443578	2275927	68.36%	6.997%
23	15.787	2136	2142	2158	rVV	410535	676896	20.33%	2.081%
24	15.892	2158	2160	2167	rVB8	10447	16569	0.50%	0.051%
25	16.716	2297	2300	2302	rBV4	3029	3922	0.12%	0.012%
26	16.845	2318	2322	2328	rVB9	3442	7000	0.21%	0.022%
27	17.028	2352	2353	2356	rBV3	3572	3391	0.10%	0.010%
28	17.092	2361	2364	2368	rBV5	5272	7519	0.23%	0.023%
29	17.422	2413	2420	2430	rBV	945199	1395336	41.91%	4.290%
30	17.522	2430	2437	2448	rBV	1585078	2321964	69.74%	7.138%
31	19.328	2741	2744	2748	rVB4	21781	26932	0.81%	0.083%
32	19.751	2810	2816	2827	rBV	1975454	2766032	83.08%	8.503%
33	21.510	3110	3115	3124	rBV	1097771	1570932	47.18%	4.829%
34	23.857	3507	3514	3528	rVB2	1592283	3329435	100.00%	10.235%
35	24.021	3536	3542	3552	rVB	812903	1703961	51.18%	5.238%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014511.D
Acq On : 04 Apr 2023 05:20
Operator : CG/JU
Sample : PB151859BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK859

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION




Sum of corrected areas: 32528312

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014511.D
Acq On : 04 Apr 2023 05:20
Operator : CG/JU
Sample : PB151859BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK859

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

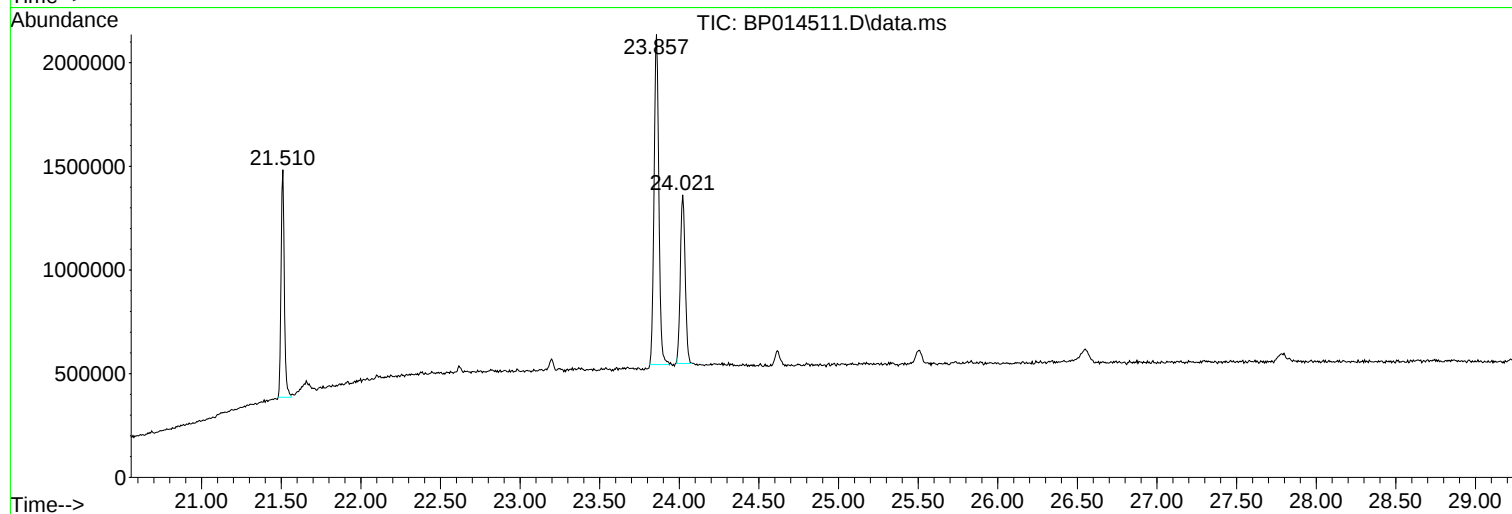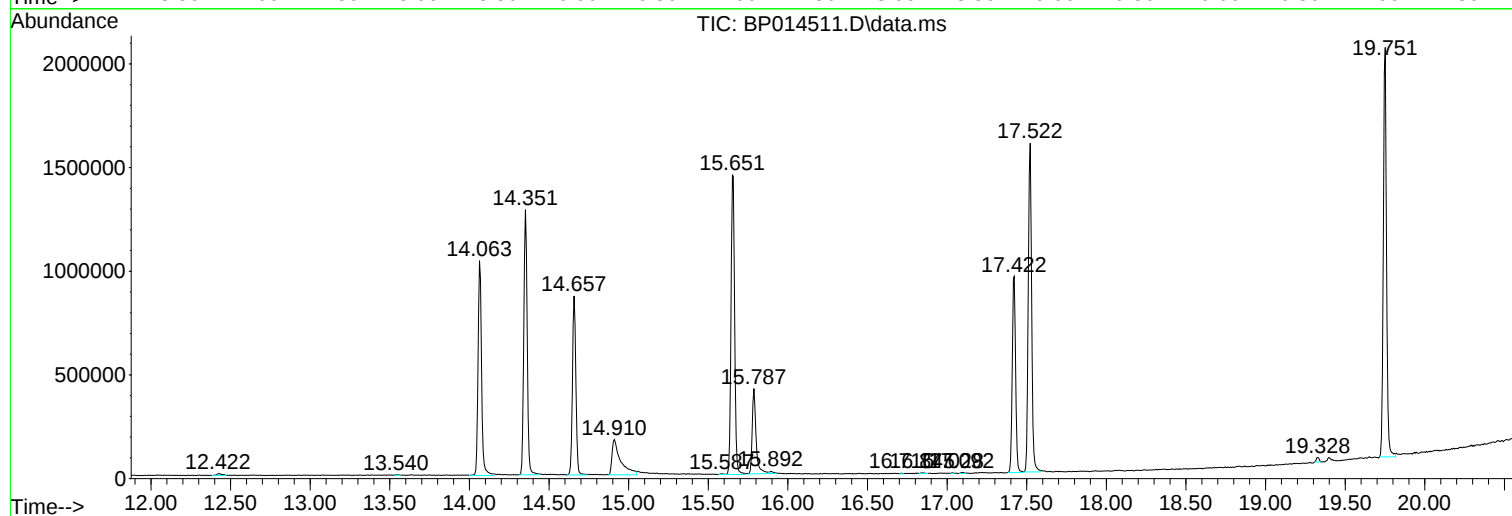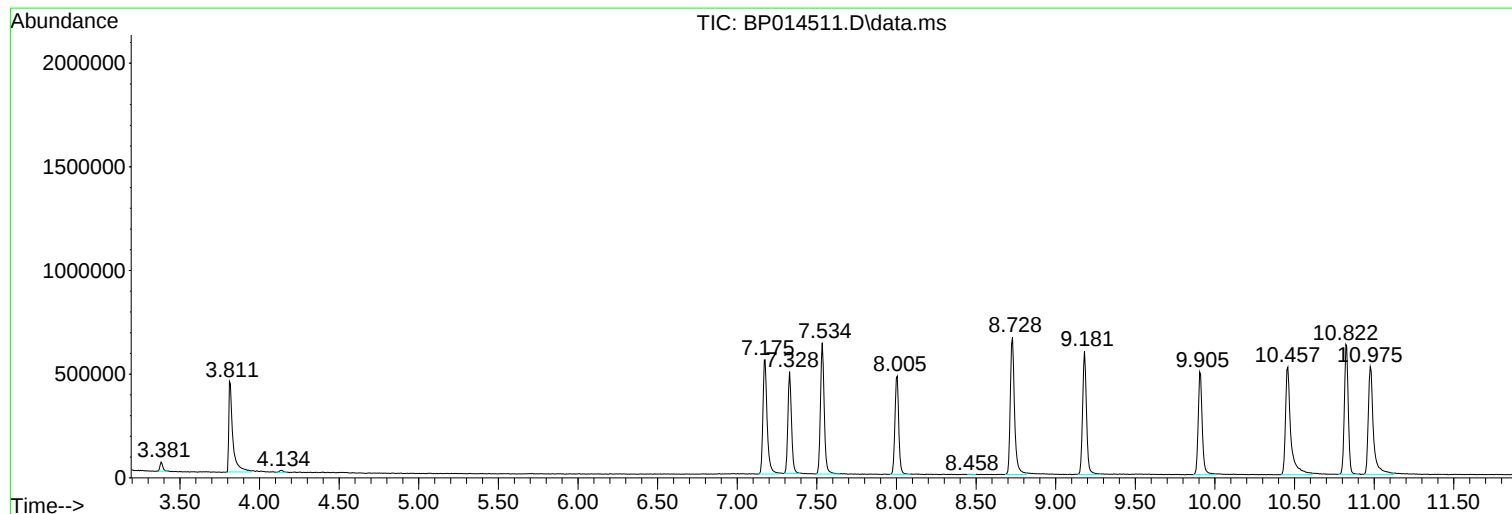

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014511.D
Acq On : 04 Apr 2023 05:20
Operator : CG/JU
Sample : PB151859BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK859

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014511.D
Acq On : 04 Apr 2023 05:20
Operator : CG/JU
Sample : PB151859BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK859

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc