

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014512.D
 Acq On : 04 Apr 2023 05:54
 Operator : CG/JU
 Sample : PB151804BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK804

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	29	33	42	rVB	41114	55282	1.69%	0.175%
2	3.817	104	107	127	rBV	386067	664198	20.25%	2.101%
3	4.134	158	161	166	rVB2	10535	15179	0.46%	0.048%
4	4.846	278	282	284	rBV4	2485	4530	0.14%	0.014%
5	5.605	408	411	416	rBV6	2893	6030	0.18%	0.019%
6	5.911	461	463	470	rVB8	2650	3679	0.11%	0.012%
7	7.093	662	664	668	rBV5	2973	4058	0.12%	0.013%
8	7.175	671	678	693	rBV	481295	882028	26.90%	2.791%
9	7.328	698	704	718	rVB	420338	672608	20.51%	2.128%
10	7.534	731	739	749	rBV	554169	912604	27.83%	2.887%
11	7.999	811	818	832	rBV	491242	826064	25.19%	2.613%
12	8.546	906	911	913	rBV5	2192	3644	0.11%	0.012%
13	8.728	935	942	957	rBV	575329	1055174	32.18%	3.338%
14	9.181	1012	1019	1030	rBV	500390	857609	26.15%	2.713%
15	9.910	1135	1143	1155	rBV	404525	739726	22.56%	2.340%
16	10.457	1230	1236	1258	rVV	450418	1023896	31.22%	3.239%
17	10.828	1290	1299	1311	rBV	647626	1119310	34.13%	3.541%
18	10.975	1316	1324	1347	rBV	428879	962456	29.35%	3.045%
19	12.428	1565	1571	1573	rBV6	6945	10077	0.31%	0.032%
20	14.063	1839	1849	1864	rBV	948905	1443615	44.02%	4.567%
21	14.351	1889	1898	1910	rBV	1106995	1687485	51.46%	5.339%
22	14.657	1941	1950	1959	rBV	925273	1387050	42.30%	4.388%
23	14.910	1987	1993	2014	rBV	159270	583309	17.79%	1.845%
24	15.222	2044	2046	2054	rVB9	3698	4881	0.15%	0.015%
25	15.598	2107	2110	2113	rBV5	2580	3902	0.12%	0.012%
26	15.651	2113	2119	2131	rVV	1325555	2066608	63.02%	6.538%
27	15.787	2136	2142	2158	rVV	393885	646077	19.70%	2.044%
28	15.892	2158	2160	2169	rVB6	10873	22396	0.68%	0.071%
29	16.716	2299	2300	2305	rVB5	2657	3591	0.11%	0.011%
30	17.422	2413	2420	2430	rBV	1090557	1625288	49.56%	5.142%
31	17.522	2430	2437	2457	rVB	1533901	2273968	69.34%	7.194%
32	19.328	2741	2744	2750	rBV4	19325	26491	0.81%	0.084%
33	19.404	2753	2757	2759	rBV3	15521	22536	0.69%	0.071%
34	19.751	2810	2816	2828	rBV	1927356	2741390	83.60%	8.673%
35	21.510	3110	3115	3124	rBV	1283961	1898835	57.90%	6.007%
36	23.857	3507	3514	3527	rVB	1644327	3279322	100.00%	10.375%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014512.D
Acq On : 04 Apr 2023 05:54
Operator : CG/JU
Sample : PB151804BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK804

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	24.021	3536	3542	3553	rVB2	969579	2073199	63.22%	6.559%
----	--------	------	------	------	------	--------	---------	--------	--------




Sum of corrected areas: 31608095

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014512.D
Acq On : 04 Apr 2023 05:54
Operator : CG/JU
Sample : PB151804BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK804

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

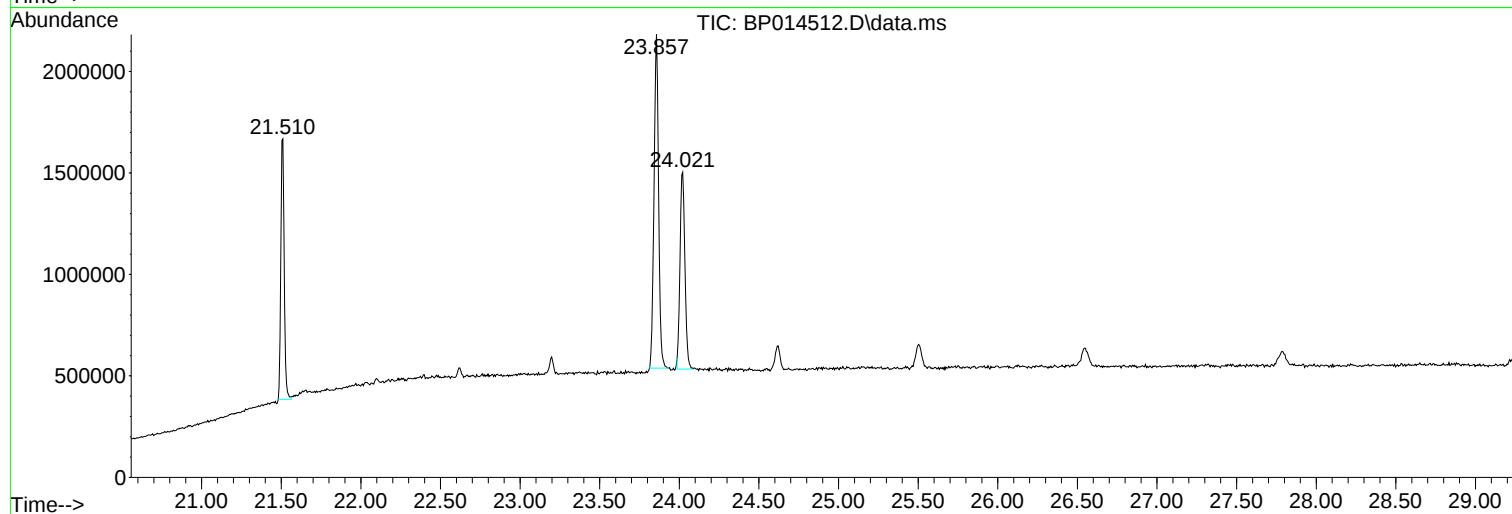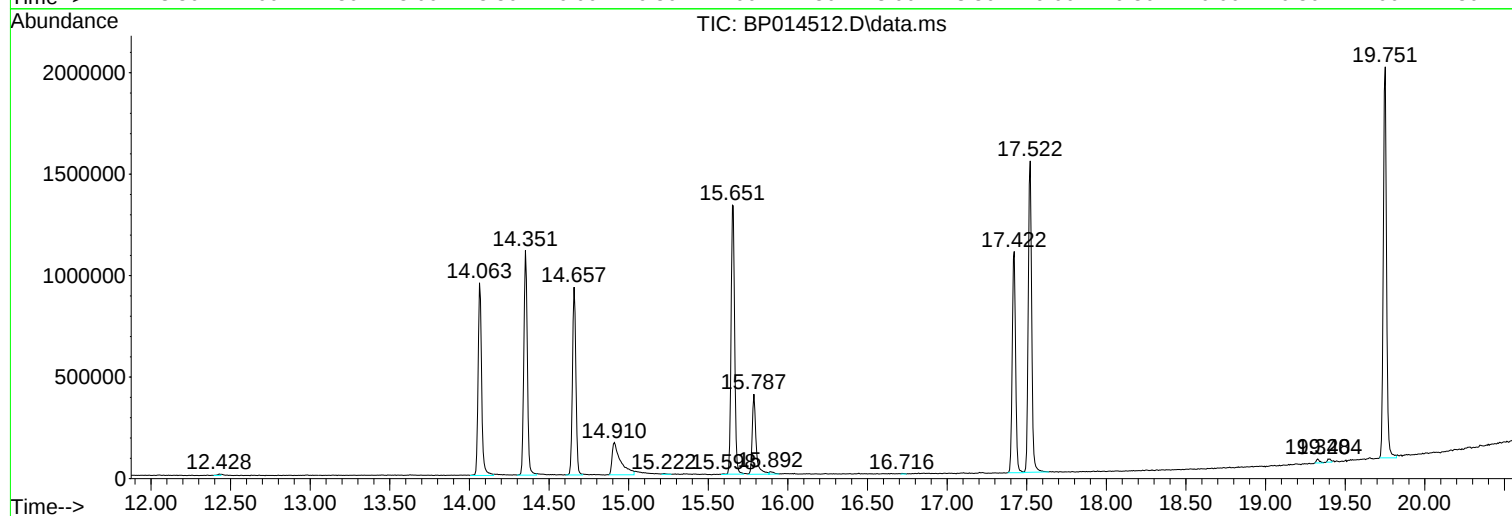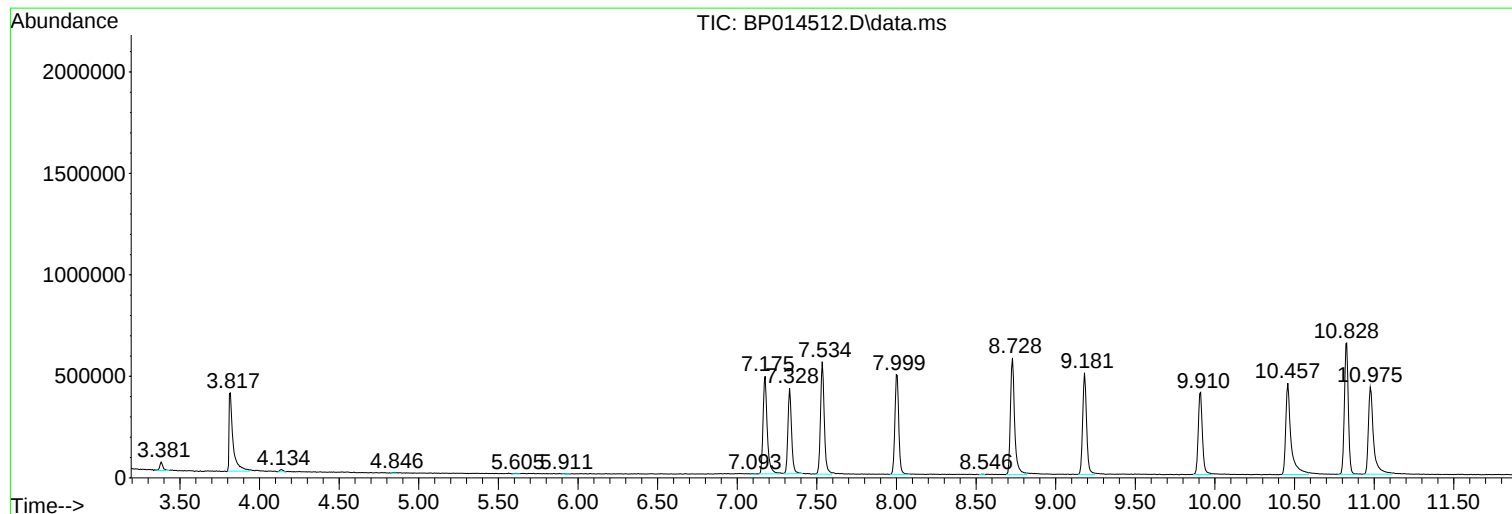

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014512.D
Acq On : 04 Apr 2023 05:54
Operator : CG/JU
Sample : PB151804BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK804

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014512.D
Acq On : 04 Apr 2023 05:54
Operator : CG/JU
Sample : PB151804BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK804

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc