

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014520.D
 Acq On : 04 Apr 2023 10:23
 Operator : CG/JU
 Sample : 02158-20
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FB(20230330)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	30	33	39	rBV	29130	38483	1.10%	0.109%
2	3.734	91	93	98	rVB5	7586	9392	0.27%	0.027%
3	3.846	110	112	124	rBV	33863	78652	2.26%	0.222%
4	4.034	140	144	150	rVB2	16008	26150	0.75%	0.074%
5	4.140	158	162	166	rBV2	9172	13507	0.39%	0.038%
6	4.252	177	181	186	rBV7	7131	11340	0.33%	0.032%
7	4.446	212	214	221	rBV8	2906	3914	0.11%	0.011%
8	4.558	231	233	238	rVB6	3508	3815	0.11%	0.011%
9	5.069	315	320	327	rBV2	13464	22121	0.64%	0.062%
10	5.987	471	476	480	rBV8	2058	4647	0.13%	0.013%
11	6.040	482	485	493	rVB9	4133	8056	0.23%	0.023%
12	6.387	539	544	550	rVB3	7268	14909	0.43%	0.042%
13	6.516	562	566	571	rVB8	2408	4798	0.14%	0.014%
14	6.869	620	626	630	rBV9	1690	4012	0.12%	0.011%
15	6.969	642	643	647	rBV4	2674	3664	0.11%	0.010%
16	7.181	673	679	696	rBV	98182	210500	6.04%	0.594%
17	7.328	698	704	717	rBV	522457	826406	23.73%	2.333%
18	7.534	732	739	757	rBV	477634	817278	23.46%	2.307%
19	8.005	811	819	827	rBV	555437	945640	27.15%	2.670%
20	8.728	935	942	957	rBV	333143	630097	18.09%	1.779%
21	8.852	957	963	968	rVB4	16105	32047	0.92%	0.090%
22	9.181	1012	1019	1039	rBV	645578	1121612	32.20%	3.166%
23	9.334	1042	1045	1048	rVV5	3856	5587	0.16%	0.016%
24	9.546	1077	1081	1087	rVB9	4342	5980	0.17%	0.017%
25	9.904	1135	1142	1153	rBV	526735	921723	26.46%	2.602%
26	10.457	1227	1236	1255	rBV	543758	1203145	34.54%	3.397%
27	10.728	1276	1282	1286	rBV9	2918	4882	0.14%	0.014%
28	10.828	1291	1299	1307	rBV	811827	1402161	40.26%	3.958%
29	10.975	1317	1324	1348	rBV	382346	846232	24.29%	2.389%
30	11.369	1386	1391	1396	rBV3	10790	19077	0.55%	0.054%
31	11.440	1396	1403	1411	rVB4	10380	27451	0.79%	0.077%
32	11.687	1441	1445	1446	rBV4	3234	3765	0.11%	0.011%
33	11.775	1457	1460	1466	rVB7	2841	4767	0.14%	0.013%
34	12.046	1502	1506	1510	rBV6	3079	3902	0.11%	0.011%
35	12.428	1565	1571	1578	rBV3	10149	19921	0.57%	0.056%
36	13.263	1708	1713	1716	rBV7	3507	4730	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014520.D
 Acq On : 04 Apr 2023 10:23
 Operator : CG/JU
 Sample : 02158-20
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FB(20230330)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	13.540	1754	1760	1767	rBV2	33152	54611	1.57%	0.154%
38	13.628	1772	1775	1779	rVB6	2805	4112	0.12%	0.012%
39	14.063	1839	1849	1864	rBV	1514661	2140804	61.46%	6.044%
40	14.351	1891	1898	1913	rBV	1615642	2392426	68.69%	6.754%
41	14.657	1943	1950	1960	rBV	1312145	1938376	55.65%	5.472%
42	14.951	1994	2000	2002	rBV4	22233	41246	1.18%	0.116%
43	15.475	2086	2089	2095	rVB6	6063	8705	0.25%	0.025%
44	15.651	2112	2119	2131	rVV	2002063	3012960	86.50%	8.506%
45	15.786	2135	2142	2153	rVV	540309	933394	26.80%	2.635%
46	15.892	2156	2160	2168	rVB8	12118	26787	0.77%	0.076%
47	16.010	2177	2180	2183	rBV3	5545	7386	0.21%	0.021%
48	16.616	2281	2283	2289	rVB7	2062	3851	0.11%	0.011%
49	16.845	2320	2322	2327	rVB6	3209	5093	0.15%	0.014%
50	17.151	2372	2374	2381	rBV8	2975	4615	0.13%	0.013%
51	17.210	2381	2384	2389	rVB7	4889	7551	0.22%	0.021%
52	17.416	2412	2419	2430	rBV	1475013	2177266	62.51%	6.147%
53	17.522	2430	2437	2449	rVV	2331564	3408782	97.86%	9.623%
54	18.075	2527	2531	2535	rVB7	5938	9473	0.27%	0.027%
55	18.292	2565	2568	2574	rBV8	13531	22796	0.65%	0.064%
56	18.651	2627	2629	2631	rBV3	5948	5583	0.16%	0.016%
57	19.327	2741	2744	2747	rVB3	25505	30325	0.87%	0.086%
58	19.398	2752	2756	2764	rBV3	28976	47086	1.35%	0.133%
59	19.745	2810	2815	2824	rBV	2498804	3483164	100.00%	9.833%
60	21.504	3110	3114	3123	rBV	1132910	1699675	48.80%	4.798%
61	23.851	3507	3513	3530	rVB	1438470	3044863	87.42%	8.596%
62	24.021	3536	3542	3551	rVB2	746322	1606769	46.13%	4.536%




Sum of corrected areas: 35422062

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014520.D
Acq On : 04 Apr 2023 10:23
Operator : CG/JU
Sample : 02158-20
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB(20230330)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

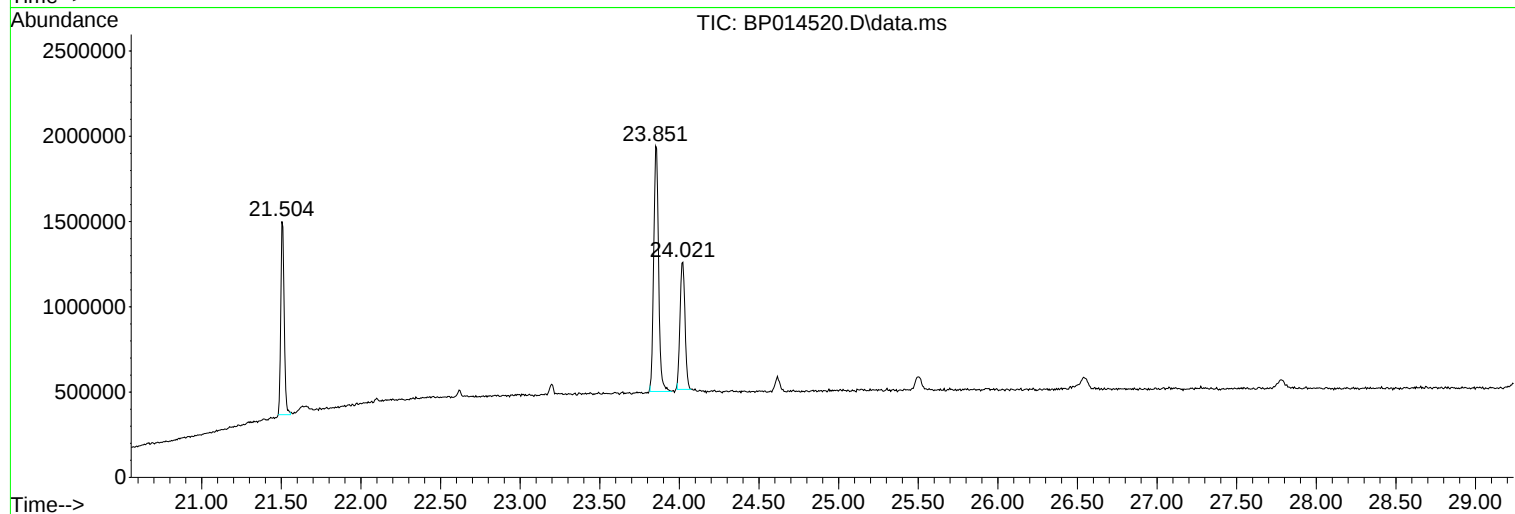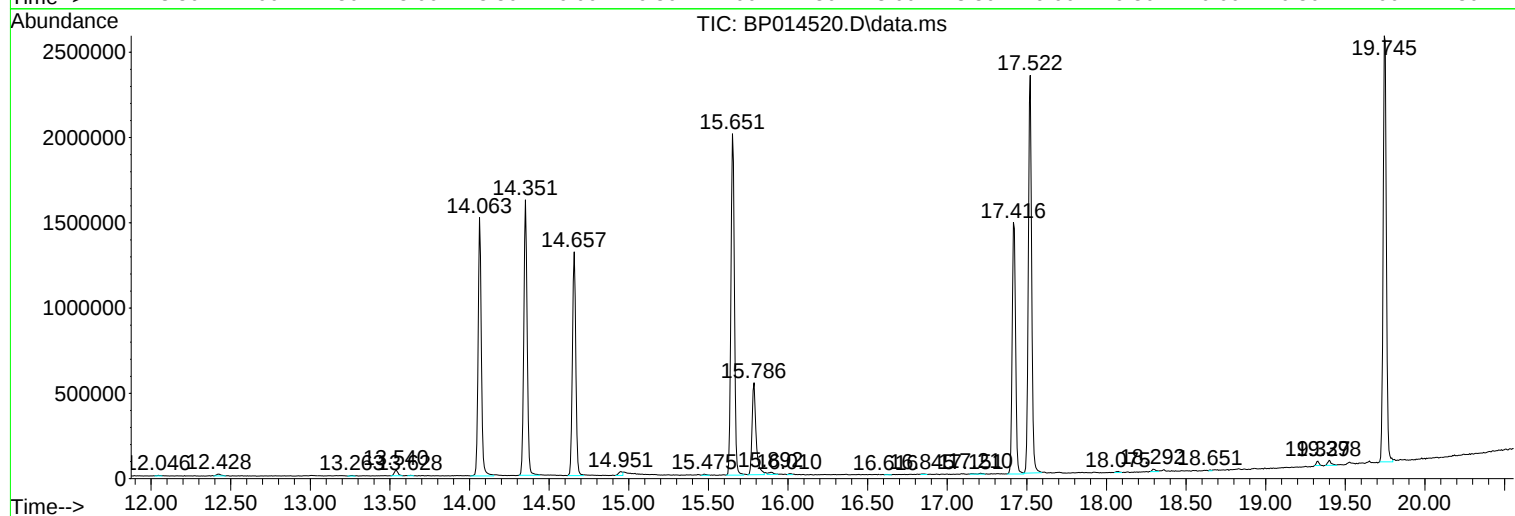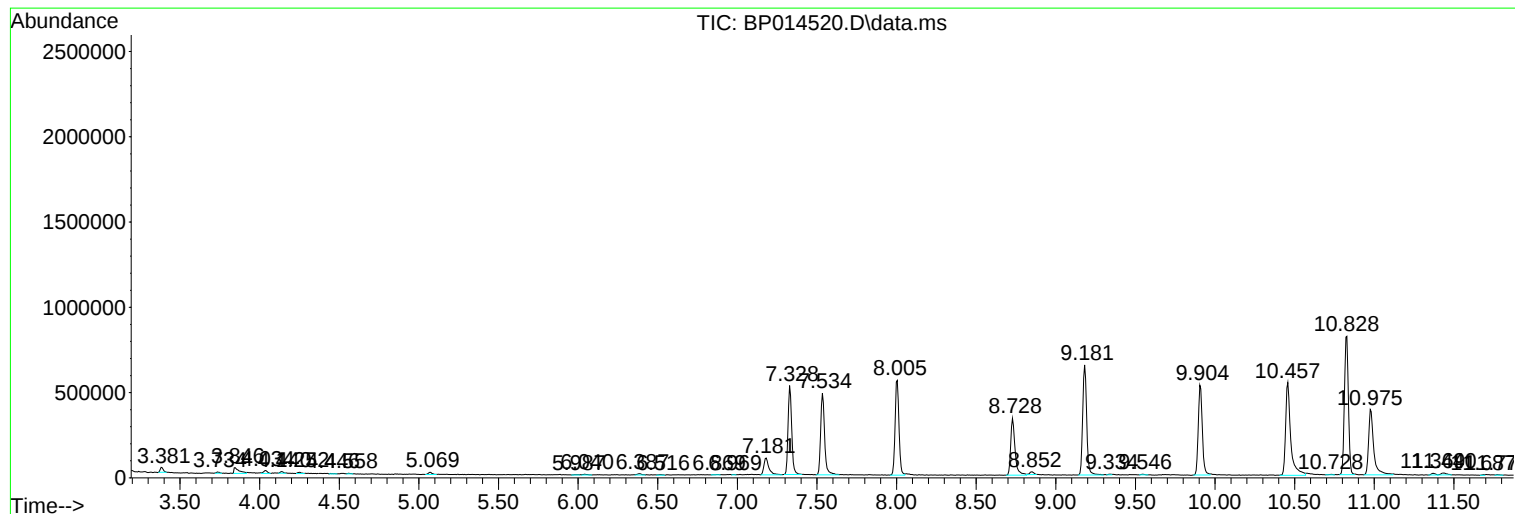

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014520.D
Acq On : 04 Apr 2023 10:23
Operator : CG/JU
Sample : 02158-20
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB(20230330)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014520.D
Acq On : 04 Apr 2023 10:23
Operator : CG/JU
Sample : 02158-20
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB(20230330)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc