

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014524.D
 Acq On : 04 Apr 2023 12:54
 Operator : CG/JU
 Sample : 02092-23DL 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB998DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.416	35	39	47	rVB	151710	184269	9.33%	1.425%
2	3.893	117	120	123	rBV4	6843	12918	0.65%	0.100%
3	4.134	157	161	167	rVB3	11424	17947	0.91%	0.139%
4	4.211	167	174	179	rBV	19848	31796	1.61%	0.246%
5	4.252	179	181	187	rVB7	5652	8321	0.42%	0.064%
6	4.593	235	239	248	rVB2	35372	58090	2.94%	0.449%
7	4.969	298	303	304	rBV5	3436	5015	0.25%	0.039%
8	5.287	355	357	361	rVB5	3535	3656	0.19%	0.028%
9	5.410	376	378	382	rVB5	3406	3480	0.18%	0.027%
10	5.540	398	400	404	rVB5	2244	3049	0.15%	0.024%
11	5.681	420	424	429	rBV7	1868	3021	0.15%	0.023%
12	5.740	429	434	440	rBV7	10978	22760	1.15%	0.176%
13	5.934	463	467	469	rVB5	2629	3633	0.18%	0.028%
14	6.269	519	524	531	rVB2	5555	10731	0.54%	0.083%
15	6.563	571	574	577	rBV5	1917	3179	0.16%	0.025%
16	6.657	582	590	593	rBV10	3180	7878	0.40%	0.061%
17	6.957	637	641	646	rBV7	6580	9687	0.49%	0.075%
18	7.204	679	683	694	rVB5	9285	22786	1.15%	0.176%
19	7.334	700	705	715	rBV	28719	57583	2.92%	0.445%
20	7.481	724	730	733	rBV7	6739	13399	0.68%	0.104%
21	7.546	733	741	752	rVV	23572	54173	2.74%	0.419%
22	7.746	771	775	781	rVB9	3070	5491	0.28%	0.042%
23	7.846	788	792	797	rVB8	2581	4883	0.25%	0.038%
24	7.904	797	802	807	rVB9	2631	5862	0.30%	0.045%
25	8.004	807	819	830	rBV	455097	780349	39.51%	6.034%
26	8.081	830	832	833	rBV2	5490	4682	0.24%	0.036%
27	8.663	927	931	932	rBV4	2606	3097	0.16%	0.024%
28	8.751	936	946	952	rBV3	19622	52482	2.66%	0.406%
29	9.004	981	989	1003	rBV	591689	1076190	54.49%	8.322%
30	9.122	1005	1009	1016	rVV5	15160	30639	1.55%	0.237%
31	9.193	1016	1021	1029	rVB	32690	63099	3.19%	0.488%
32	9.316	1039	1042	1044	rBV4	2393	3551	0.18%	0.027%
33	9.375	1048	1052	1057	rVV8	5285	10048	0.51%	0.078%
34	9.528	1071	1078	1085	rVV8	12502	27429	1.39%	0.212%
35	9.587	1086	1088	1092	rVV4	4881	5163	0.26%	0.040%
36	9.651	1094	1099	1107	rVB9	6487	16824	0.85%	0.130%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014524.D
 Acq On : 04 Apr 2023 12:54
 Operator : CG/JU
 Sample : 02092-23DL 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB998DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	9.734	1107	1113	1122	rBV9	5403	15252	0.77%	0.118%
38	9.916	1137	1144	1156	rBV6	21311	61404	3.11%	0.475%
39	10.034	1159	1164	1168	rVV6	9490	19986	1.01%	0.155%
40	10.087	1168	1173	1182	rVV4	14775	33083	1.67%	0.256%
41	10.234	1194	1198	1203	rVV8	2407	4563	0.23%	0.035%
42	10.363	1210	1220	1229	rBV7	20509	50696	2.57%	0.392%
43	10.451	1231	1235	1236	rBV4	4173	4693	0.24%	0.036%
44	10.498	1236	1243	1257	rVV6	22480	75998	3.85%	0.588%
45	10.828	1289	1299	1313	rBV	590480	1083789	54.87%	8.381%
46	10.951	1316	1320	1323	rVV5	12287	20700	1.05%	0.160%
47	11.004	1323	1329	1337	rVV3	27120	73726	3.73%	0.570%
48	11.063	1337	1339	1340	rVV2	6237	6091	0.31%	0.047%
49	11.087	1340	1343	1353	rVV2	8150	22480	1.14%	0.174%
50	11.157	1353	1355	1356	rVV2	3405	3406	0.17%	0.026%
51	11.187	1358	1360	1366	rVB7	5057	6736	0.34%	0.052%
52	11.393	1391	1395	1397	rBV5	2660	3494	0.18%	0.027%
53	11.422	1397	1400	1402	rVV4	2739	3175	0.16%	0.025%
54	11.534	1416	1419	1424	rVB7	2710	3824	0.19%	0.030%
55	11.657	1438	1440	1442	rVV3	4518	5438	0.28%	0.042%
56	11.681	1442	1444	1449	rVV6	4820	6972	0.35%	0.054%
57	11.810	1462	1466	1470	rVB7	3150	5502	0.28%	0.043%
58	12.028	1499	1503	1510	rBV9	7302	14891	0.75%	0.115%
59	12.175	1522	1528	1533	rBV3	11063	22927	1.16%	0.177%
60	12.222	1534	1536	1540	rVB4	3515	3294	0.17%	0.025%
61	12.275	1542	1545	1551	rBV8	5316	9026	0.46%	0.070%
62	12.351	1551	1558	1568	rBV2	54635	134437	6.81%	1.040%
63	12.457	1571	1576	1584	rVB10	12801	33711	1.71%	0.261%
64	12.551	1584	1592	1595	rBV10	5351	10755	0.54%	0.083%
65	12.616	1601	1603	1606	rBV4	3045	3882	0.20%	0.030%
66	12.651	1606	1609	1613	rVV6	3733	7020	0.36%	0.054%
67	12.822	1635	1638	1643	rVV5	9185	14987	0.76%	0.116%
68	12.916	1652	1654	1661	rVB8	5328	8706	0.44%	0.067%
69	12.975	1661	1664	1666	rBV4	2735	3739	0.19%	0.029%
70	13.281	1714	1716	1719	rVB4	3977	4801	0.24%	0.037%
71	13.387	1732	1734	1739	rVB6	4301	4849	0.25%	0.037%
72	13.463	1745	1747	1751	rVB5	5339	5121	0.26%	0.040%
73	13.539	1758	1760	1766	rVB7	7447	9577	0.48%	0.074%
74	13.628	1770	1775	1778	rBV7	3298	5657	0.29%	0.044%
75	13.710	1783	1789	1796	rBV7	9975	20999	1.06%	0.162%
76	14.069	1845	1850	1858	rVB	75089	128496	6.51%	0.994%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014524.D
 Acq On : 04 Apr 2023 12:54
 Operator : CG/JU
 Sample : 02092-23DL 10X
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB998DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

77	14.351	1893	1898	1905	rBV	88185	147078	7.45%	1.137%
78	14.469	1914	1918	1920	rBV5	6691	10222	0.52%	0.079%
79	14.581	1932	1937	1941	rVB4	33134	45502	2.30%	0.352%
80	14.657	1943	1950	1959	rBV	841191	1267368	64.17%	9.801%
81	15.263	2049	2053	2058	rVB8	8634	16078	0.81%	0.124%
82	15.398	2073	2076	2082	rBV4	9506	17951	0.91%	0.139%
83	15.475	2085	2089	2097	rVB2	33120	53284	2.70%	0.412%
84	15.657	2114	2120	2133	rVB	115649	191884	9.72%	1.484%
85	15.822	2143	2148	2153	rBV9	9256	19318	0.98%	0.149%
86	15.922	2159	2165	2172	rBV9	11033	24763	1.25%	0.191%
87	16.028	2180	2183	2187	rVB4	12797	16849	0.85%	0.130%
88	16.116	2194	2198	2202	rVB7	6083	8901	0.45%	0.069%
89	16.180	2203	2209	2217	rBV	85311	147343	7.46%	1.139%
90	16.698	2293	2297	2304	rBV	39283	69685	3.53%	0.539%
91	16.951	2338	2340	2343	rVB3	8191	6680	0.34%	0.052%
92	17.210	2379	2384	2385	rBV5	6209	10748	0.54%	0.083%
93	17.422	2413	2420	2432	rBV	953305	1485888	75.23%	11.490%
94	17.522	2432	2437	2446	rVB2	128219	196594	9.95%	1.520%
95	18.286	2564	2567	2573	rBV6	21113	35920	1.82%	0.278%
96	19.045	2693	2696	2701	rVB5	31448	38347	1.94%	0.297%
97	19.751	2811	2816	2821	rBV	191195	268534	13.60%	2.077%
98	21.510	3110	3115	3122	rBV	1272600	1806155	91.45%	13.967%
99	23.857	3510	3514	3525	rVB	242986	486249	24.62%	3.760%
100	24.015	3535	3541	3552	rVB2	903155	1975122	100.00%	15.274%




Sum of corrected areas: 12931506

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014524.D
Acq On : 04 Apr 2023 12:54
Operator : CG/JU
Sample : 02092-23DL 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB998DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

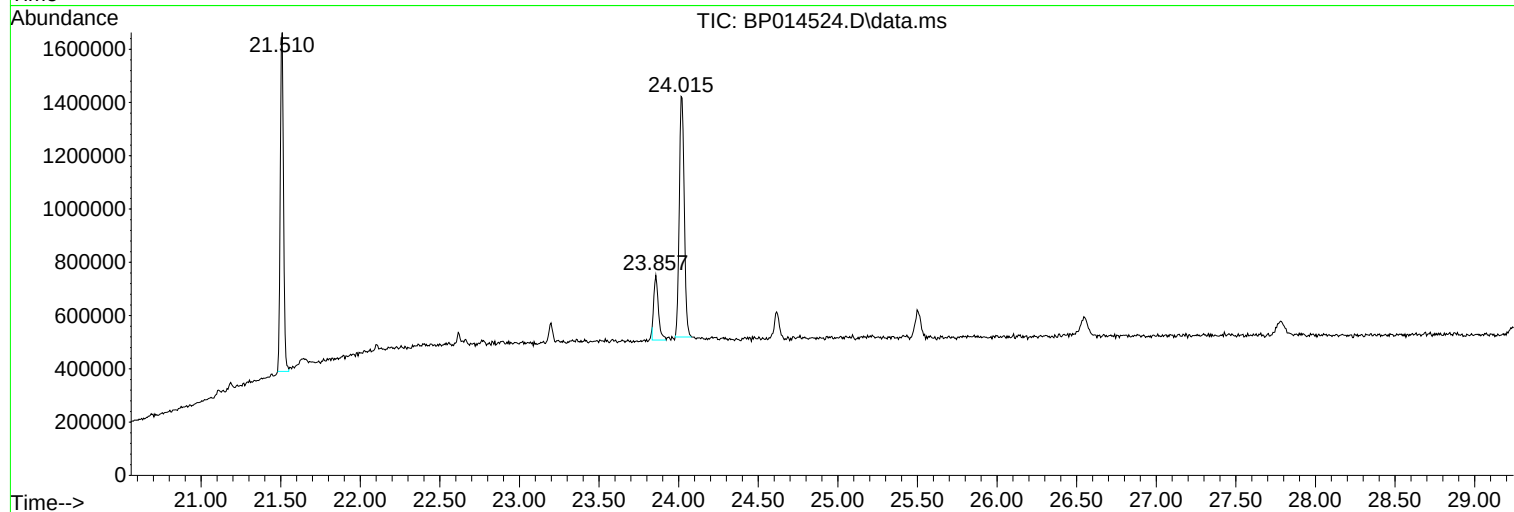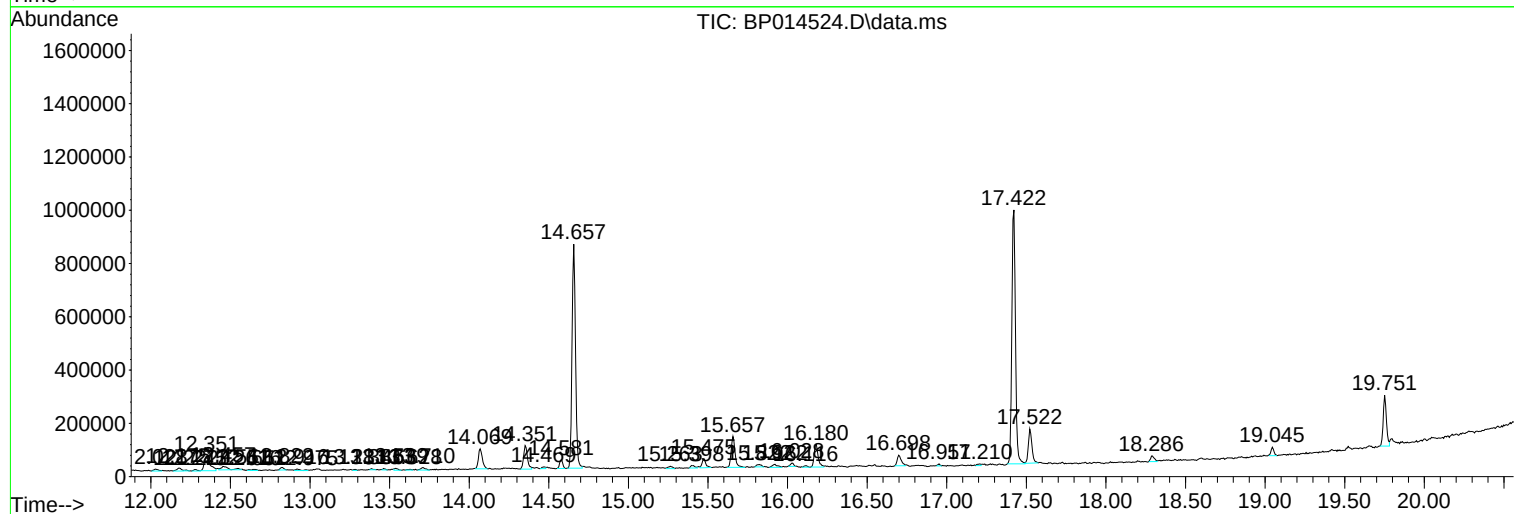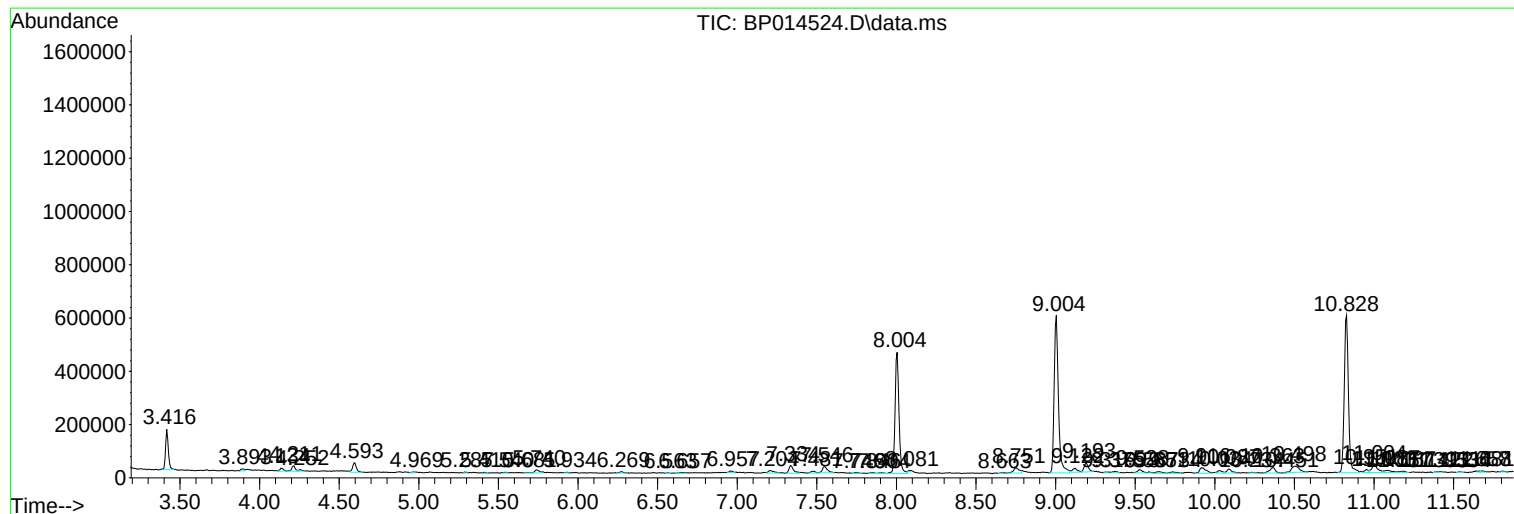

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014524.D
Acq On : 04 Apr 2023 12:54
Operator : CG/JU
Sample : 02092-23DL 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB998DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzenamine, 3-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.004	27.58 ng/ul	1076190	1,4-Dichlorobenzene-d4	8.004

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzenamine, 3-methyl-	107	C7H9N	000108-44-1	97
2			Benzenamine, 3-methyl-	107	C7H9N	000108-44-1	97
3			Benzenamine, 3-methyl-	107	C7H9N	000108-44-1	97
4			Benzenamine, 3-methyl-	107	C7H9N	000108-44-1	96
5			o-Toluidine	107	C7H9N	000095-53-4	94

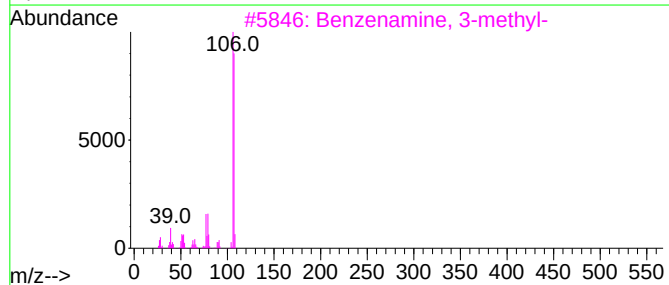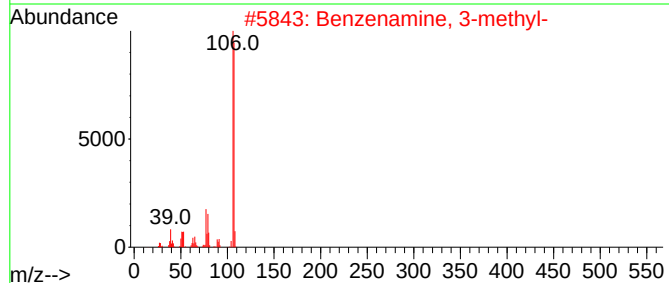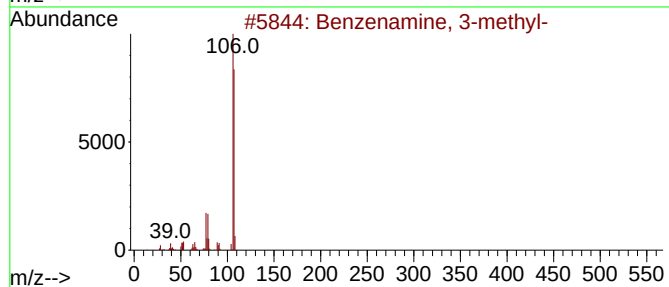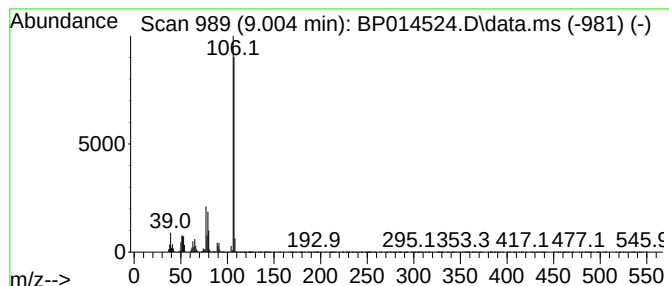

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014524.D
Acq On : 04 Apr 2023 12:54
Operator : CG/JU
Sample : 02092-23DL 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB998DL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Benzenamine, 3-chloro-4-met... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.351	2.48 ng/ul	134437	Naphthalene-d8	10.828

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzenamine, 3-chloro-4-methyl-	141	C7H8ClN	000095-74-9	98
2			Benzenamine, 3-chloro-4-methyl-	141	C7H8ClN	000095-74-9	98
3			Benzenamine, 2-chloro-4-methyl-	141	C7H8ClN	000615-65-6	95
4			Benzenamine, 3-chloro-4-methyl-	141	C7H8ClN	000095-74-9	95
5			Benzenamine, 2-chloro-4-methyl-	141	C7H8ClN	000615-65-6	94

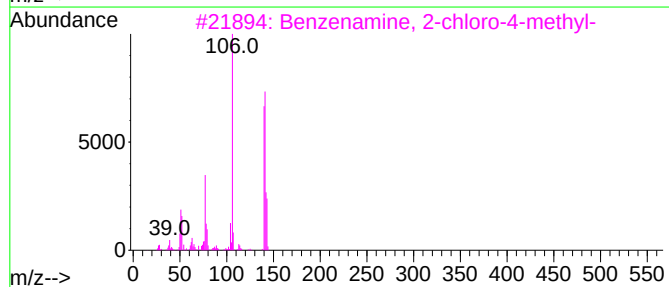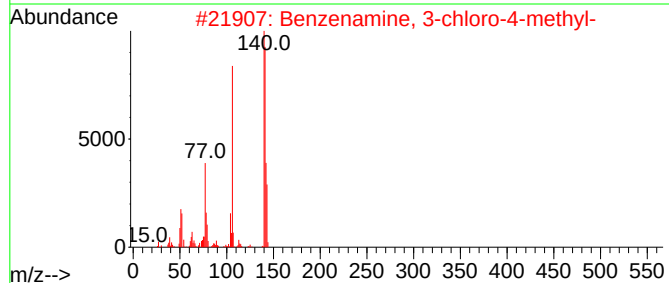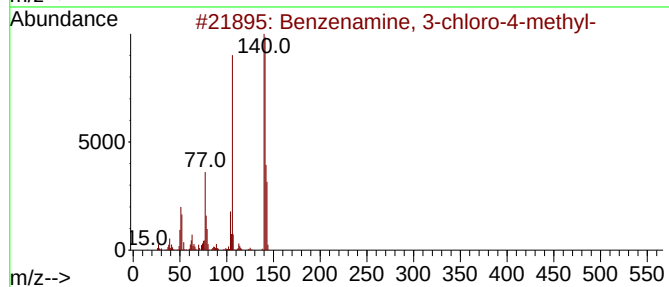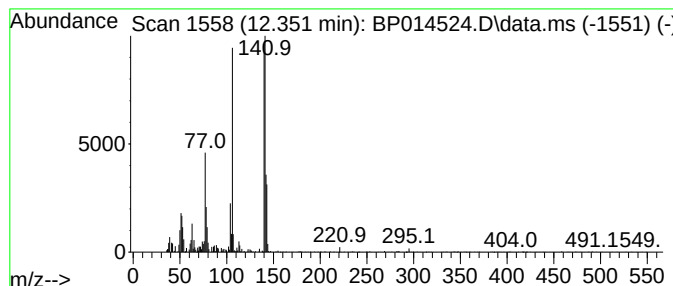

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014524.D
Acq On : 04 Apr 2023 12:54
Operator : CG/JU
Sample : 02092-23DL 10X
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB998DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzenamine, 3-...	9.004	27.6	ng/ul	1076190	1	8.004	780349	20.0
Benzenamine, 3-...	12.351	2.5	ng/ul	134437	2	10.828	1083790	20.0