

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014528.D
 Acq On : 04 Apr 2023 15:10
 Operator : CG/JU
 Sample : PB151803BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK803

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	29	33	39	rVB	32091	39649	1.25%	0.134%
2	3.817	105	107	127	rBV	329850	569828	17.90%	1.931%
3	4.140	159	162	169	rVB3	8459	11628	0.37%	0.039%
4	5.028	310	313	317	rVB6	2535	3212	0.10%	0.011%
5	5.999	475	478	483	rVB7	2916	4321	0.14%	0.015%
6	7.175	671	678	696	rBV	380785	745430	23.42%	2.526%
7	7.328	698	704	716	rVV	344561	552172	17.35%	1.871%
8	7.534	733	739	756	rVV	445099	745810	23.43%	2.527%
9	8.005	810	819	832	rBV	397252	676594	21.26%	2.293%
10	8.093	832	834	839	rVB6	2579	4032	0.13%	0.014%
11	8.728	936	942	955	rBV	450638	874310	27.47%	2.963%
12	9.181	1010	1019	1033	rBV	423367	731792	22.99%	2.480%
13	9.905	1132	1142	1161	rBV	332703	640970	20.14%	2.172%
14	10.458	1229	1236	1257	rBV	342553	855173	26.87%	2.898%
15	10.822	1291	1298	1312	rVV	552530	962670	30.24%	3.262%
16	10.975	1318	1324	1342	rBV	277798	664507	20.88%	2.252%
17	12.434	1566	1572	1574	rBV7	5554	9231	0.29%	0.031%
18	13.622	1772	1774	1777	rBV4	2947	3640	0.11%	0.012%
19	14.063	1840	1849	1866	rBV	875992	1373285	43.14%	4.654%
20	14.351	1891	1898	1911	rBV	1035171	1549157	48.67%	5.250%
21	14.657	1943	1950	1962	rBV	894968	1303793	40.96%	4.418%
22	14.910	1986	1993	2012	rBV2	153941	566019	17.78%	1.918%
23	15.204	2041	2043	2048	rVB6	2660	3266	0.10%	0.011%
24	15.651	2113	2119	2135	rVV	1275944	1990102	62.52%	6.744%
25	15.787	2135	2142	2157	rBV	371078	638822	20.07%	2.165%
26	15.898	2157	2161	2165	rVB6	8062	14148	0.44%	0.048%
27	16.563	2270	2274	2276	rBV5	2862	4850	0.15%	0.016%
28	17.098	2363	2365	2370	rVB6	2728	3397	0.11%	0.012%
29	17.298	2397	2399	2403	rBV5	2179	3568	0.11%	0.012%
30	17.416	2412	2419	2430	rBV	1144137	1660931	52.18%	5.628%
31	17.516	2430	2436	2448	rBV	1501200	2264131	71.13%	7.672%
32	19.328	2740	2744	2750	rBV5	24304	38099	1.20%	0.129%
33	19.398	2753	2756	2758	rBV3	16898	18628	0.59%	0.063%
34	19.745	2810	2815	2828	rBV	1971941	2826832	88.81%	9.579%
35	21.504	3109	3114	3123	rBV	1292648	1954670	61.41%	6.624%
36	23.851	3506	3513	3527	rVB	1536596	3183015	100.00%	10.786%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014528.D
Acq On : 04 Apr 2023 15:10
Operator : CG/JU
Sample : PB151803BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK803

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37 24.016 3535 3541 3556 rVB2 937442 2018768 63.42% 6.841%




Sum of corrected areas: 29510450

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014528.D
Acq On : 04 Apr 2023 15:10
Operator : CG/JU
Sample : PB151803BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK803

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

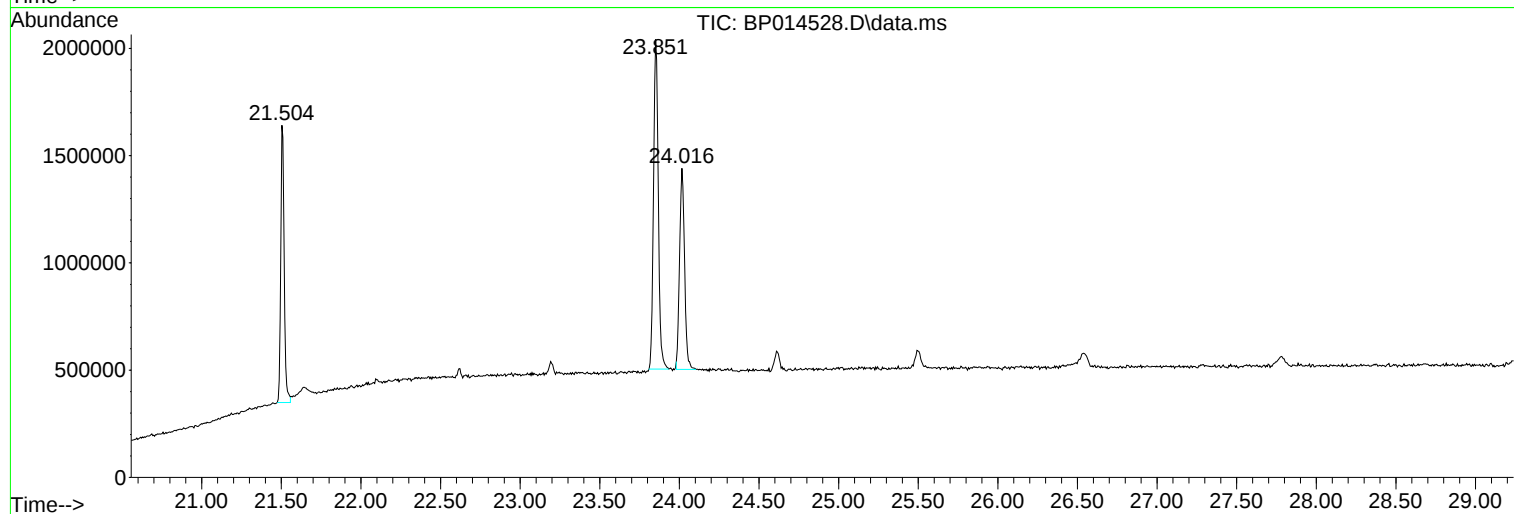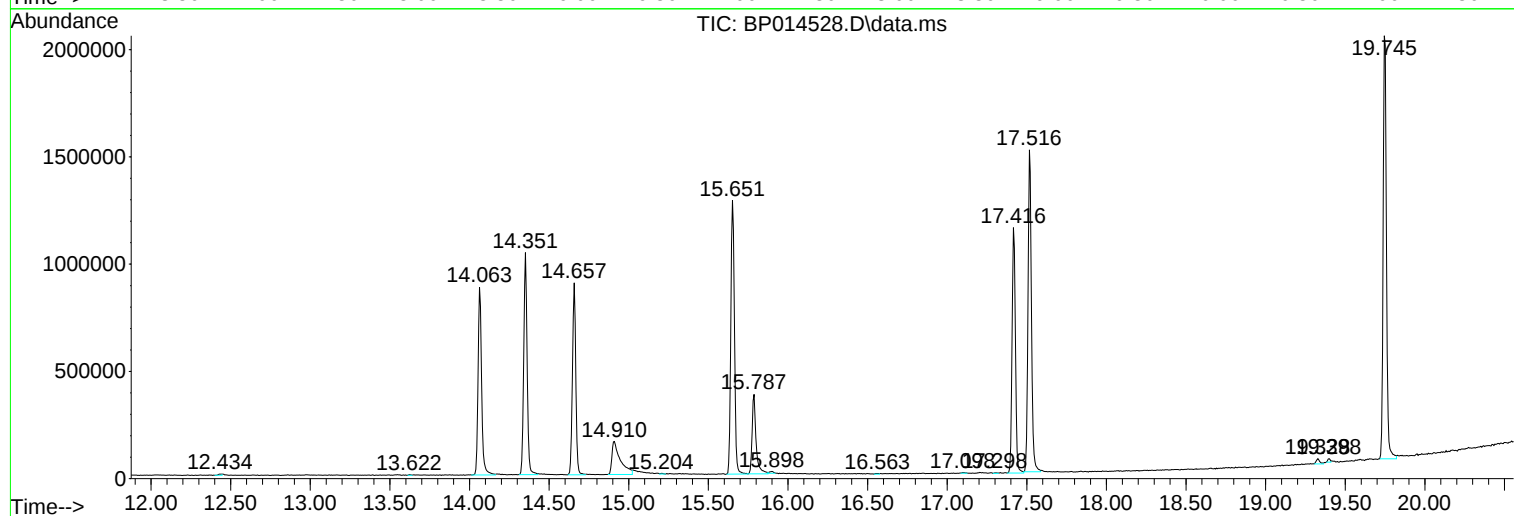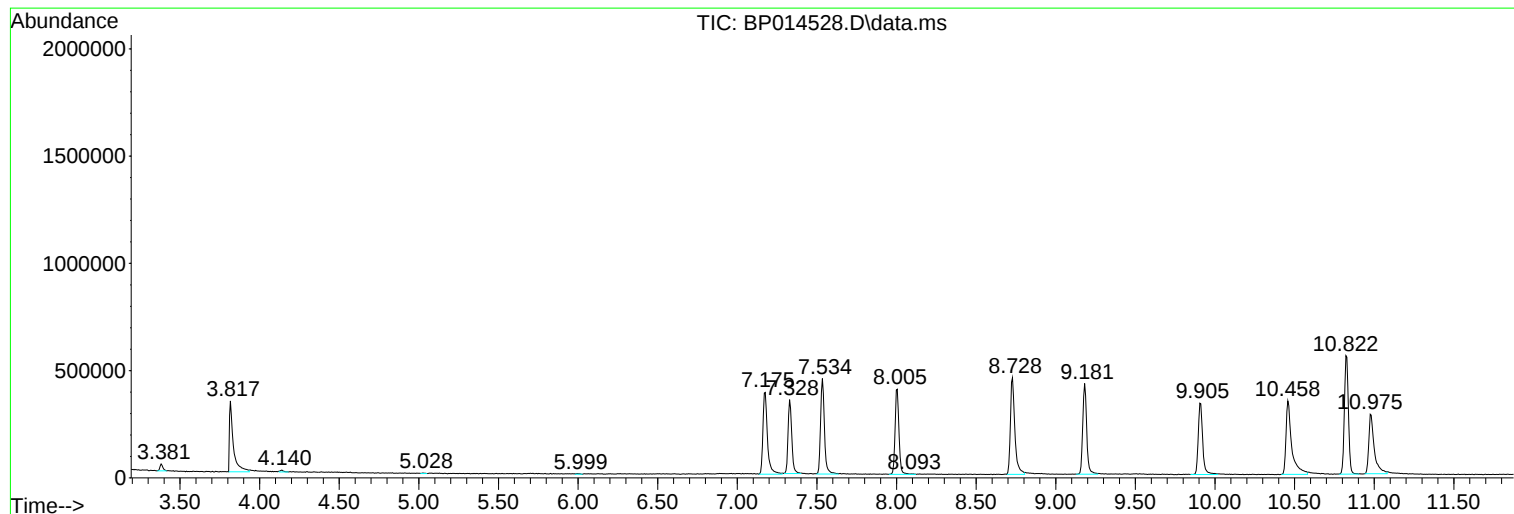

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014528.D
Acq On : 04 Apr 2023 15:10
Operator : CG/JU
Sample : PB151803BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK803

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014528.D
Acq On : 04 Apr 2023 15:10
Operator : CG/JU
Sample : PB151803BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK803

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc