

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014534.D
 Acq On : 04 Apr 2023 18:36
 Operator : CG/JU
 Sample : 02158-21
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FB(20230331)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	30	33	38	rBV	29293	36584	0.78%	0.101%
2	3.740	91	94	98	rVB5	6343	8668	0.19%	0.024%
3	3.834	108	110	122	rBV	67093	119196	2.54%	0.329%
4	4.034	141	144	148	rVB3	11691	13950	0.30%	0.038%
5	4.140	158	162	169	rBV3	9223	14351	0.31%	0.040%
6	4.252	178	181	185	rVB6	7676	10690	0.23%	0.029%
7	5.069	316	320	331	rVB	10378	18007	0.38%	0.050%
8	6.034	481	484	486	rBV4	3526	4690	0.10%	0.013%
9	6.387	540	544	549	rVB6	6530	9972	0.21%	0.028%
10	7.181	673	679	694	rVV	87740	180844	3.86%	0.499%
11	7.328	698	704	719	rVB	408601	656074	14.00%	1.810%
12	7.534	731	739	755	rBV	397202	696849	14.88%	1.922%
13	8.004	812	819	828	rBV	471152	784624	16.75%	2.164%
14	8.734	936	943	956	rBV	272869	544704	11.63%	1.503%
15	8.846	959	962	969	rVB3	13323	23685	0.51%	0.065%
16	9.181	1012	1019	1033	rBV	519875	903797	19.29%	2.493%
17	9.346	1039	1047	1049	rBV8	4009	8801	0.19%	0.024%
18	9.551	1076	1082	1088	rVB8	3334	6999	0.15%	0.019%
19	9.904	1136	1142	1156	rBV	397246	733154	15.65%	2.022%
20	10.457	1229	1236	1262	rBV	438329	1025345	21.89%	2.828%
21	10.822	1290	1298	1309	rVB	672428	1153478	24.62%	3.182%
22	10.975	1316	1324	1345	rBV	411644	877280	18.73%	2.420%
23	11.375	1387	1392	1397	rBV4	6136	12187	0.26%	0.034%
24	11.434	1397	1402	1408	rBV4	9906	19292	0.41%	0.053%
25	12.422	1564	1570	1576	rBV7	8532	15716	0.34%	0.043%
26	13.251	1708	1711	1714	rBV5	3429	4863	0.10%	0.013%
27	13.539	1751	1760	1766	rBV3	29848	52748	1.13%	0.146%
28	14.063	1838	1849	1861	rBV	1255534	1798608	38.39%	4.961%
29	14.298	1882	1889	1891	rBV8	3523	6660	0.14%	0.018%
30	14.351	1891	1898	1908	rBV	1326339	1999705	42.69%	5.516%
31	14.657	1941	1950	1960	rBV	1098481	1624446	34.68%	4.481%
32	14.945	1992	1999	2009	rBV7	29597	112304	2.40%	0.310%
33	15.475	2085	2089	2093	rBV6	5502	8762	0.19%	0.024%
34	15.651	2112	2119	2131	rBV	1783578	2660678	56.80%	7.339%
35	15.786	2136	2142	2152	rBV	429745	756118	16.14%	2.086%
36	15.892	2158	2160	2167	rVB4	12589	18827	0.40%	0.052%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014534.D
Acq On : 04 Apr 2023 18:36
Operator : CG/JU
Sample : 02158-21
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB(20230331)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	16.010	2176	2180	2185	rBV8	6699	8556	0.18%	0.024%
38	17.416	2413	2419	2429	rBV	1467529	2100916	44.85%	5.795%
39	17.516	2430	2436	2451	rVV	2287824	3327935	71.04%	9.180%
40	18.292	2564	2568	2576	rBV6	31510	65642	1.40%	0.181%
41	18.357	2577	2579	2584	rVB2	18439	18850	0.40%	0.052%
42	19.398	2753	2756	2762	rVB	33500	44007	0.94%	0.121%
43	19.745	2810	2815	2827	rBV	3033121	4048679	86.42%	11.168%
44	21.504	3109	3114	3122	rBV	1784337	2494071	53.24%	6.880%
45	23.851	3506	3513	3527	rBV2	2325759	4684636	100.00%	12.922%
46	24.015	3535	3541	3551	rVB2	1204121	2536473	54.14%	6.997%




Sum of corrected areas: 36252421

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014534.D
Acq On : 04 Apr 2023 18:36
Operator : CG/JU
Sample : 02158-21
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB(20230331)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

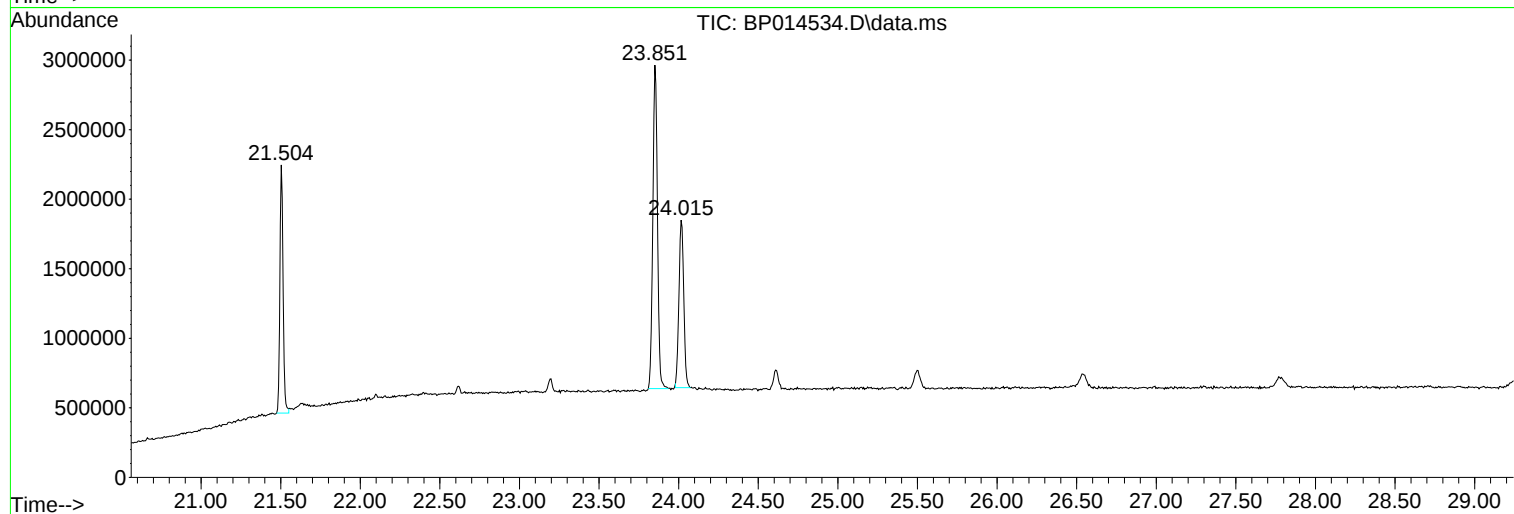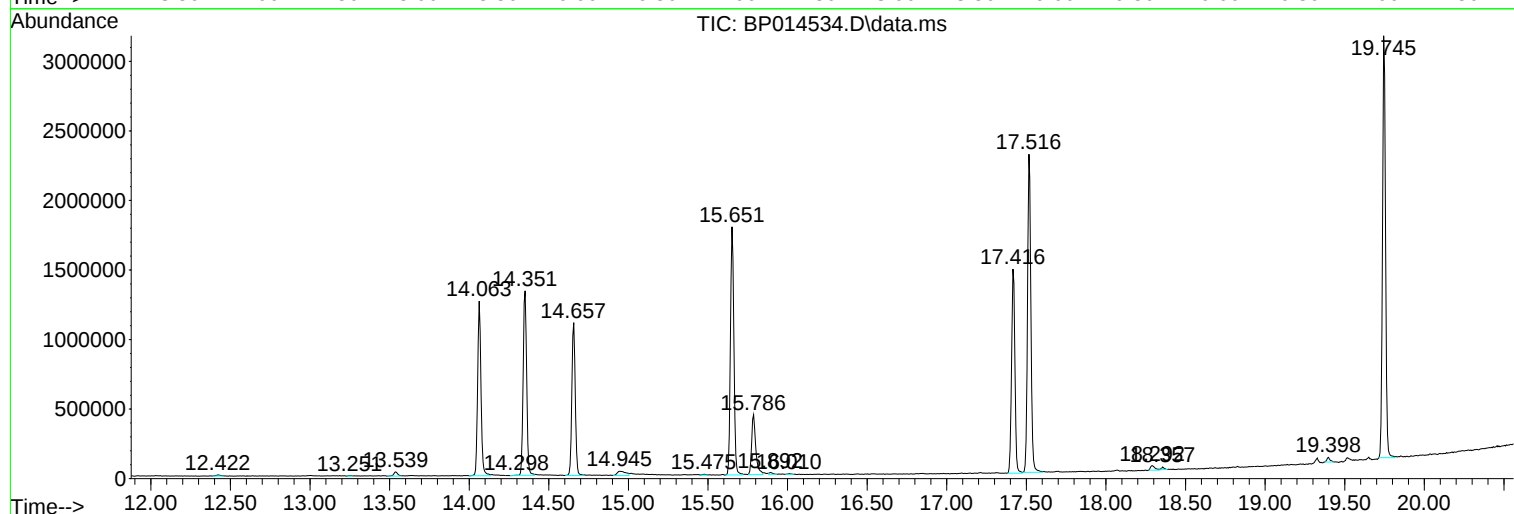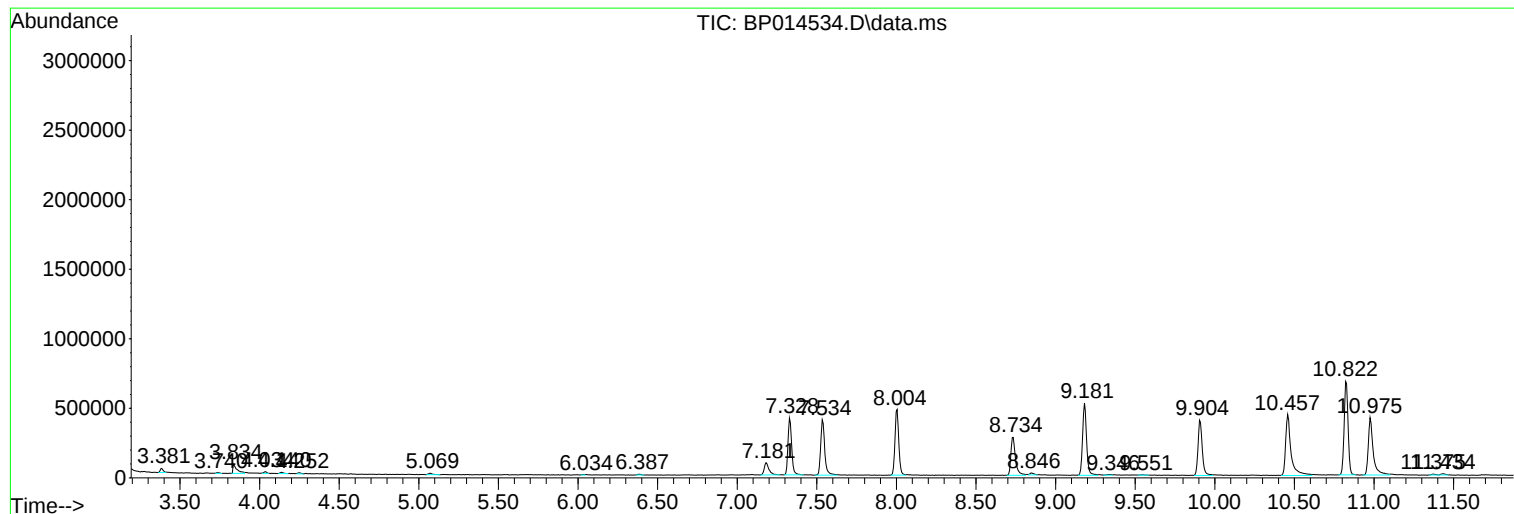

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014534.D
Acq On : 04 Apr 2023 18:36
Operator : CG/JU
Sample : 02158-21
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB(20230331)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014534.D
Acq On : 04 Apr 2023 18:36
Operator : CG/JU
Sample : 02158-21
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB(20230331)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------