

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014535.D
 Acq On : 04 Apr 2023 19:10
 Operator : CG/JU
 Sample : 02158-22
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EB(20230331)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014535.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	29	33	39	rBV	27788	34887	0.88%	0.121%
2	3.734	91	93	100	rVB6	4303	7066	0.18%	0.025%
3	3.846	110	112	127	rBV	31287	77335	1.96%	0.269%
4	4.034	140	144	149	rVB2	12173	17414	0.44%	0.060%
5	4.134	158	161	166	rBV3	9602	13007	0.33%	0.045%
6	4.252	177	181	186	rVB7	7364	10552	0.27%	0.037%
7	5.070	315	320	325	rBV2	8844	15212	0.38%	0.053%
8	6.046	483	486	489	rVB4	2829	3977	0.10%	0.014%
9	6.387	539	544	549	rBV7	6049	10298	0.26%	0.036%
10	7.087	659	663	668	rBV8	2677	4700	0.12%	0.016%
11	7.181	673	679	691	rBV	77524	169095	4.27%	0.587%
12	7.328	697	704	718	rBV	365435	599703	15.16%	2.082%
13	7.534	733	739	755	rBV	342804	601093	15.20%	2.087%
14	8.005	811	819	828	rBV	418373	708203	17.90%	2.459%
15	8.069	828	830	836	rVB7	5059	7460	0.19%	0.026%
16	8.734	934	943	956	rBV	227986	469279	11.86%	1.630%
17	8.852	959	963	971	rVB3	13283	26216	0.66%	0.091%
18	9.181	1012	1019	1036	rBV	448856	776872	19.64%	2.698%
19	9.334	1043	1045	1050	rBV6	2990	4974	0.13%	0.017%
20	9.552	1077	1082	1084	rBV6	3732	4836	0.12%	0.017%
21	9.905	1136	1142	1154	rBV	335340	619026	15.65%	2.150%
22	10.463	1229	1237	1265	rBV	321193	844195	21.34%	2.931%
23	10.822	1291	1298	1311	rVB	578869	969415	24.51%	3.366%
24	10.987	1318	1326	1343	rBV	120137	307401	7.77%	1.067%
25	11.375	1389	1392	1396	rBV4	4682	7242	0.18%	0.025%
26	11.440	1399	1403	1411	rVB6	7254	14101	0.36%	0.049%
27	11.699	1441	1447	1449	rBV7	3260	6394	0.16%	0.022%
28	12.428	1566	1571	1578	rBV8	7309	14789	0.37%	0.051%
29	13.257	1708	1712	1715	rBV6	3633	4900	0.12%	0.017%
30	13.534	1753	1759	1767	rBV2	25589	45037	1.14%	0.156%
31	14.063	1840	1849	1869	rBV	919579	1414462	35.76%	4.912%
32	14.351	1891	1898	1910	rBV2	999188	1565955	39.59%	5.438%
33	14.657	1941	1950	1961	rBV	810570	1261784	31.90%	4.381%
34	14.951	1989	2000	2012	rBV3	24504	102574	2.59%	0.356%
35	15.481	2087	2090	2096	rVB8	5629	6990	0.18%	0.024%
36	15.593	2106	2109	2112	rBV4	4309	4025	0.10%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014535.D
Acq On : 04 Apr 2023 19:10
Operator : CG/JU
Sample : 02158-22
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB(20230331)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	15.651	2112	2119	2133	rBV	1387555	2062380	52.14%	7.162%
38	15.787	2136	2142	2156	rBV	361367	659443	16.67%	2.290%
39	16.010	2177	2180	2184	rVB6	5354	7747	0.20%	0.027%
40	16.540	2268	2270	2275	rVV6	2982	4691	0.12%	0.016%
41	17.416	2413	2419	2430	rBV	1066458	1523385	38.51%	5.290%
42	17.516	2430	2436	2451	rVV2	1764785	2682108	67.80%	9.314%
43	18.292	2564	2568	2570	rBV4	13279	19911	0.50%	0.069%
44	18.357	2576	2579	2583	rBV2	9068	10783	0.27%	0.037%
45	19.322	2741	2743	2750	rVB5	23661	29875	0.76%	0.104%
46	19.745	2810	2815	2824	rBV	2414620	3310645	83.69%	11.496%
47	21.504	3109	3114	3123	rBV	1267779	1846627	46.68%	6.412%
48	23.851	3507	3513	3524	rVB2	1991802	3955743	100.00%	13.736%
49	24.016	3535	3541	3550	rVB2	884100	1934192	48.90%	6.716%




Sum of corrected areas: 28797999

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014535.D
Acq On : 04 Apr 2023 19:10
Operator : CG/JU
Sample : 02158-22
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB(20230331)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

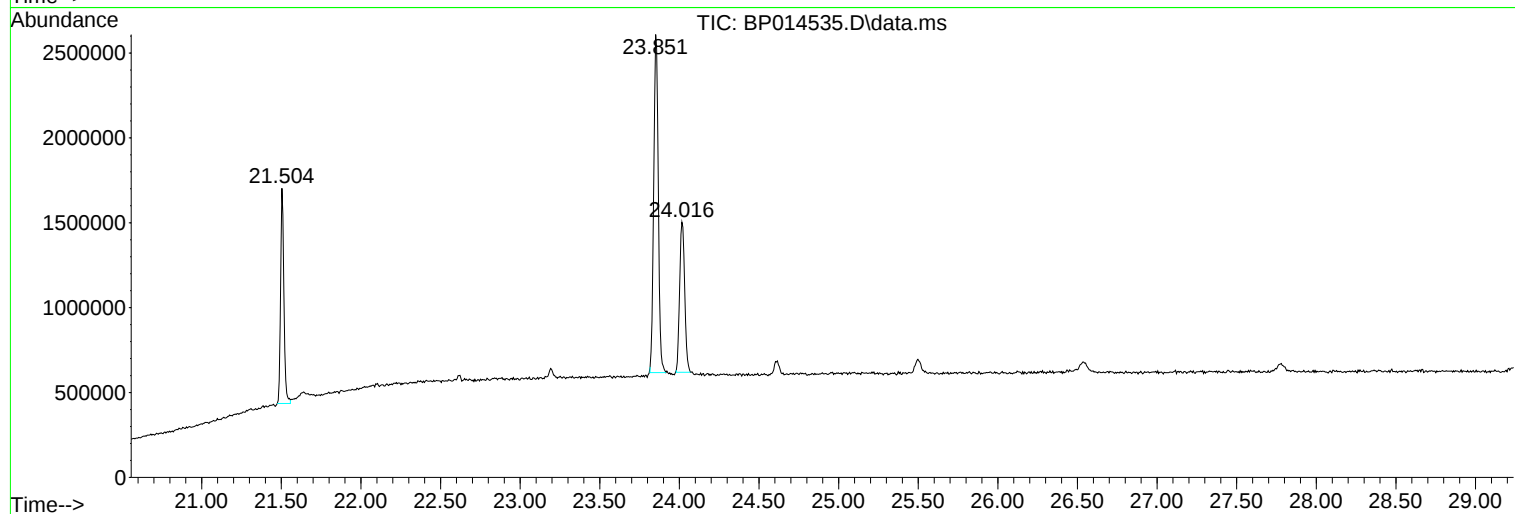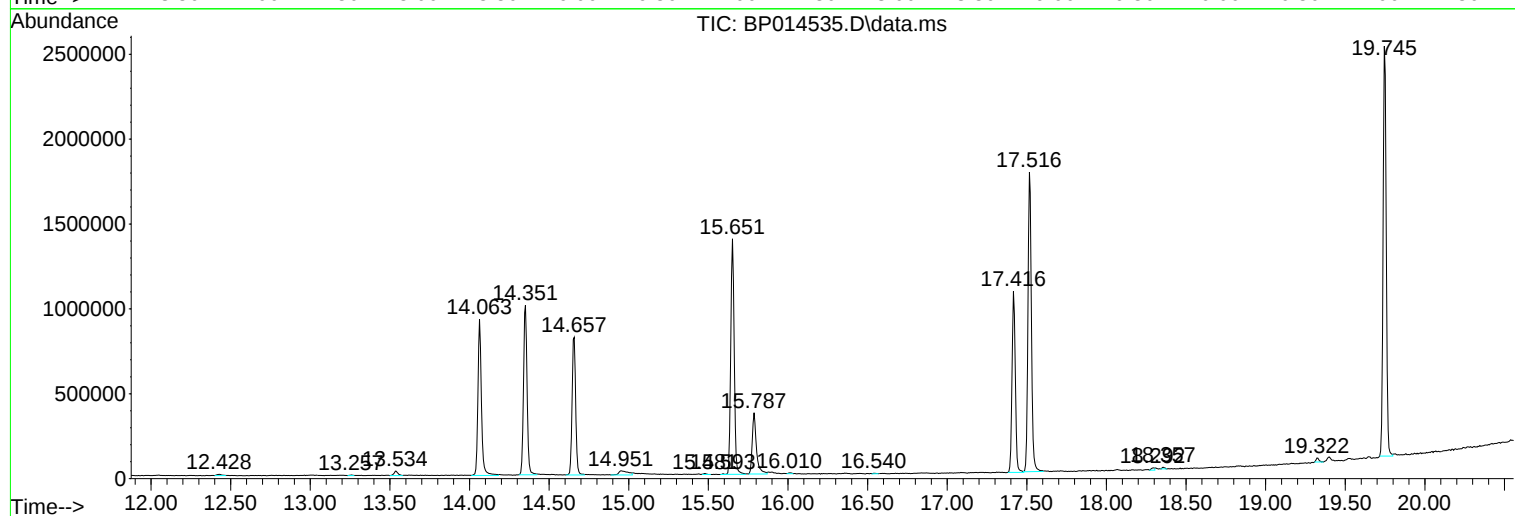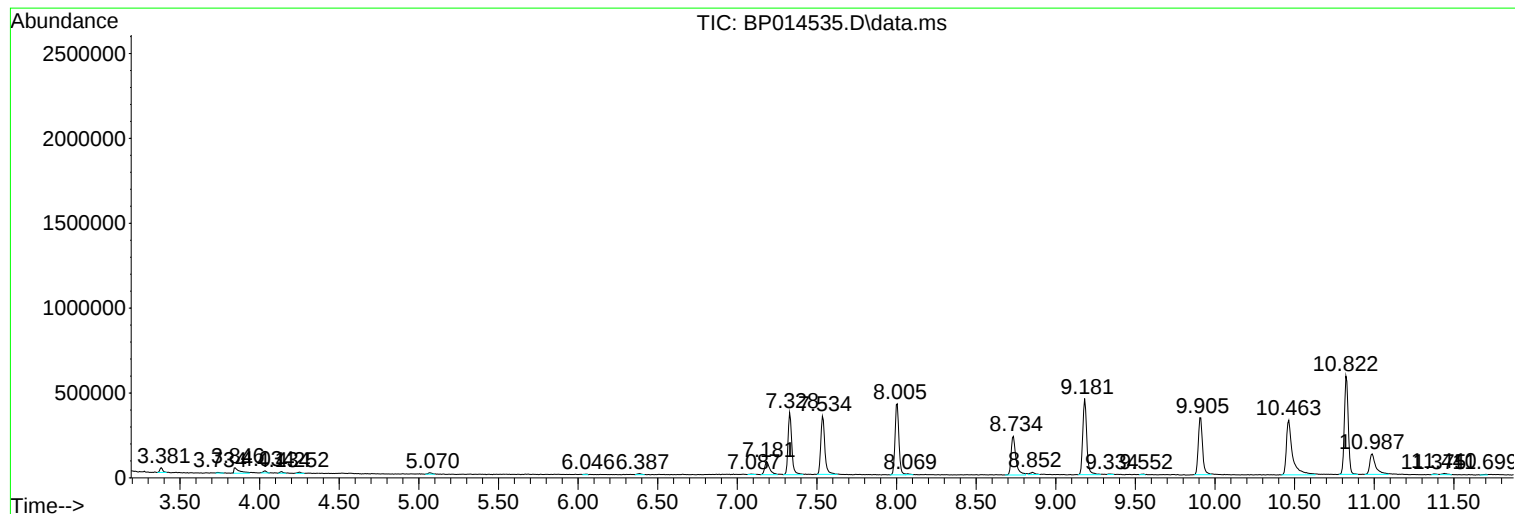

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014535.D
Acq On : 04 Apr 2023 19:10
Operator : CG/JU
Sample : 02158-22
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB(20230331)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014535.D
Acq On : 04 Apr 2023 19:10
Operator : CG/JU
Sample : 02158-22
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EB(20230331)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc