

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014541.D
 Acq On : 04 Apr 2023 22:34
 Operator : CG/JU
 Sample : 02158-24
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MW-1(20230331)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014541.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	30	33	41	rVB	28188	37392	0.84%	0.100%
2	3.828	108	109	125	rBV	91990	173673	3.88%	0.466%
3	4.034	140	144	149	rVB3	12318	19145	0.43%	0.051%
4	4.140	157	162	172	rVB3	10846	19754	0.44%	0.053%
5	4.246	177	180	184	rVB6	7767	11163	0.25%	0.030%
6	5.069	316	320	324	rBV	12803	17068	0.38%	0.046%
7	6.381	538	543	548	rVB5	6676	12238	0.27%	0.033%
8	7.181	673	679	693	rBV2	109047	225354	5.04%	0.605%
9	7.328	698	704	716	rBV	437452	699483	15.64%	1.877%
10	7.534	732	739	753	rVV	447612	765475	17.11%	2.054%
11	7.998	811	818	831	rBV	485927	801204	17.91%	2.150%
12	8.728	936	942	954	rBV	327238	616777	13.79%	1.655%
13	9.181	1012	1019	1034	rBV	541798	955717	21.36%	2.565%
14	9.339	1042	1046	1048	rVV5	2841	4994	0.11%	0.013%
15	9.357	1048	1049	1056	rVB6	3934	6885	0.15%	0.018%
16	9.545	1076	1081	1087	rVB8	6926	14037	0.31%	0.038%
17	9.904	1134	1142	1158	rBV	448225	808550	18.07%	2.170%
18	10.457	1229	1236	1263	rBV	473276	1103958	24.68%	2.962%
19	10.686	1269	1275	1285	rVB	31640	54534	1.22%	0.146%
20	10.822	1290	1298	1309	rBV	684295	1145695	25.61%	3.074%
21	10.975	1317	1324	1345	rBV	424494	928565	20.76%	2.492%
22	11.216	1362	1365	1369	rVB6	4617	5448	0.12%	0.015%
23	11.675	1435	1443	1446	rBV9	5889	11373	0.25%	0.031%
24	12.033	1500	1504	1512	rVB9	4108	8646	0.19%	0.023%
25	12.422	1564	1570	1576	rBV9	9485	22492	0.50%	0.060%
26	12.998	1662	1668	1670	rBV7	3644	6749	0.15%	0.018%
27	13.257	1707	1712	1715	rBV7	5325	8444	0.19%	0.023%
28	13.457	1741	1746	1750	rVB8	4018	6931	0.15%	0.019%
29	13.628	1769	1775	1777	rBV6	2441	4620	0.10%	0.012%
30	13.886	1815	1819	1824	rBV8	4205	6858	0.15%	0.018%
31	14.063	1840	1849	1863	rBV	1242073	1817277	40.62%	4.877%
32	14.169	1866	1867	1872	rVV5	6859	7014	0.16%	0.019%
33	14.251	1876	1881	1883	rBV3	4935	7397	0.17%	0.020%
34	14.351	1891	1898	1911	rBV	1389010	2094009	46.81%	5.619%
35	14.657	1940	1950	1958	rBV	1019458	1579113	35.30%	4.237%
36	14.939	1991	1998	2008	rBV6	41129	141787	3.17%	0.380%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014541.D
 Acq On : 04 Apr 2023 22:34
 Operator : CG/JU
 Sample : 02158-24
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 MW-1(20230331)

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	15.480	2086	2090	2096	rVB2	26408	36589	0.82%	0.098%
38	15.592	2104	2109	2112	rBV6	4232	7488	0.17%	0.020%
39	15.651	2112	2119	2133	rBV	1936124	2690625	60.14%	7.220%
40	15.786	2136	2142	2153	rVV	476602	819006	18.31%	2.198%
41	15.886	2157	2159	2164	rVB5	17203	24262	0.54%	0.065%
42	16.021	2176	2182	2191	rVB	236210	357831	8.00%	0.960%
43	16.345	2233	2237	2245	rBV	53826	84633	1.89%	0.227%
44	16.586	2273	2278	2285	rVB	29799	47584	1.06%	0.128%
45	17.145	2369	2373	2377	rBV	38132	46567	1.04%	0.125%
46	17.416	2413	2419	2430	rBV	1444811	2034197	45.47%	5.459%
47	17.516	2430	2436	2451	rVV2	2261177	3311522	74.02%	8.886%
48	17.880	2496	2498	2504	rVB2	17391	20131	0.45%	0.054%
49	18.063	2527	2529	2534	rVB4	16572	16897	0.38%	0.045%
50	18.286	2564	2567	2573	rBV5	38523	64421	1.44%	0.173%
51	19.321	2741	2743	2748	rVB3	31796	38546	0.86%	0.103%
52	19.515	2774	2776	2784	rBV8	22644	33754	0.75%	0.091%
53	19.745	2810	2815	2823	rBV	3079575	4041496	90.34%	10.845%
54	21.504	3109	3114	3121	rBV	1708576	2413590	53.95%	6.477%
55	23.850	3506	3513	3521	rVB	2295829	4473594	100.00%	12.005%
56	24.015	3534	3541	3551	rVB2	1199094	2553265	57.07%	6.851%




Sum of corrected areas: 37265817

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014541.D
Acq On : 04 Apr 2023 22:34
Operator : CG/JU
Sample : 02158-24
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-1(20230331)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

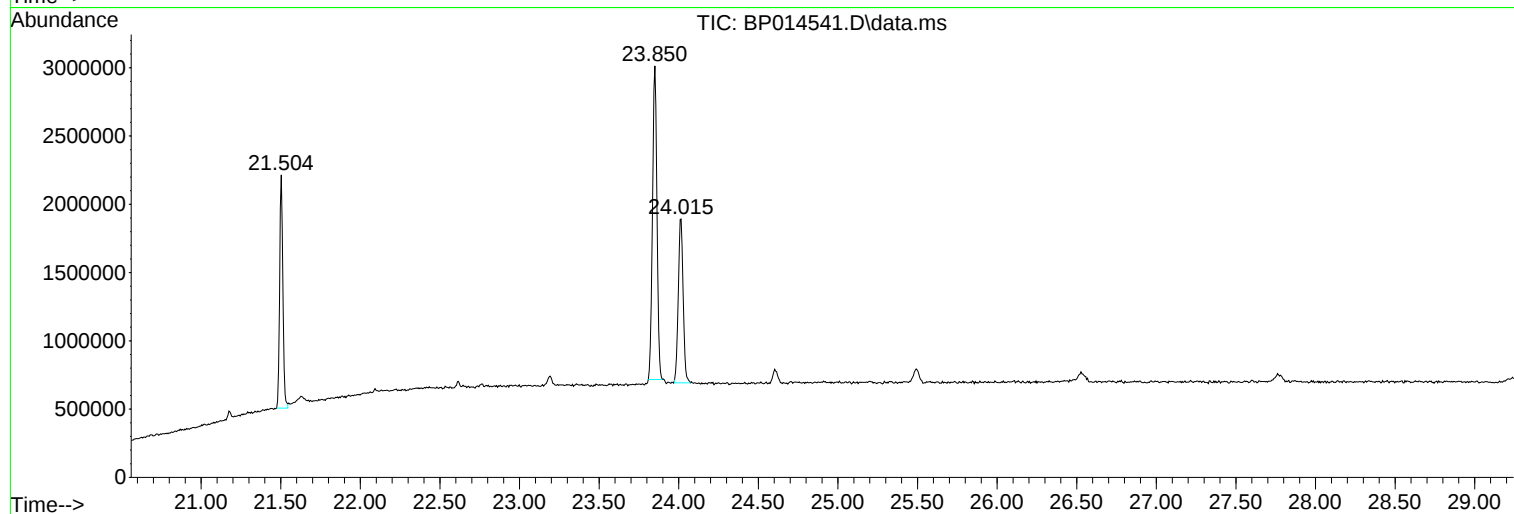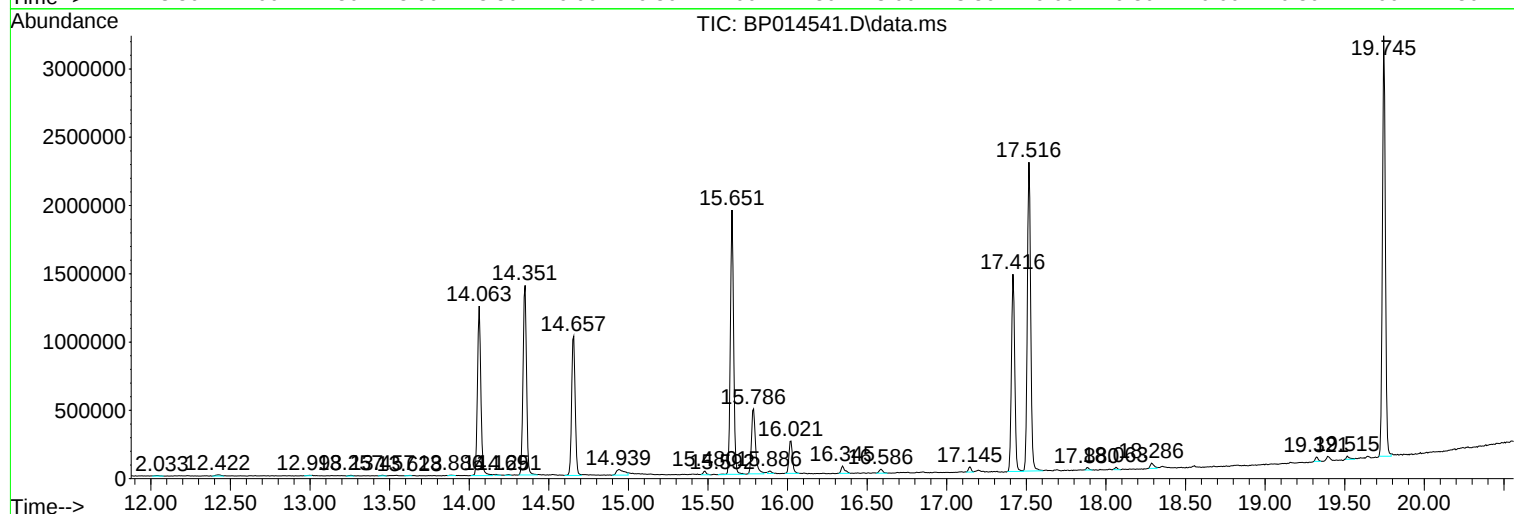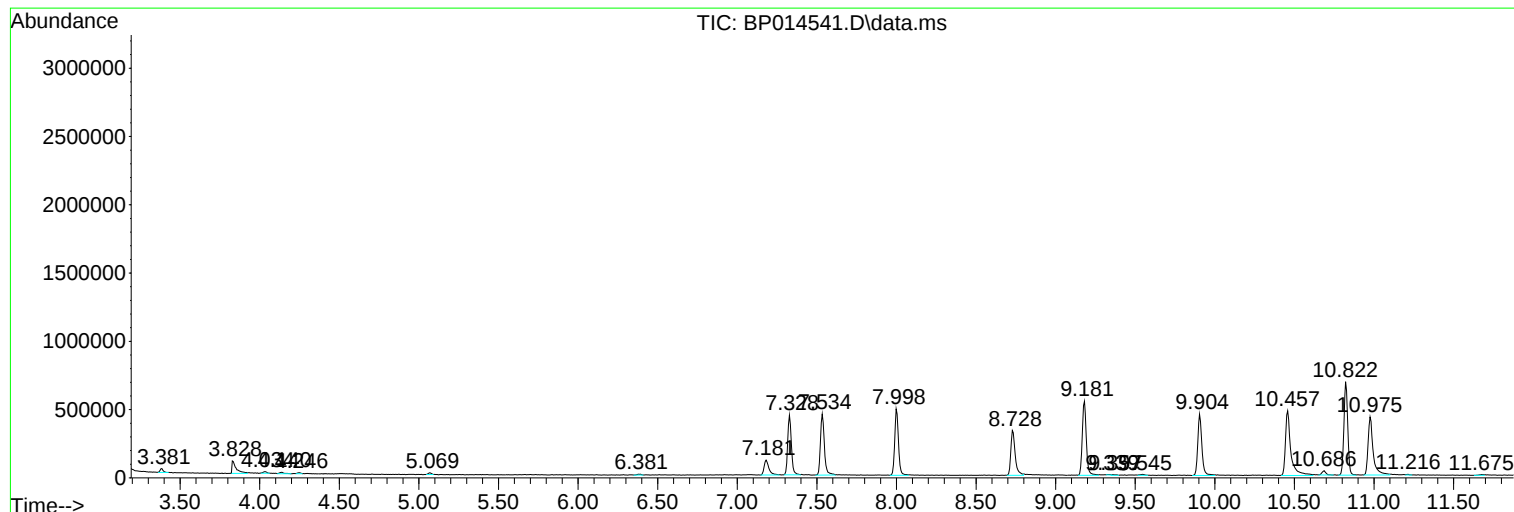

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014541.D
Acq On : 04 Apr 2023 22:34
Operator : CG/JU
Sample : 02158-24
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-1(20230331)










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.022	4.53 ng/ul	357831	Acenaphthene-d10	14.657

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	97
3			Benzophenone	182	C13H10O	000119-61-9	96
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Benzophenone	182	C13H10O	000119-61-9	89

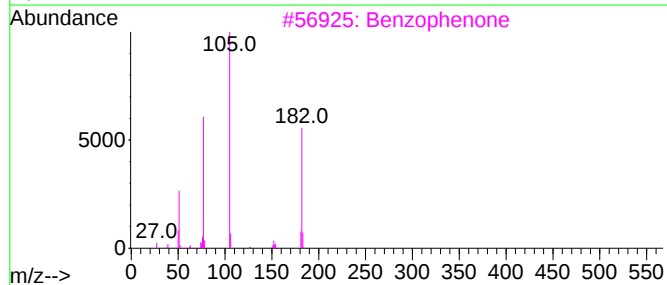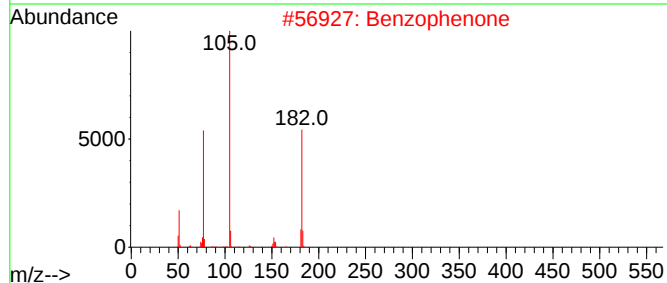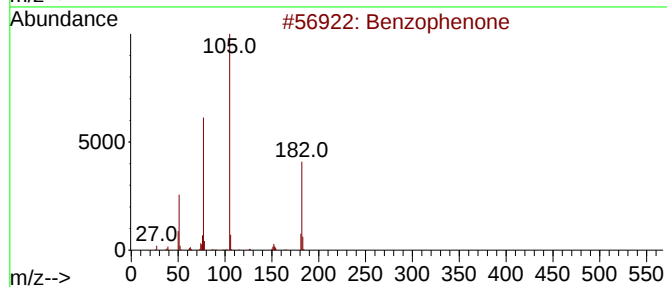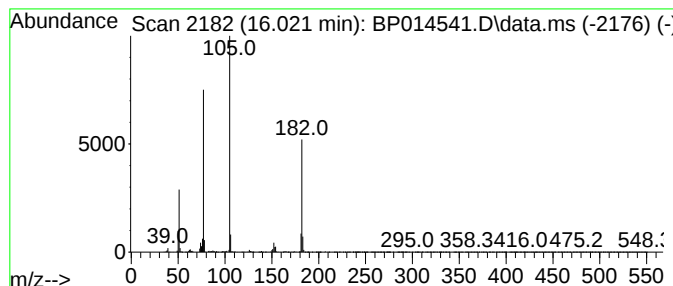

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014541.D
Acq On : 04 Apr 2023 22:34
Operator : CG/JU
Sample : 02158-24
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
MW-1(20230331)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	16.022	4.5	ng/u1	357831	3	14.657	1579110	20.0