

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
 Data File : BP014547.D
 Acq On : 05 Apr 2023 02:32
 Operator : CG/JU
 Sample : PB151869BL
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK869

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.381	29	33	39	rVB	42315	50021	1.22%	0.145%
2	3.811	104	106	125	rBV	395414	701320	17.14%	2.036%
3	4.128	158	160	166	rBV3	8123	12349	0.30%	0.036%
4	7.169	670	677	693	rBV	519711	962285	23.52%	2.793%
5	7.328	698	704	716	rVV	437702	699152	17.09%	2.030%
6	7.528	730	738	752	rBV	560268	973047	23.78%	2.825%
7	7.999	811	818	827	rBV	473524	758894	18.55%	2.203%
8	8.722	933	941	956	rBV	612600	1137310	27.80%	3.301%
9	9.175	1011	1018	1036	rBV	533961	929486	22.72%	2.698%
10	9.904	1135	1142	1153	rBV	436167	789459	19.30%	2.292%
11	10.451	1227	1235	1260	rBV	465739	1123068	27.45%	3.260%
12	10.822	1290	1298	1309	rBV	614224	1061198	25.94%	3.080%
13	10.975	1317	1324	1345	rBV	454504	1031601	25.21%	2.995%
14	11.110	1345	1347	1351	rVB5	4562	5186	0.13%	0.015%
15	12.434	1566	1572	1579	rBV9	7445	17995	0.44%	0.052%
16	14.063	1840	1849	1863	rBV	982892	1568029	38.33%	4.552%
17	14.345	1890	1897	1910	rBV	1210077	1854318	45.32%	5.383%
18	14.651	1942	1949	1961	rBV	879671	1353651	33.09%	3.929%
19	14.904	1986	1992	2017	rBV4	199910	725994	17.74%	2.107%
20	15.581	2103	2107	2111	rBV7	3250	6448	0.16%	0.019%
21	15.651	2112	2119	2136	rVV	1519033	2296272	56.12%	6.666%
22	15.781	2136	2141	2157	rVV	348530	626223	15.31%	1.818%
23	15.892	2157	2160	2172	rVV	13214	32784	0.80%	0.095%
24	17.204	2380	2383	2386	rBV5	4549	6232	0.15%	0.018%
25	17.416	2413	2419	2429	rBV	1150239	1649278	40.31%	4.788%
26	17.516	2429	2436	2447	rBV	1752081	2588041	63.26%	7.513%
27	19.322	2740	2743	2748	rBV4	27360	40077	0.98%	0.116%
28	19.745	2809	2815	2826	rBV	2246041	3211790	78.50%	9.323%
29	21.504	3109	3114	3121	rBV	1340687	1973852	48.24%	5.730%
30	23.845	3505	3512	3527	rVB	1936329	4091366	100.00%	11.877%
31	24.010	3534	3540	3553	rVB	990692	2172361	53.10%	6.306%




Sum of corrected areas: 34449087

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014547.D
Acq On : 05 Apr 2023 02:32
Operator : CG/JU
Sample : PB151869BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK869

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

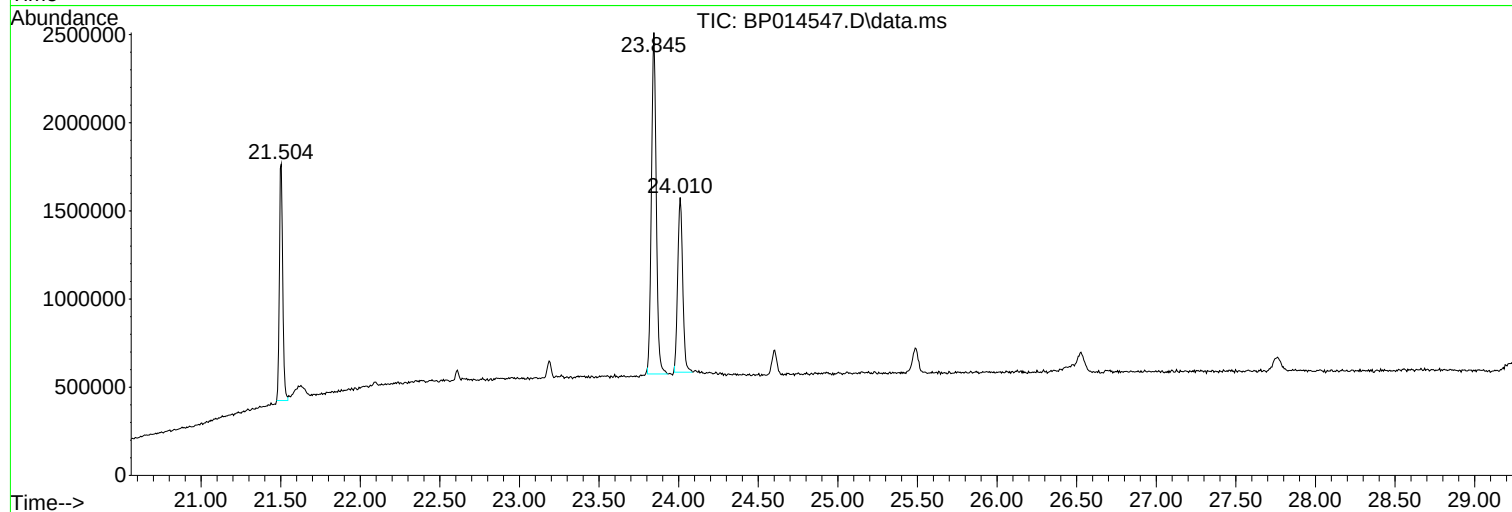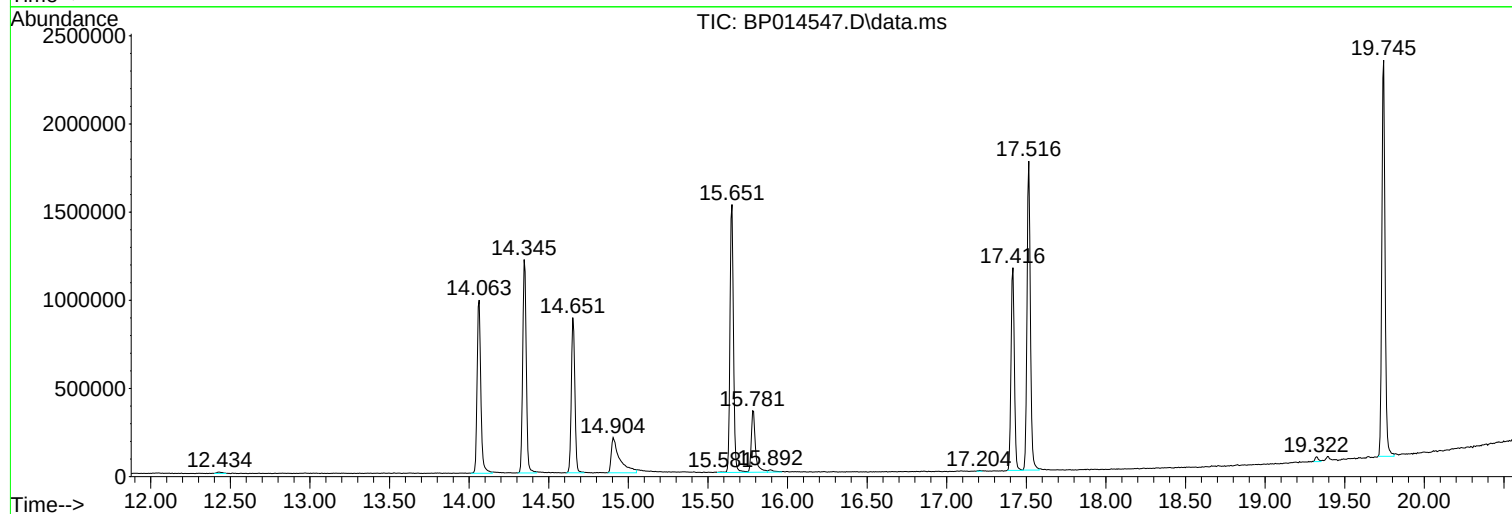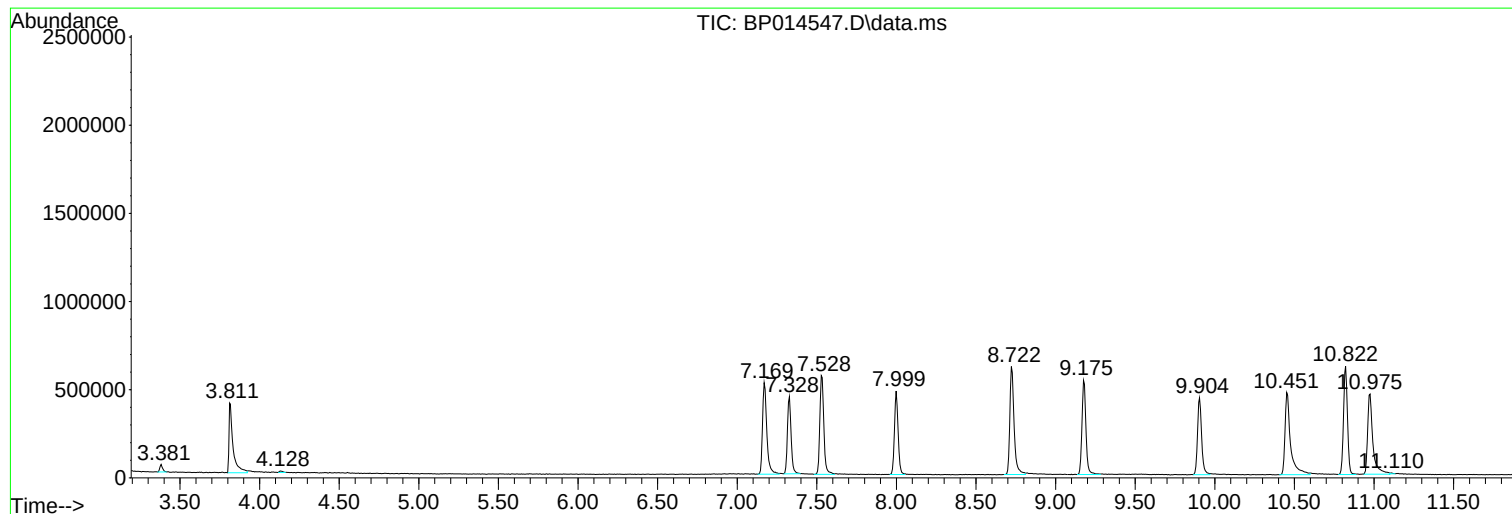

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014547.D
Acq On : 05 Apr 2023 02:32
Operator : CG/JU
Sample : PB151869BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK869

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040323\
Data File : BP014547.D
Acq On : 05 Apr 2023 02:32
Operator : CG/JU
Sample : PB151869BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK869

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------