
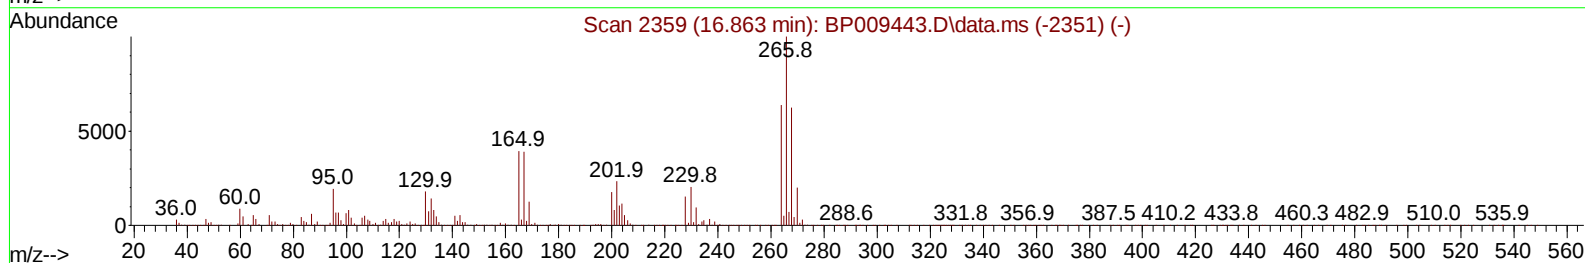
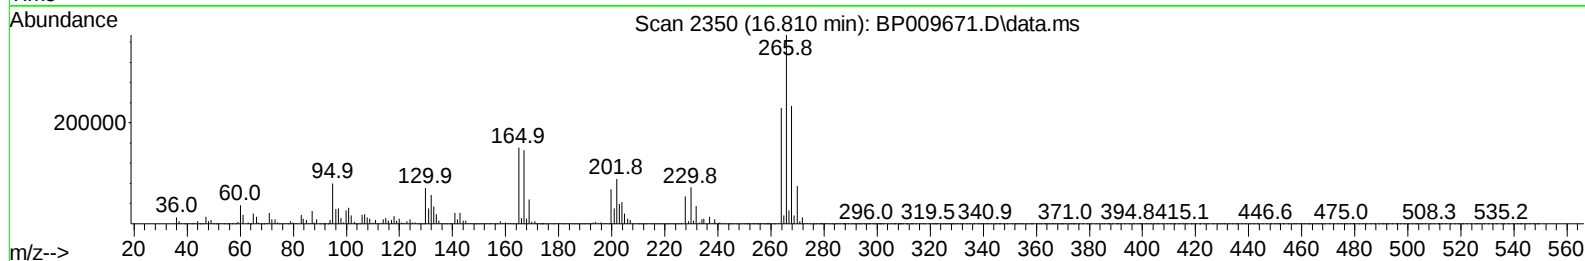


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
Data File : BP009671.D
Acq On : 04 Apr 2022 09:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 00:51:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 31 04:36:51 2022
Response via : Initial Calibration

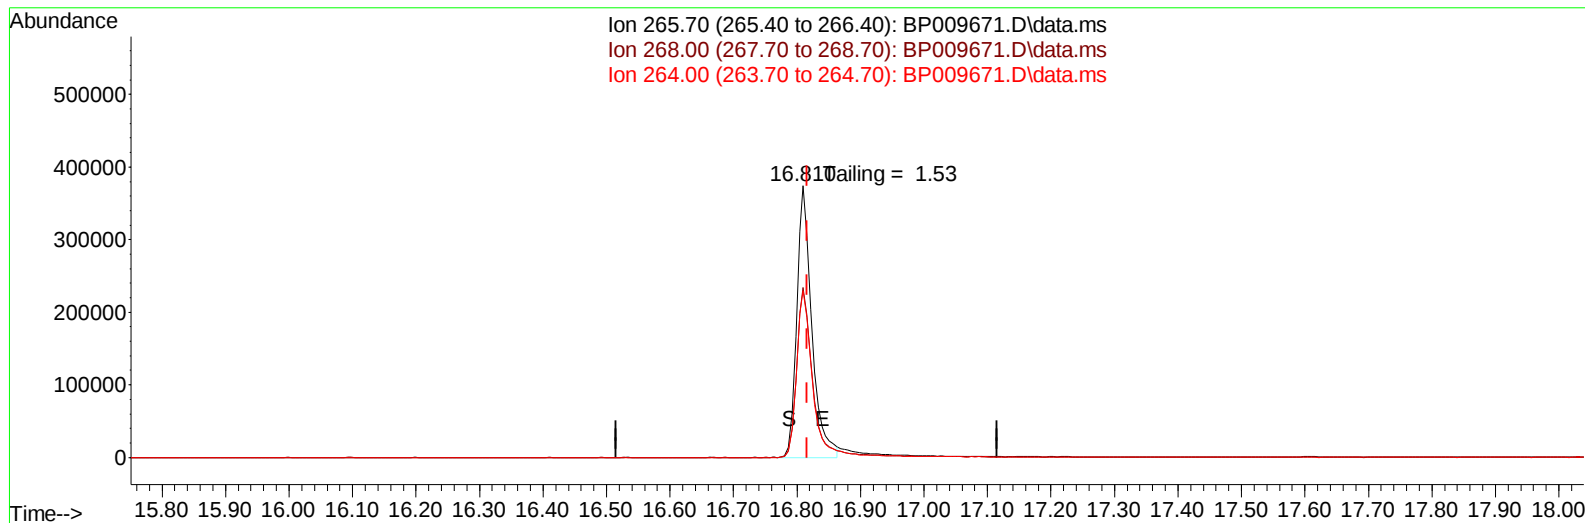




TIC: BP009671.D\data.ms

(70) Pentachlorophenol (C)**16.810min (-0.006) 217141.55 ng****response 665319**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.55
264.00	63.60	61.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
Data File : BP009671.D
Acq On : 04 Apr 2022 09:54
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 00:51:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 31 04:36:51 2022
Response via : Initial Calibration

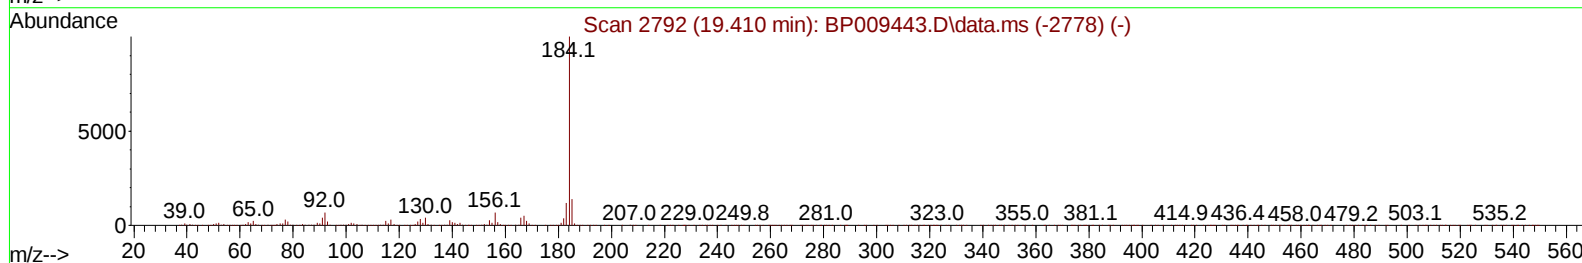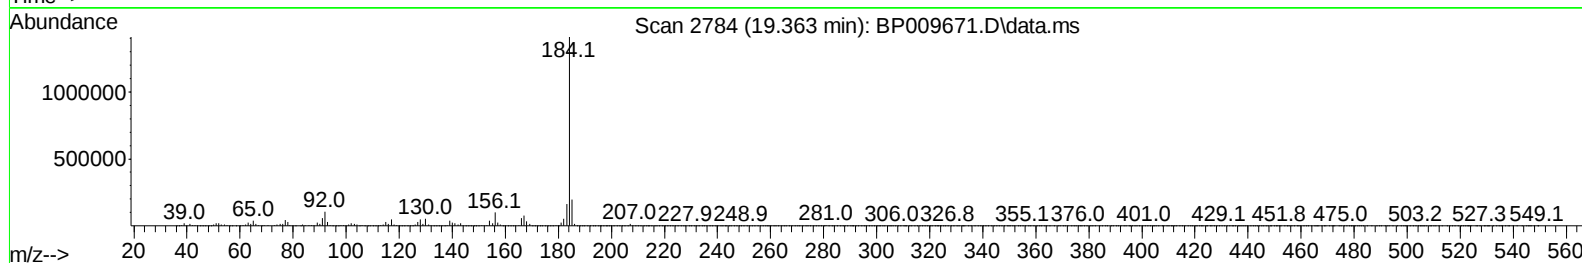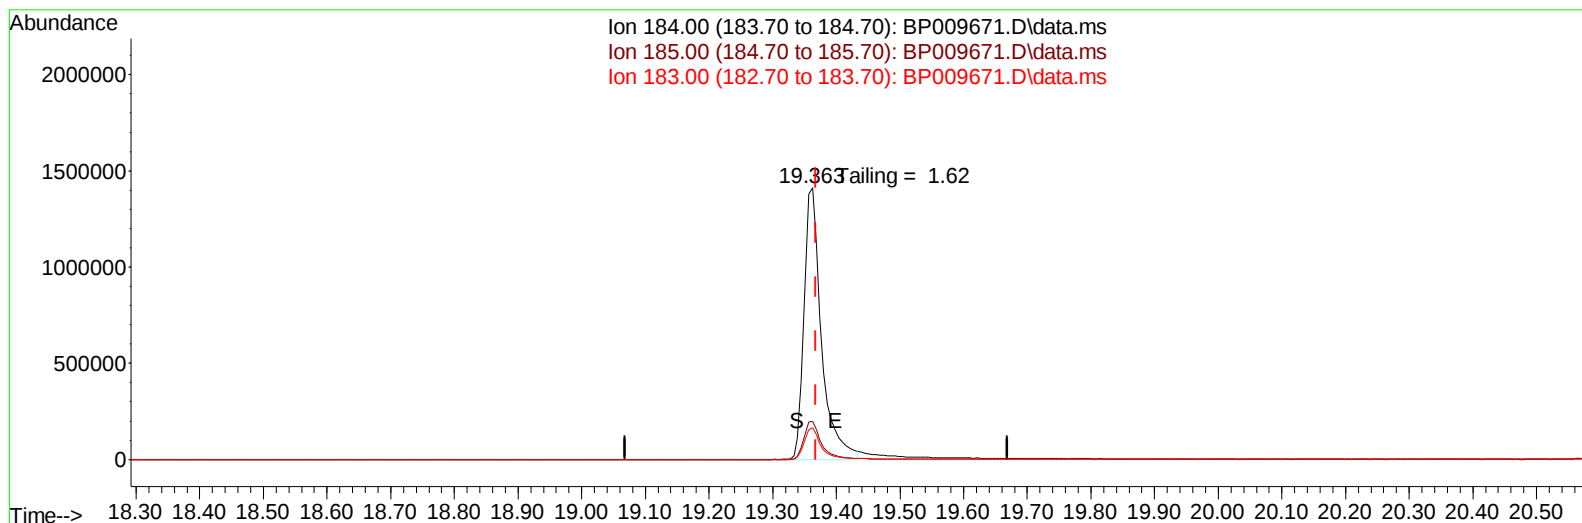

TIC: BP009671.D\data.ms

(77) Benzidine**19.363min (-0.006) 1118826.02 ng****response 2824662**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.98
183.00	11.70	11.66
0.00	0.00	0.00