

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
 Data File : BP009674.D
 Acq On : 04 Apr 2022 12:14
 Operator : CG/JU
 Sample : PB143797BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143797BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009674.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.334	392	399	419	rBV	4304108	7297798	56.38%	11.520%
2	6.922	662	669	693	rBV	3791552	7122665	55.03%	11.244%
3	7.728	799	806	826	rBV	817047	1466165	11.33%	2.315%
4	8.887	994	1003	1025	rBV	2464254	4713933	36.42%	7.441%
5	10.522	1271	1281	1306	rBV	884873	1903024	14.70%	3.004%
6	12.998	1694	1702	1731	rBV	5947030	10262570	79.29%	16.201%
7	14.269	1910	1918	1930	rBV4	29707	132663	1.02%	0.209%
8	14.381	1930	1937	1949	rVV	1277444	2209078	17.07%	3.487%
9	15.881	2185	2192	2217	rBV	3814524	6781608	52.40%	10.706%
10	17.145	2400	2407	2423	rBV	1419516	2434816	18.81%	3.844%
11	19.727	2840	2846	2858	rBV	10068502	12942821	100.00%	20.432%
12	21.263	3102	3107	3118	rBV	1803034	2785342	21.52%	4.397%
13	21.380	3123	3127	3131	rBV	233219	335734	2.59%	0.530%
14	23.639	3505	3511	3524	rVB2	1365106	2958440	22.86%	4.670%

Sum of corrected areas: 63346657

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
Data File : BP009674.D
Acq On : 04 Apr 2022 12:14
Operator : CG/JU
Sample : PB143797BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143797BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.380	2.41 ng	335734	Chrysene-d12	21.263

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	95
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	52
3			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	45
4			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
5			2-Phenyl-6-(trifluoromethyl)-1H-...	277	C15H10F3NO	1000387-59-3	37

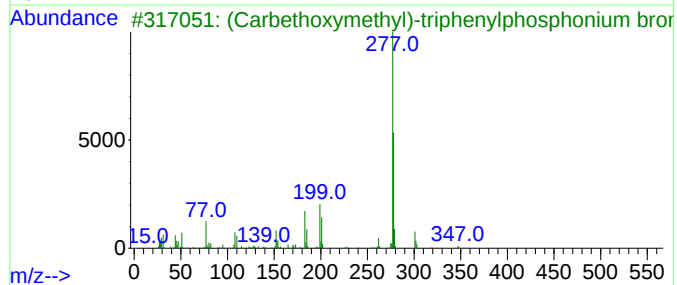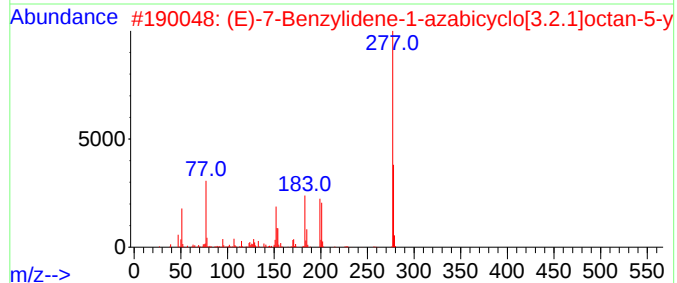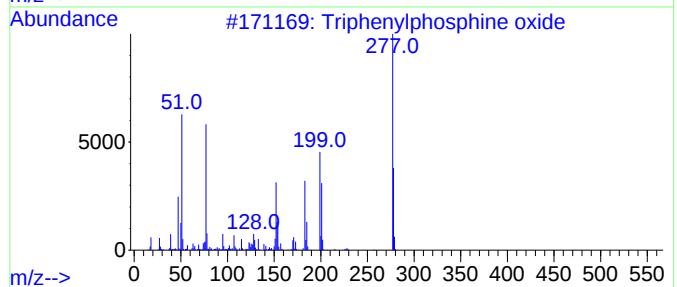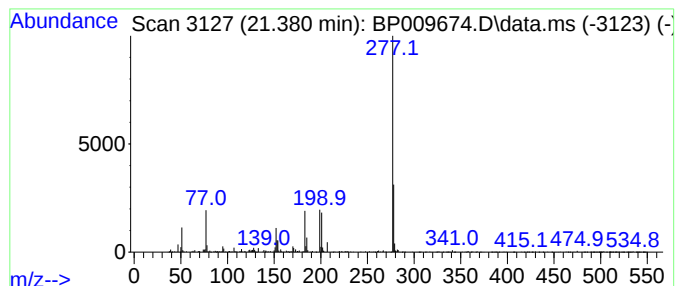

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
Data File : BP009674.D
Acq On : 04 Apr 2022 12:14
Operator : CG/JU
Sample : PB143797BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143797BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	21.380	2.4	ng	335734	5	21.263	2785340	20.0