

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
 Data File : BP009685.D
 Acq On : 04 Apr 2022 18:41
 Operator : CG/JU
 Sample : N2226-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PFS-TP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009685.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.334	392	399	417	rBV	3384816	5882615	45.99%	9.012%
2	6.922	661	669	698	rBV	3133496	6055411	47.34%	9.277%
3	7.722	797	805	816	rBV	713924	1304081	10.20%	1.998%
4	8.881	994	1002	1028	rBV	1936782	3949764	30.88%	6.051%
5	10.516	1271	1280	1297	rBV	940221	1854040	14.50%	2.840%
6	12.993	1693	1701	1717	rBV	5263621	8590957	67.17%	13.161%
7	14.251	1908	1915	1920	rBV2	53604	146480	1.15%	0.224%
8	14.375	1929	1936	1956	rVB	1531574	2531516	19.79%	3.878%
9	15.881	2184	2192	2220	rBV	4151376	7218048	56.43%	11.058%
10	17.139	2400	2406	2421	rBV	1815494	3076056	24.05%	4.712%
11	18.051	2553	2561	2570	rBV2	135925	292064	2.28%	0.447%
12	19.169	2746	2751	2757	rBV	172259	270017	2.11%	0.414%
13	19.522	2807	2811	2821	rVB	214412	345577	2.70%	0.529%
14	19.722	2839	2845	2859	rBV	9724383	12790703	100.00%	19.595%
15	20.974	3054	3058	3068	rBV2	635306	871068	6.81%	1.334%
16	21.257	3101	3106	3111	rBV	2412697	3497370	27.34%	5.358%
17	21.374	3121	3126	3141	rBV	1951135	3094009	24.19%	4.740%
18	23.633	3503	3510	3525	rVB2	1537142	3506012	27.41%	5.371%




Sum of corrected areas: 65275788

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
Data File : BP009685.D
Acq On : 04 Apr 2022 18:41
Operator : CG/JU
Sample : N2226-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PFS-TP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

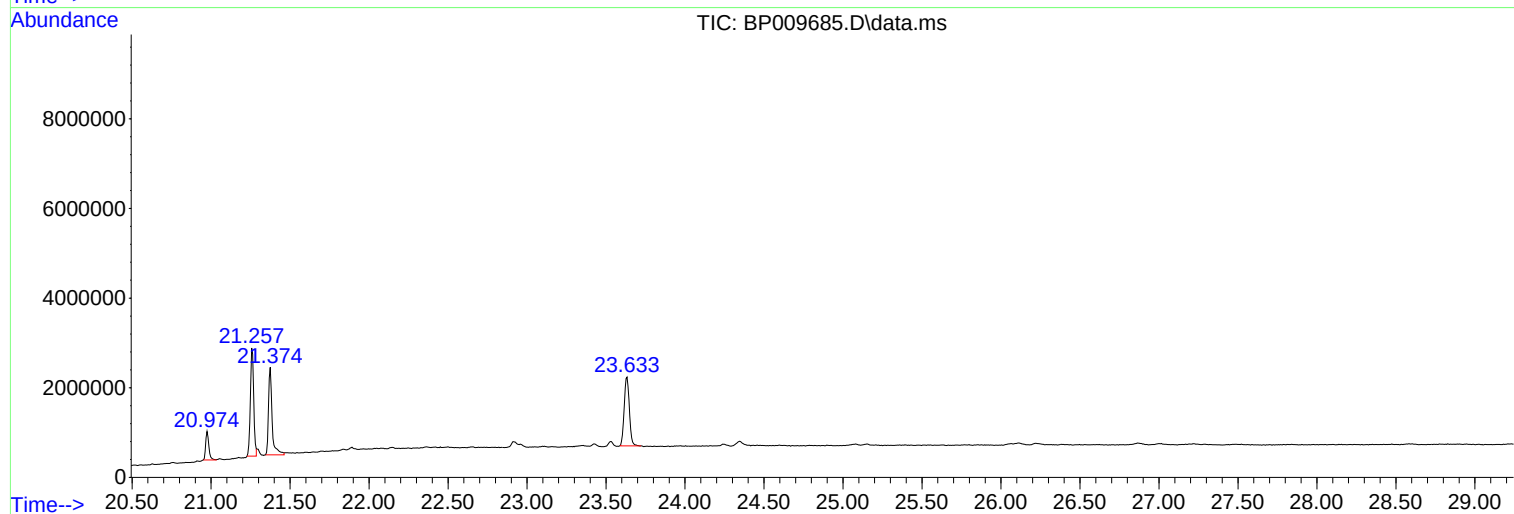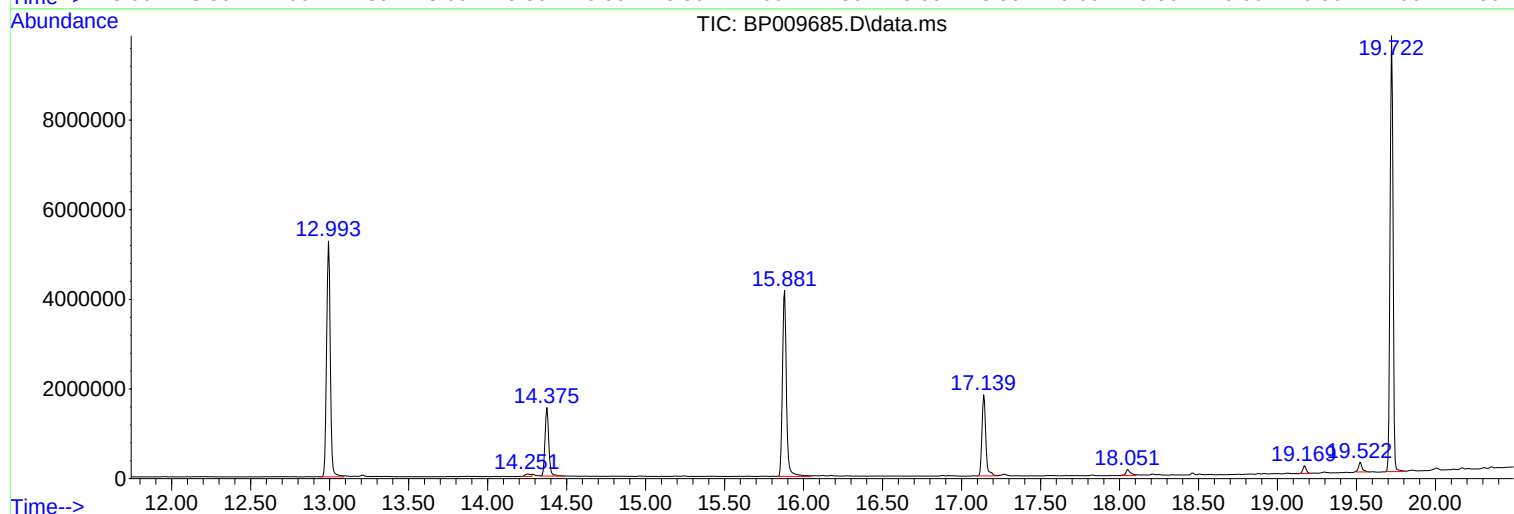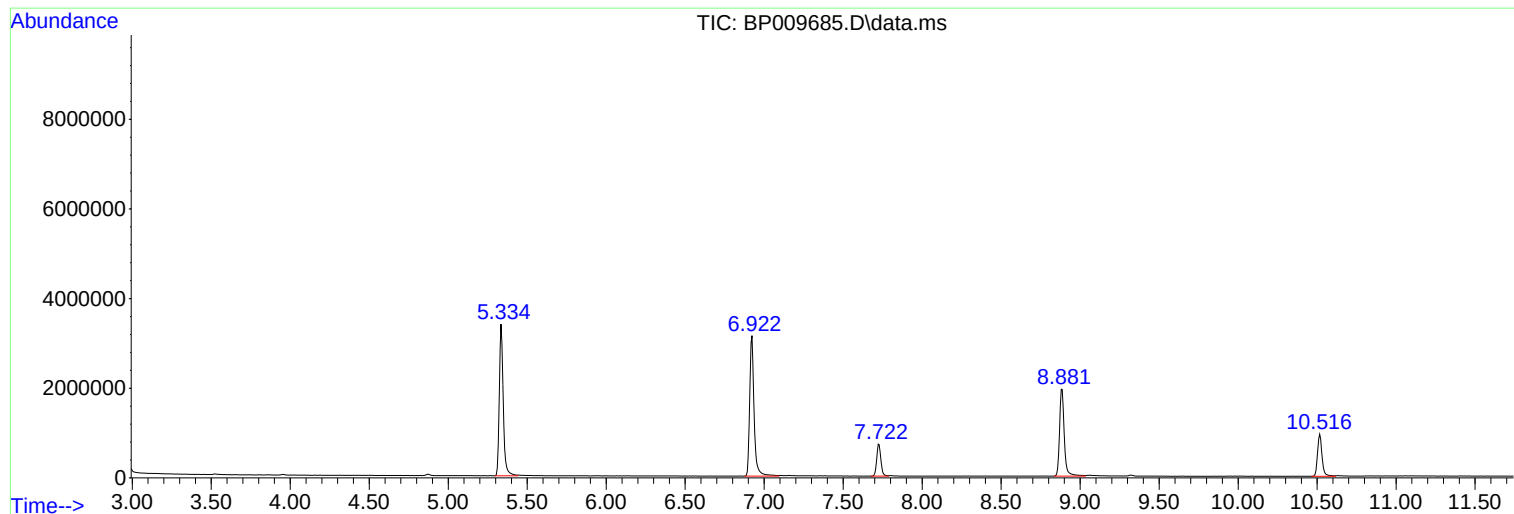

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
Data File : BP009685.D
Acq On : 04 Apr 2022 18:41
Operator : CG/JU
Sample : N2226-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PFS-TP










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Heneicosanol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.974	4.98 ng	871068	Chrysene-d12	21.257

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Heneicosanol	312	C21H44O	015594-90-8	95
2			n-Nonadecanol-1	284	C19H40O	001454-84-8	95
3			Carbonic acid, octadecyl 2,2,2-t...	444	C21H39Cl3O3	1000314-56-3	94
4			Pentacos-1-ene	350	C25H50	016980-85-1	94
5			Heptafluorobutyric acid, n-tetra...	410	C18H29F7O2	007365-36-8	94

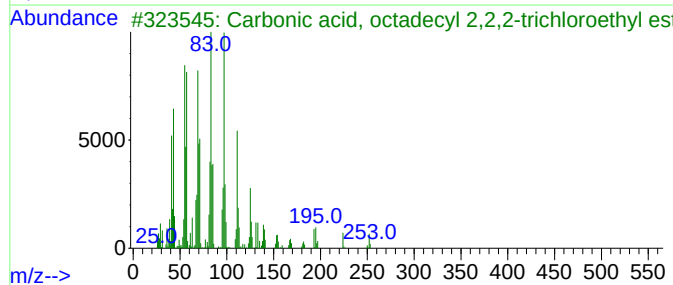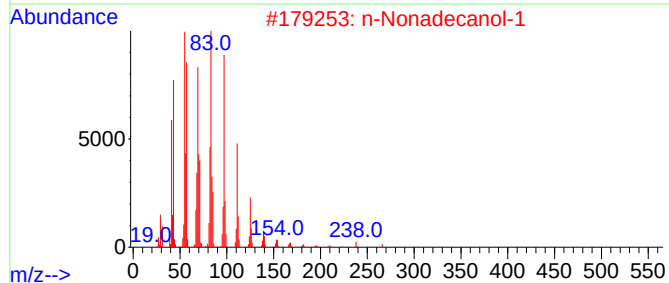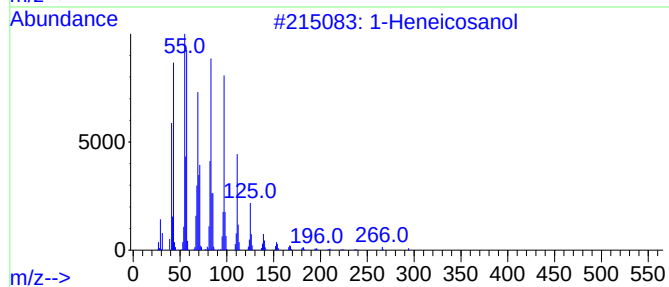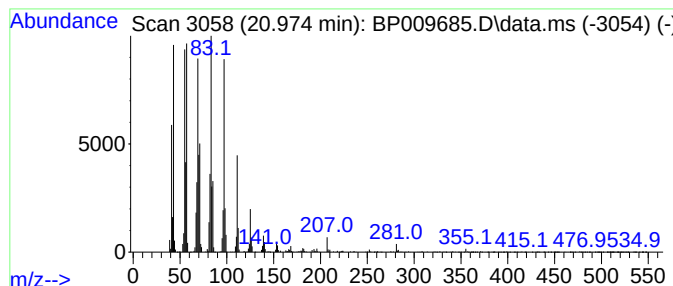

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
Data File : BP009685.D
Acq On : 04 Apr 2022 18:41
Operator : CG/JU
Sample : N2226-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PFS-TP










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.374	17.69 ng	3094010	Chrysene-d12	21.257

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	94
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	91
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
4			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	25
5			3-(3,4-Dichlorophenyl)-2-thioxo-...	277	C9H5Cl2NOS2	017046-34-3	25

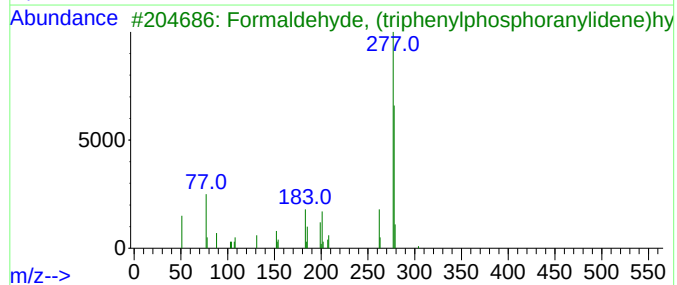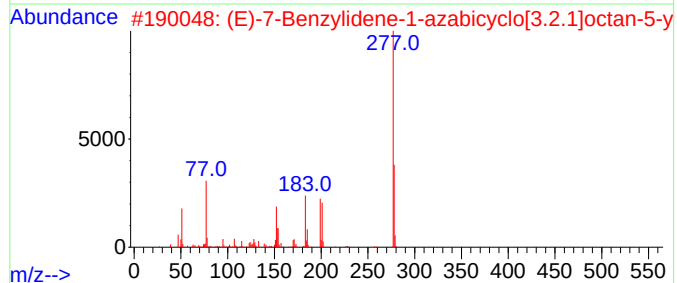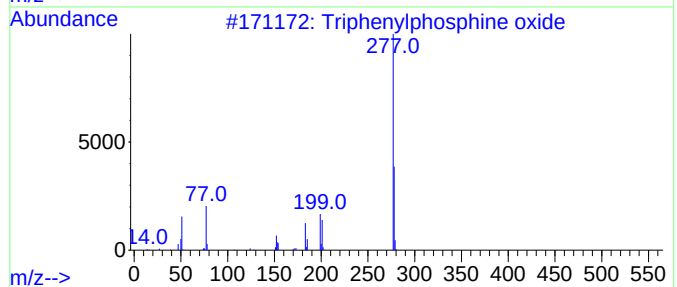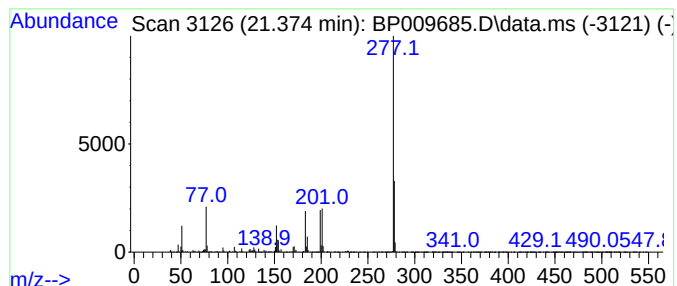

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
Data File : BP009685.D
Acq On : 04 Apr 2022 18:41
Operator : CG/JU
Sample : N2226-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PFS-TP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Heneicosanol	20.974	5.0	ng	871068	5	21.257	3497370	20.0
Triphenylphosph...	21.374	17.7	ng	3094010	5	21.257	3497370	20.0