

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
 Data File : BP009690.D
 Acq On : 04 Apr 2022 21:30
 Operator : CG/JU
 Sample : N2241-01 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CL-02-040122

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009690.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.340	394	400	418	rBV	262038	547454	15.36%	2.173%
2	6.934	664	671	693	rBV2	199363	546476	15.33%	2.169%
3	7.728	798	806	823	rBV	753251	1417790	39.78%	5.628%
4	8.893	997	1004	1023	rBV	137109	378113	10.61%	1.501%
5	10.516	1271	1280	1301	rBV	1001279	2003928	56.23%	7.954%
6	12.993	1693	1701	1716	rBV	495074	919822	25.81%	3.651%
7	14.098	1882	1889	1899	rBV	50054	98376	2.76%	0.390%
8	14.251	1907	1915	1928	rBV3	62551	230594	6.47%	0.915%
9	14.375	1929	1936	1944	rBV	1528757	2524765	70.84%	10.022%
10	15.434	2112	2116	2129	rVB3	18702	44782	1.26%	0.178%
11	15.881	2186	2192	2205	rBV	340178	648010	18.18%	2.572%
12	17.139	2400	2406	2411	rBV	1848409	2937389	82.42%	11.660%
13	17.181	2411	2413	2420	rVB	185238	274788	7.71%	1.091%
14	17.281	2426	2430	2437	rVB	57423	97241	2.73%	0.386%
15	18.022	2552	2556	2559	rBV2	26181	39446	1.11%	0.157%
16	18.069	2561	2564	2570	rVB2	33803	55909	1.57%	0.222%
17	18.204	2583	2587	2591	rBV2	56446	94969	2.66%	0.377%
18	19.169	2746	2751	2758	rBV	440623	660530	18.53%	2.622%
19	19.522	2803	2811	2820	rBV	409389	771382	21.64%	3.062%
20	19.722	2840	2845	2852	rBV	1023488	1316711	36.95%	5.227%
21	20.110	2908	2911	2915	rBV	60210	76315	2.14%	0.303%
22	21.257	3101	3106	3111	rBV	2573982	3563875	100.00%	14.146%
23	21.369	3121	3125	3140	rBV	1406639	2391817	67.11%	9.494%
24	23.633	3503	3510	3527	rVB2	1583965	3552392	99.68%	14.101%

Sum of corrected areas: 25192874

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
Data File : BP009690.D
Acq On : 04 Apr 2022 21:30
Operator : CG/JU
Sample : N2241-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-040122










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.369	13.42 ng	2391820	Chrysene-d12	21.257

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	91
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	90
3			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	64
4			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	50
5			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	25

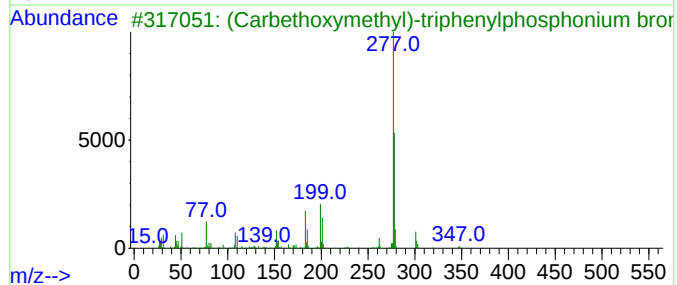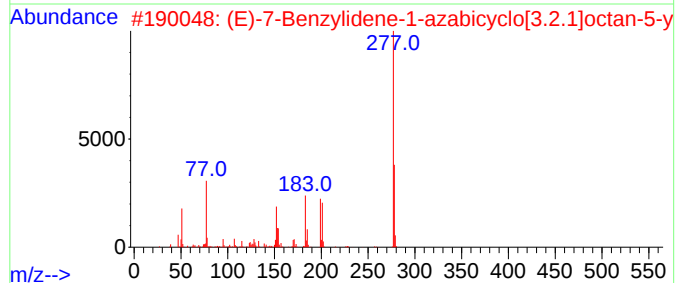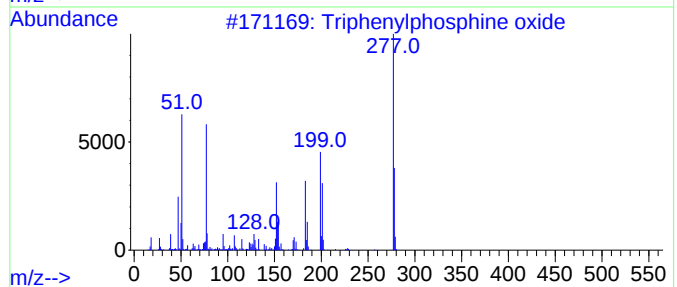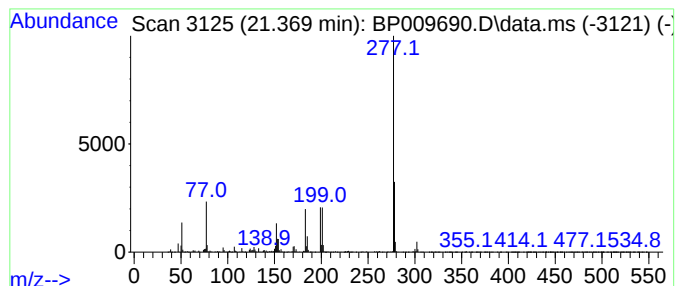

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
Data File : BP009690.D
Acq On : 04 Apr 2022 21:30
Operator : CG/JU
Sample : N2241-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CL-02-040122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	21.369	13.4	ng	2391820	5	21.257	3563880	20.0