
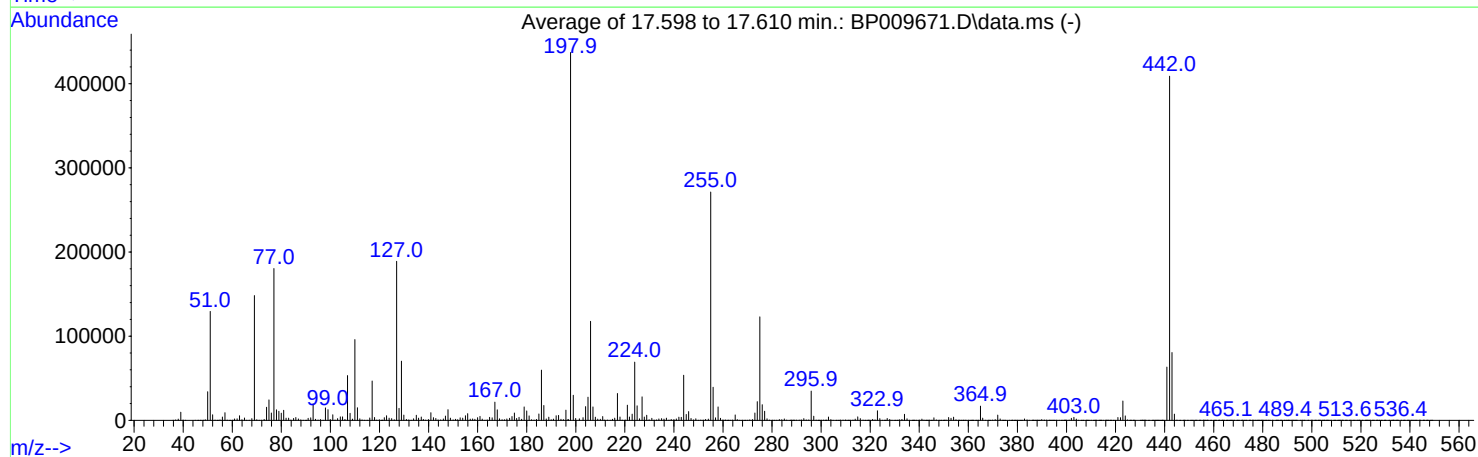


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
 Data File : BP009671.D
 Acq On : 04 Apr 2022 09:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 05 13:35:48 2022

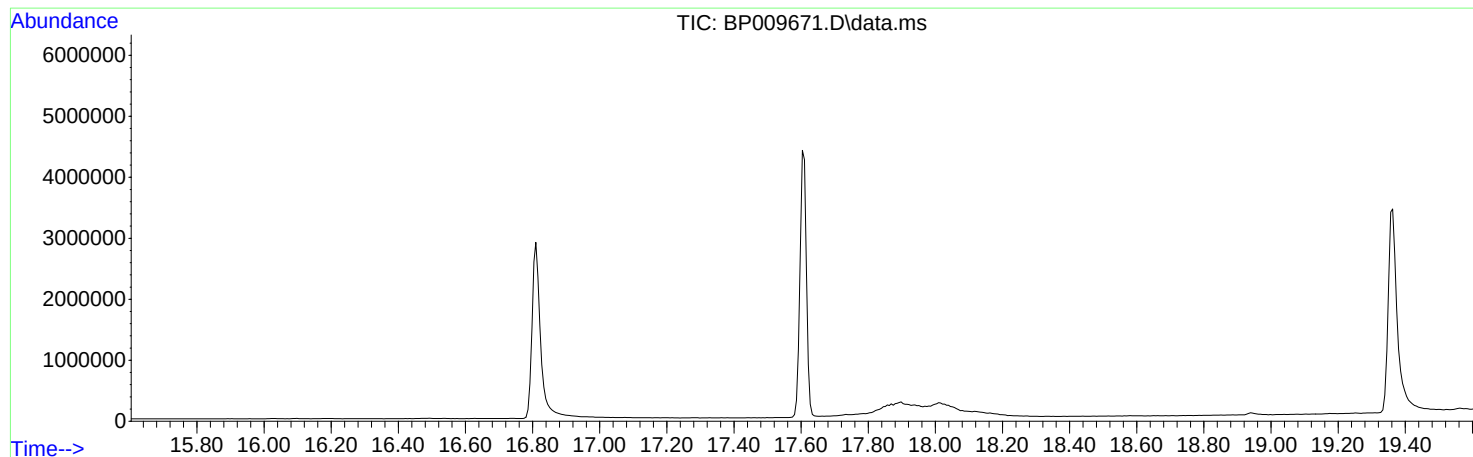




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	129393	PASS
68	69	0.00	2	1.5	2170	PASS
69	198	0.00	100	33.9	148375	PASS
70	69	0.00	2	0.5	698	PASS
127	198	10	80	43.2	188964	PASS
197	198	0.00	2	0.3	1247	PASS
198	198	100	100	100.0	437113	PASS
199	198	5	9	6.8	29853	PASS
275	198	10	60	28.2	123077	PASS
365	198	1	100	3.9	16851	PASS
441	198	0.01	100	14.5	63259	PASS
442	442	100	100	100.0	408939	PASS
443	442	15	24	19.7	80632	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
Data File : BP009671.D
Acq On : 04 Apr 2022 09:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 05 00:51:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 31 04:36:51 2022
Response via : Initial Calibration

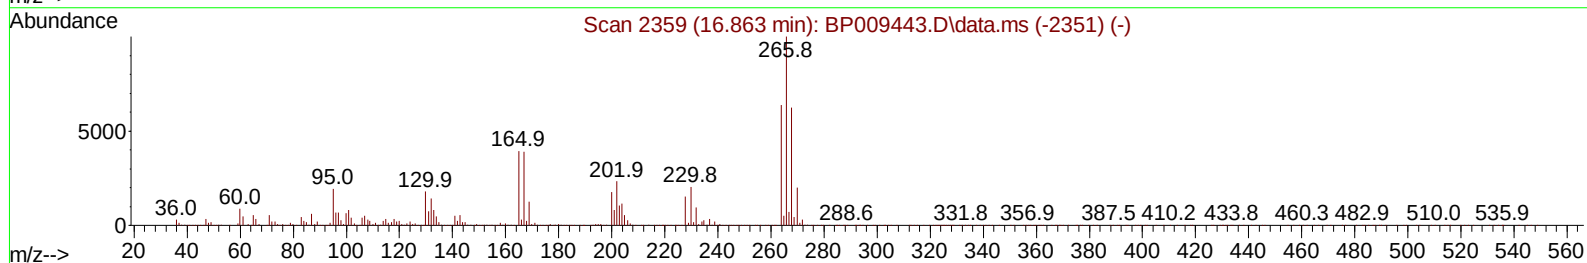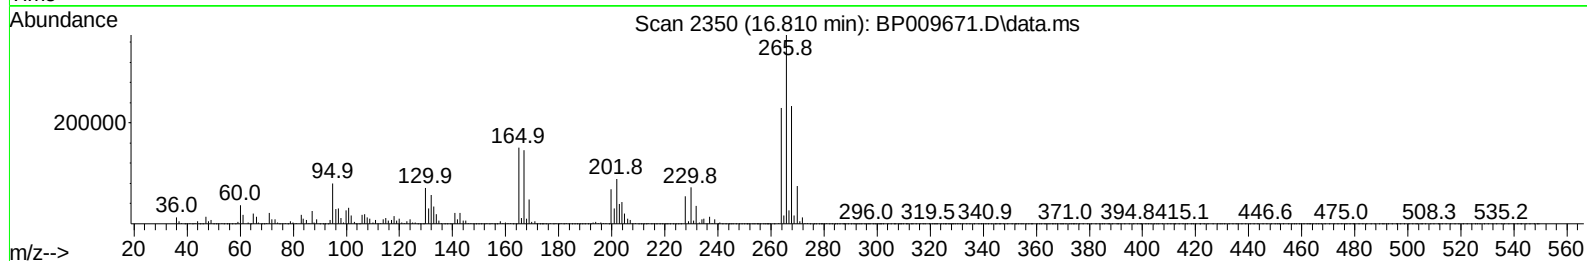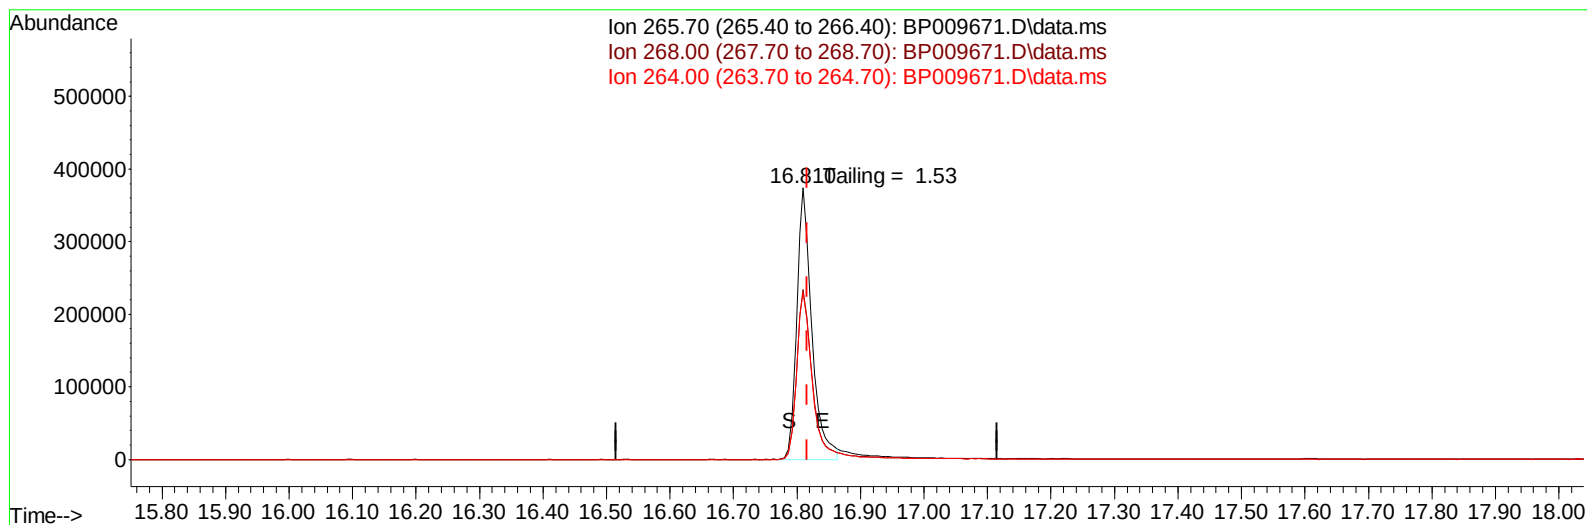

TIC: BP009671.D\data.ms

(70) Pentachlorophenol (C)

16.810min (-0.006) 217141.55 ng




response 665319

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.55
264.00	63.60	61.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040422\
Data File : BP009671.D
Acq On : 04 Apr 2022 09:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 05 00:51:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 31 04:36:51 2022
Response via : Initial Calibration

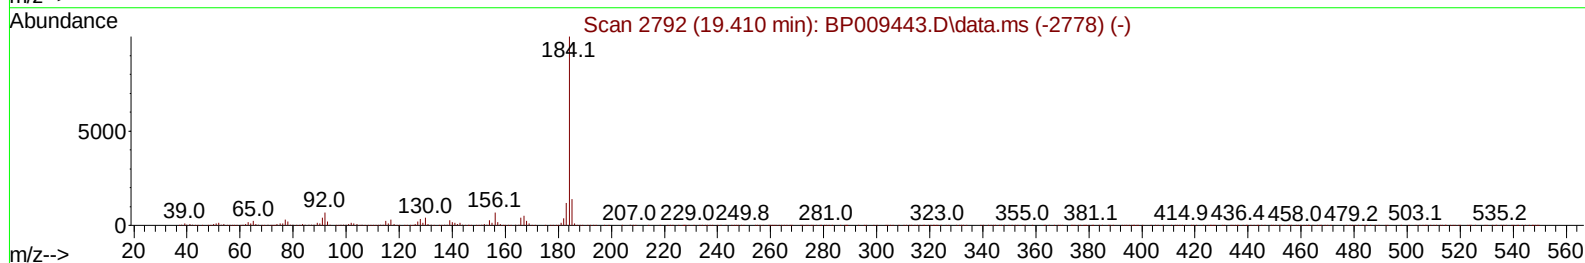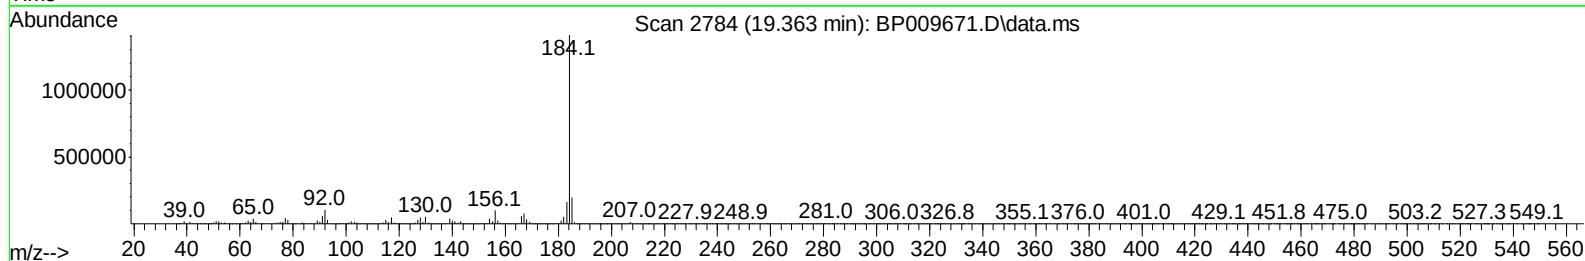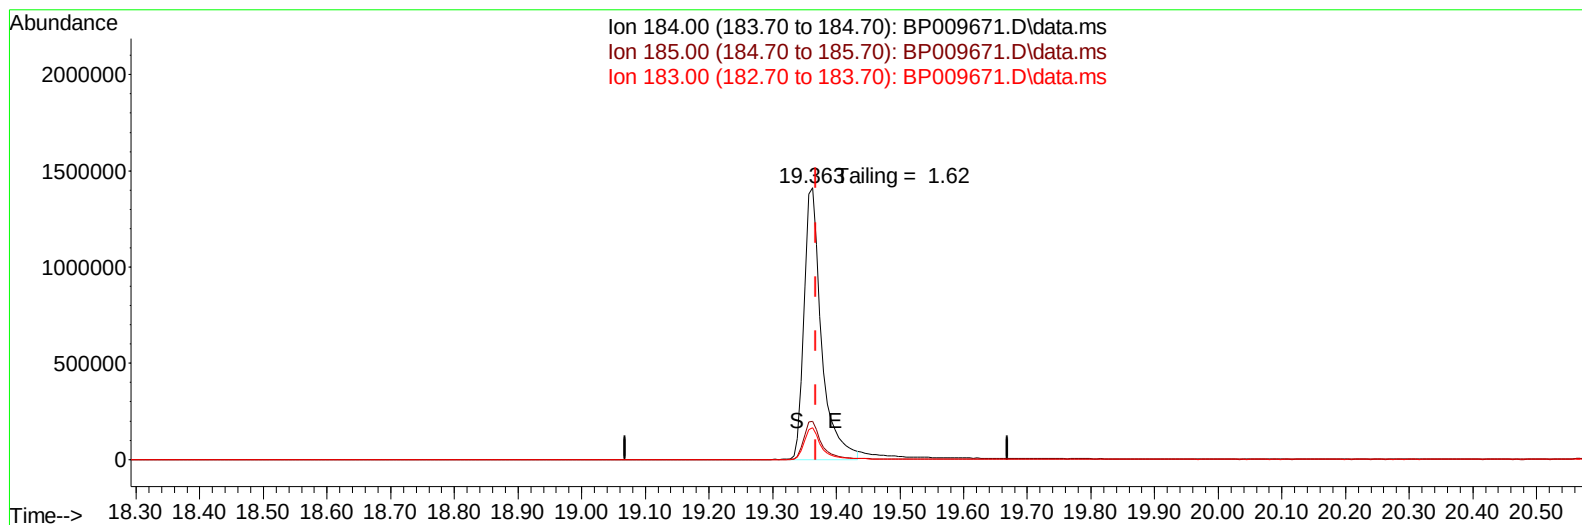

TIC: BP009671.D\data.ms

(77) Benzidine

19.363min (-0.006) 1118826.02 ng

response 2824662

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.98
183.00	11.70	11.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/4/2022	BNA_P	<u>BP009671.D</u>
Compound Name	Response	Retention Time
DDT	1570792	20.568
DDD	58763	20.139
DDE	6425	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
65188	1635980	3.98

Instrument :
BNA_P
ClientSampleId :
DFTPP