




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014571.D
Acq On : 05 Apr 2023 23:21
Operator : CG/JU
Sample : PB151872BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK872

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/06/2023
Supervised By :Jagrut Upadhyay 04/06/2023

Quant Time: Apr 06 01:01:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 06 00:55:13 2023
Response via : Initial Calibration

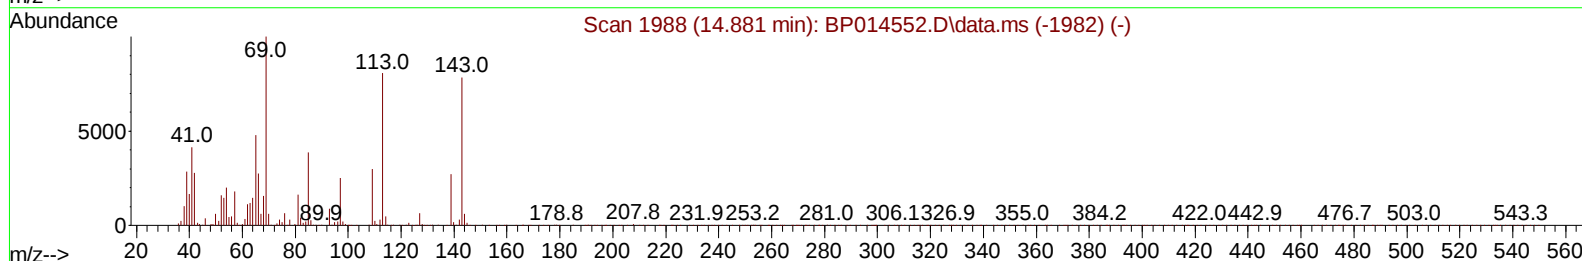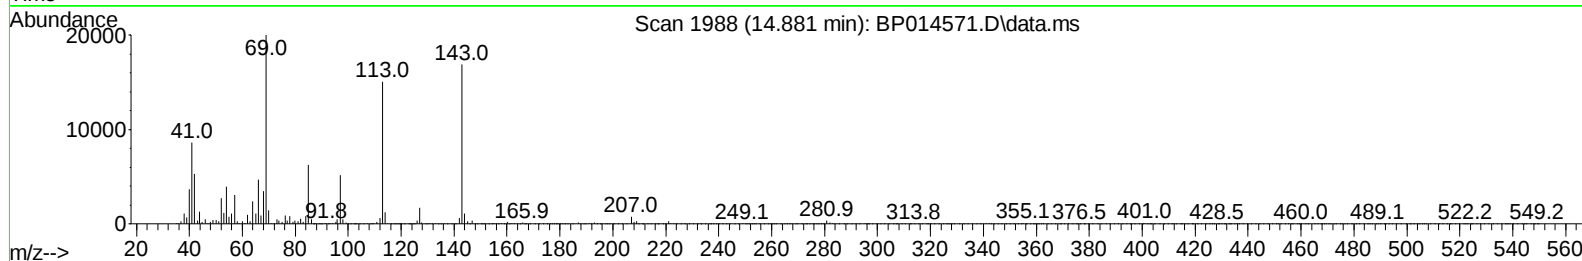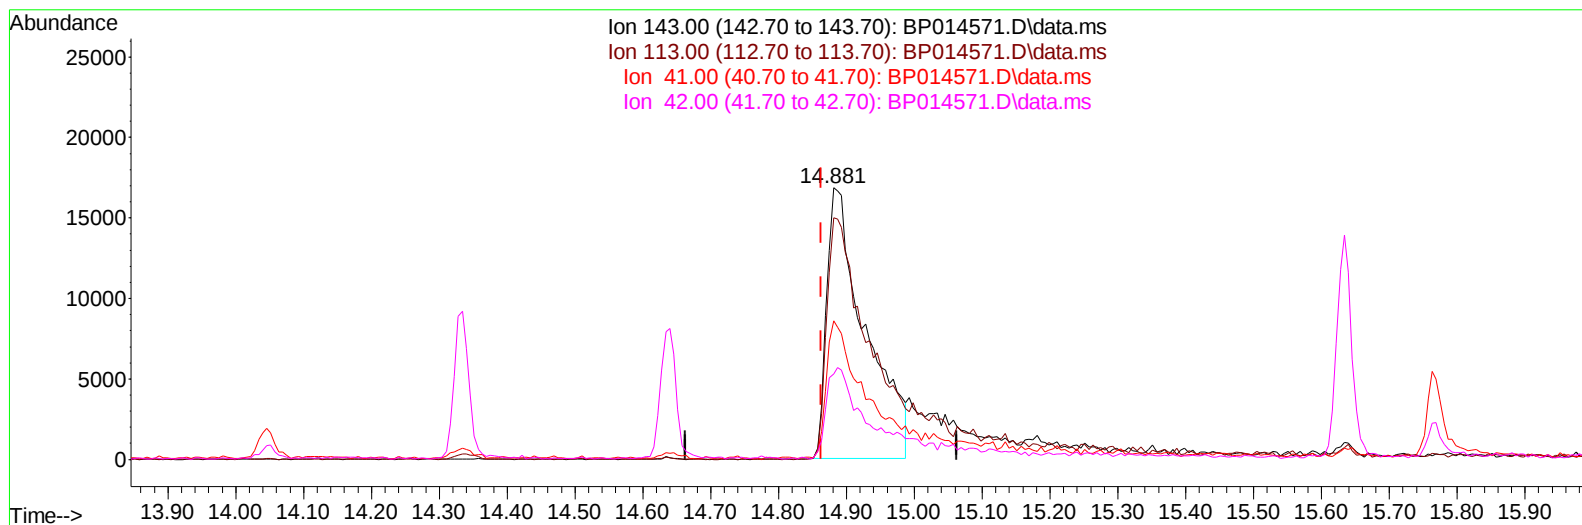

TIC: BP014571.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.881min (+ 0.018) 17.46 ng/u1

response 66164

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	89.10
41.00	44.20	51.06
42.00	31.50	31.43




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014571.D
 Acq On : 05 Apr 2023 23:21
 Operator : CG/JU
 Sample : PB151872BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK872

Manual IntegrationsAPPROVED

Quant Time: Apr 06 01:01:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 06 00:55:13 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/06/2023
 Supervised By :Jagrut Upadhyay 04/06/2023

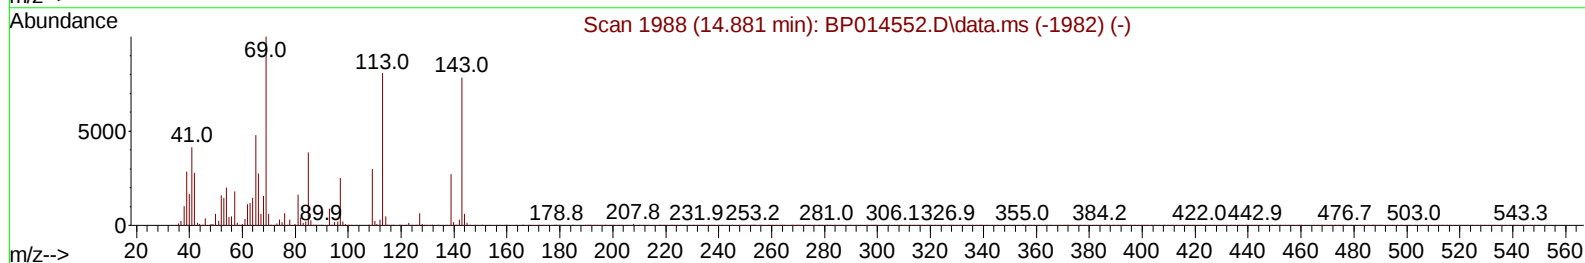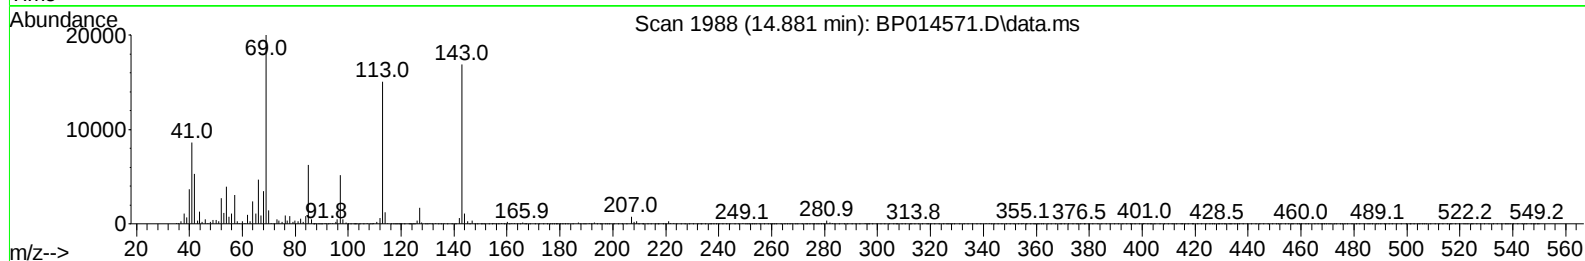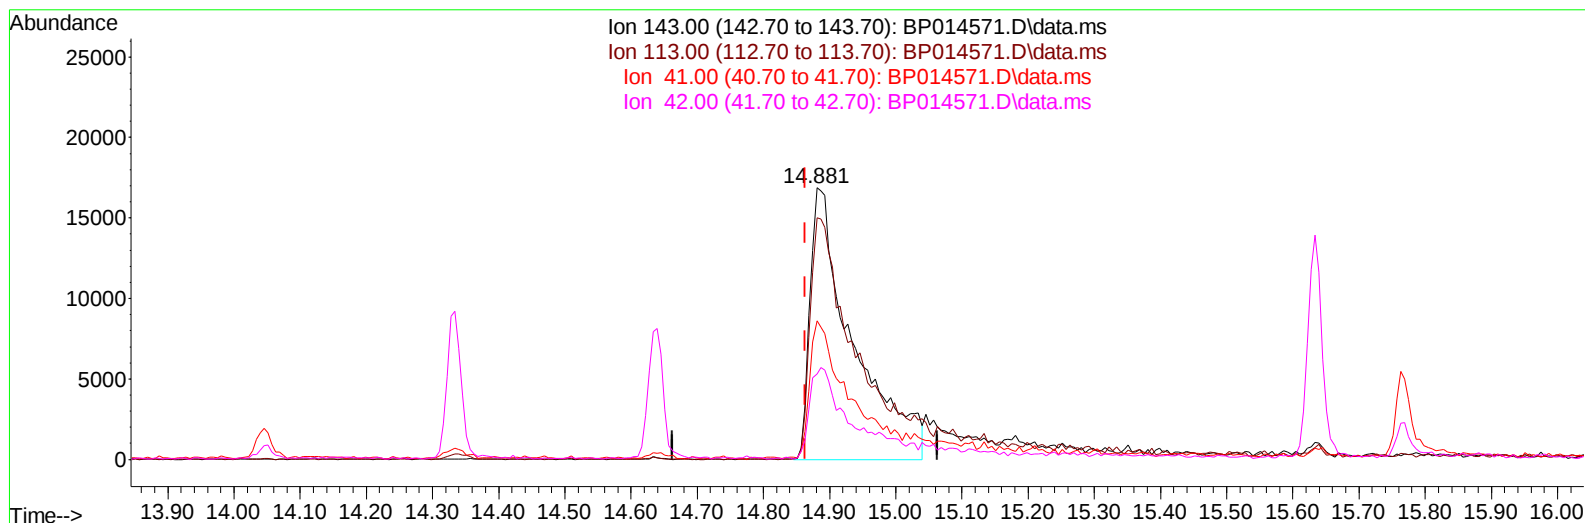

TIC: BP014571.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.881min (+ 0.018) 20.02 ng/ul m

response 75896

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	89.10
41.00	44.20	51.06
42.00	31.50	31.43

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014571.D
 Acq On : 05 Apr 2023 23:21
 Operator : CG/JU
 Sample : PB151872BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK872

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/06/2023
 Supervised By :Jagrut Upadhyay 04/06/2023

Quant Time: Apr 06 01:01:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 06 00:55:13 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.987	152	113884	20.000	ng/ul	0.00
20) Naphthalene-d8	10.805	136	490855	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.640	164	309423	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	667244	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	600800	20.000	ng/ul	0.00
88) Perylene-d12	23.992	264	686690	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	20020	6.817	ng/uL	0.00
4) Pyridine-d5	3.799	84	206771	27.475	ng/ul	0.00
7) Phenol-d5	7.152	99	311640	29.672	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.311	67	226779	33.653	ng/ul	0.00
11) 2-Chlorophenol-d4	7.516	132	239569	31.559	ng/ul	0.00
15) 4-Methylphenol-d8	8.711	113	241736	28.534	ng/ul	0.00
21) Nitrobenzene-d5	9.163	128	118188	29.826	ng/ul	0.00
24) 2-Nitrophenol-d4	9.887	143	125408	27.638	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	203901	24.675	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	281389	25.852	ng/ul	0.00
46) Dimethylphthalate-d6	14.046	166	796716	31.756	ng/ul	0.00
49) Acenaphthylene-d8	14.334	160	882482	31.700	ng/ul	0.00
54) 4-Nitrophenol-d4	14.881	143	75896m	20.024	ng/ul	0.02
60) Fluorene-d10	15.634	176	675893	32.305	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.769	200	101960	20.767	ng/ul	0.00
73) Anthracene-d10	17.498	188	1047135	32.427	ng/ul	0.00
81) Pyrene-d10	19.728	212	1215236	30.113	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.827	264	1203908	32.999	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014571.D
Acq On : 05 Apr 2023 23:21
Operator : CG/JU
Sample : PB151872BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK872

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/06/2023
Supervised By :Jagrut Upadhyay 04/06/2023

Quant Time: Apr 06 01:01:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 06 00:55:13 2023
Response via : Initial Calibration

