




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014593.D
Acq On : 06 Apr 2023 18:22
Operator : CG/JU
Sample : PB151949BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK949

Manual IntegrationsAPPROVED

Quant Time: Apr 07 00:47:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/07/2023
Supervised By :Jagrut Upadhyay 04/07/2023

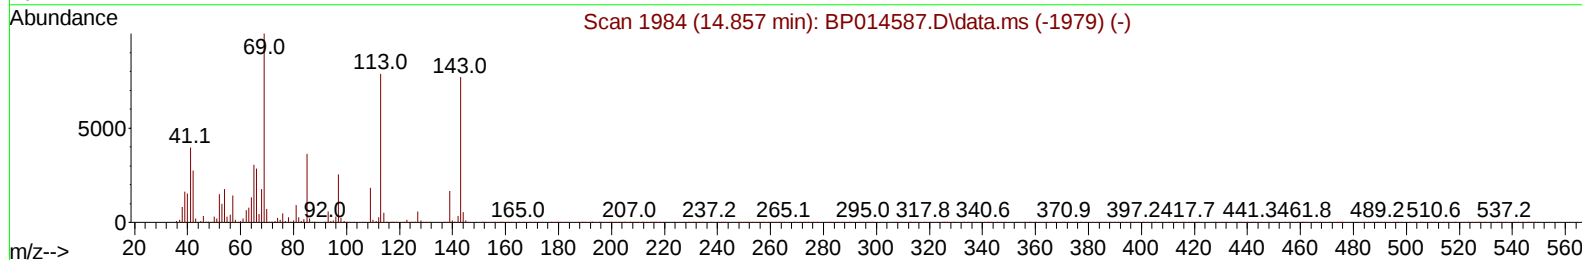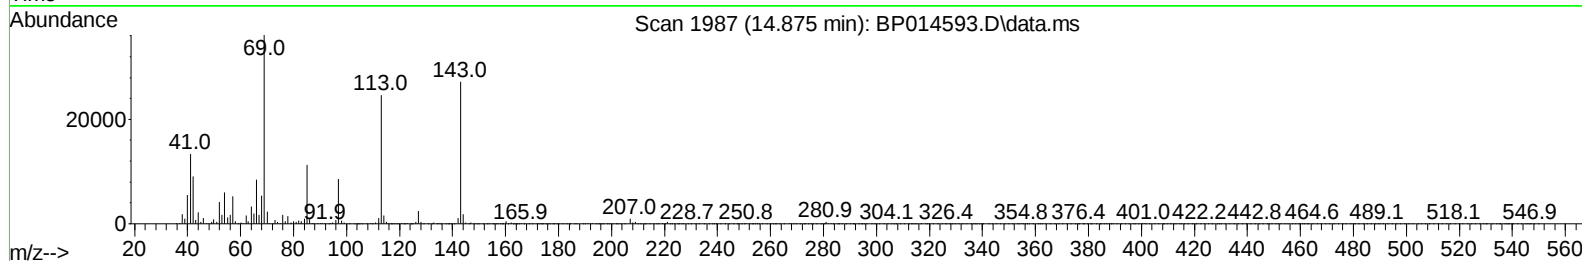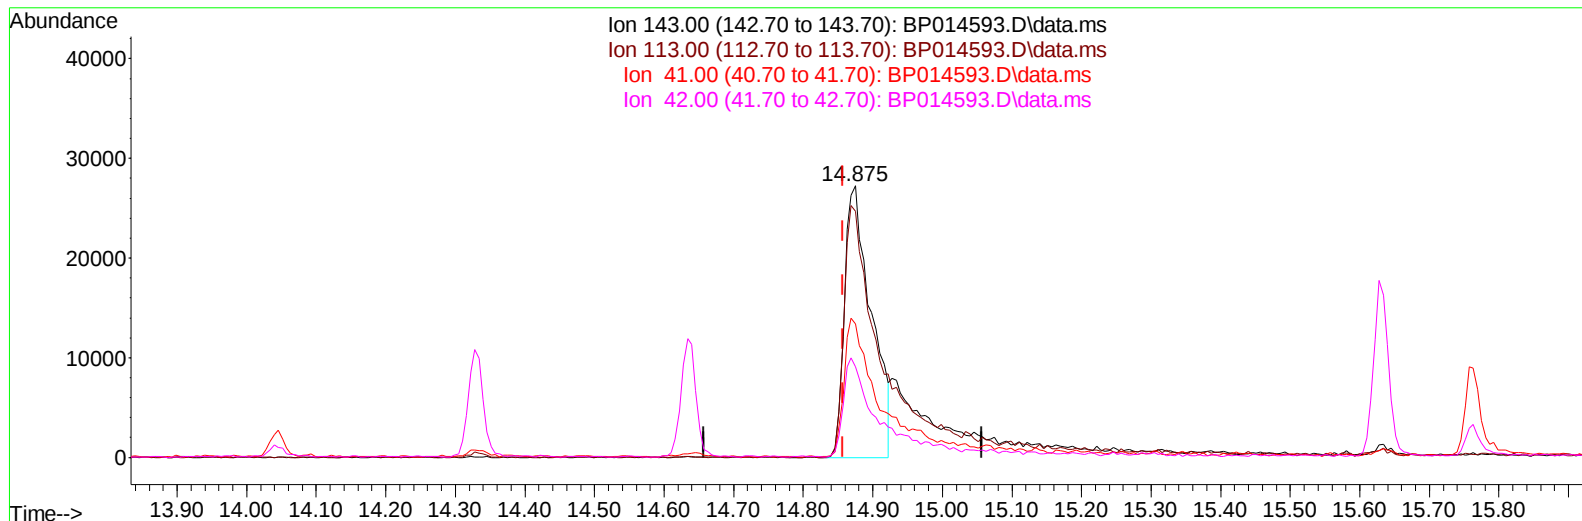

TIC: BP014593.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.875min (+ 0.018) 13.39 ng/u1

response 72623

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	90.63
41.00	44.20	49.27
42.00	31.50	33.35




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014593.D
Acq On : 06 Apr 2023 18:22
Operator : CG/JU
Sample : PB151949BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK949

Manual IntegrationsAPPROVED

Quant Time: Apr 07 00:47:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/07/2023
Supervised By :Jagrut Upadhyay 04/07/2023

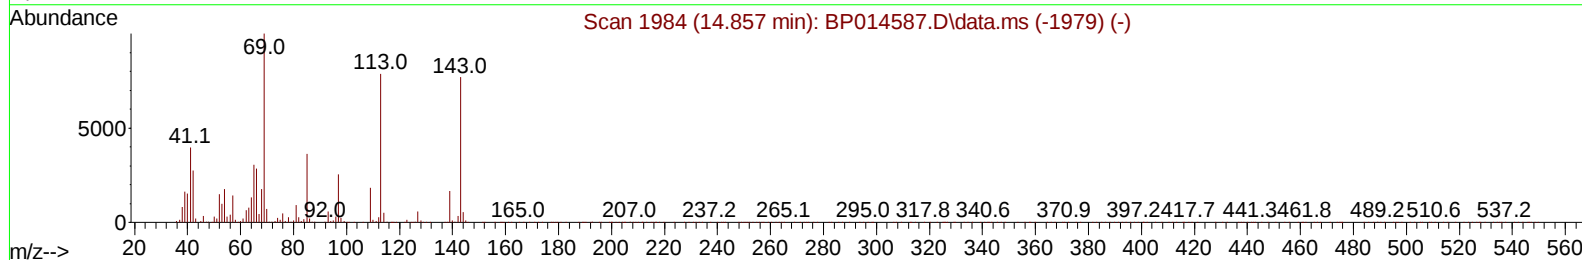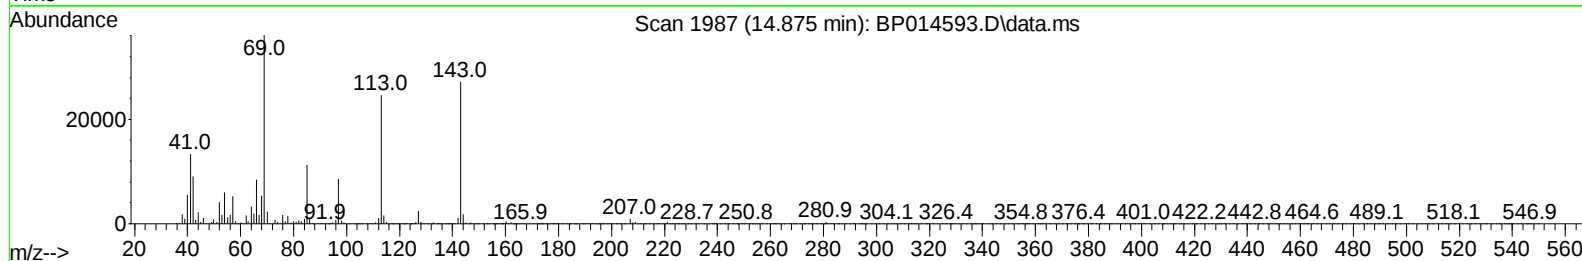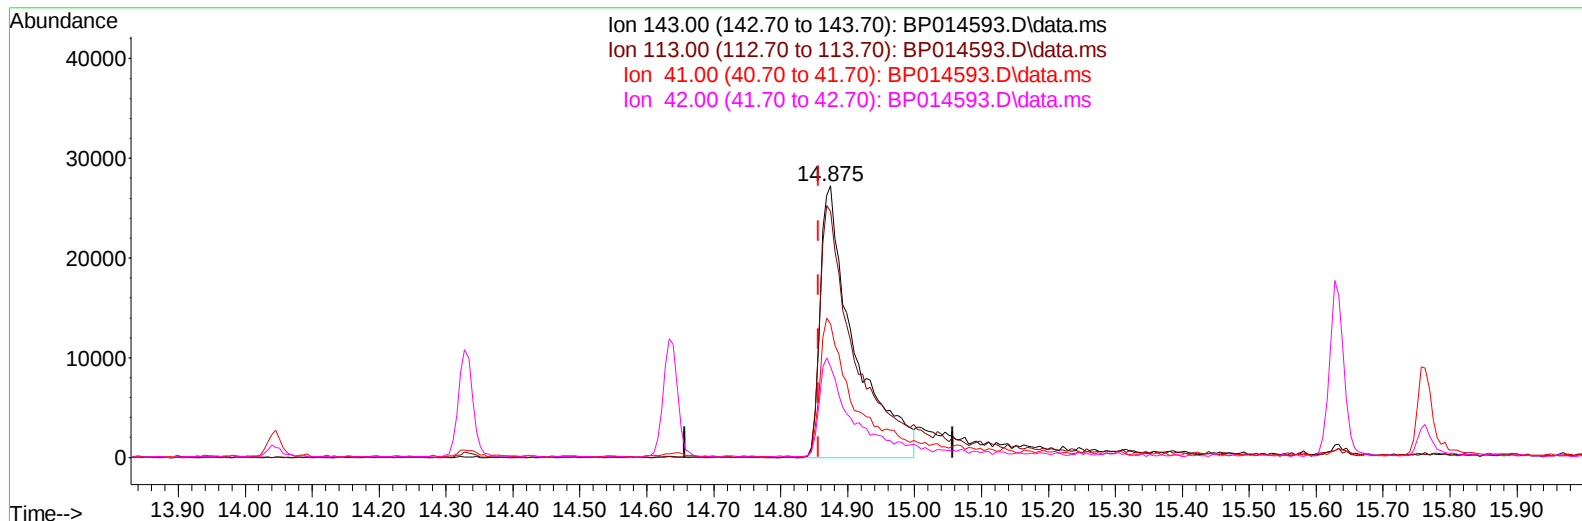

TIC: BP014593.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.875min (+ 0.018) 17.55 ng/ul m

response 95204

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	90.63
41.00	44.20	49.27
42.00	31.50	33.35

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014593.D
 Acq On : 06 Apr 2023 18:22
 Operator : CG/JU
 Sample : PB151949BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK949

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/07/2023
 Supervised By :Jagrut Upadhyay 04/07/2023

Quant Time: Apr 07 00:47:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 07 00:45:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.981	152	146244	20.000	ng/ul	0.00
20) Naphthalene-d8	10.805	136	650955	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.634	164	442792	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	1019271	20.000	ng/ul	0.00
79) Chrysene-d12	21.486	240	832415	20.000	ng/ul	0.00
88) Perylene-d12	23.986	264	729457	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	19808	5.252	ng/uL	0.00
4) Pyridine-d5	3.799	84	196133	20.295	ng/ul	0.00
7) Phenol-d5	7.152	99	329037	24.396	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.311	67	239009	27.620	ng/ul	0.00
11) 2-Chlorophenol-d4	7.516	132	252662	25.919	ng/ul	0.00
15) 4-Methylphenol-d8	8.705	113	271755	24.979	ng/ul	0.00
21) Nitrobenzene-d5	9.163	128	129294	24.604	ng/ul	0.00
24) 2-Nitrophenol-d4	9.887	143	151688	25.208	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	246016	22.449	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	282309	19.557	ng/ul	0.00
46) Dimethylphthalate-d6	14.046	166	967443	26.946	ng/ul	0.00
49) Acenaphthylene-d8	14.328	160	1028645	25.821	ng/ul	0.00
54) 4-Nitrophenol-d4	14.875	143	95204m	17.553	ng/ul	0.02
60) Fluorene-d10	15.634	176	816166	27.260	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.763	200	151948	20.260	ng/ul	0.00
73) Anthracene-d10	17.498	188	1325377	26.869	ng/ul	0.00
81) Pyrene-d10	19.728	212	1539328	27.531	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.821	264	1061901	27.400	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014593.D
Acq On : 06 Apr 2023 18:22
Operator : CG/JU
Sample : PB151949BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK949

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/07/2023
Supervised By :Jagrut Upadhyay 04/07/2023

Quant Time: Apr 07 00:47:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

