




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014595.D
Acq On : 06 Apr 2023 19:31
Operator : CG/JU
Sample : 02194-09
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDW6

Manual IntegrationsAPPROVED

Quant Time: Apr 07 00:47:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/07/2023
Supervised By :Jagrut Upadhyay 04/07/2023

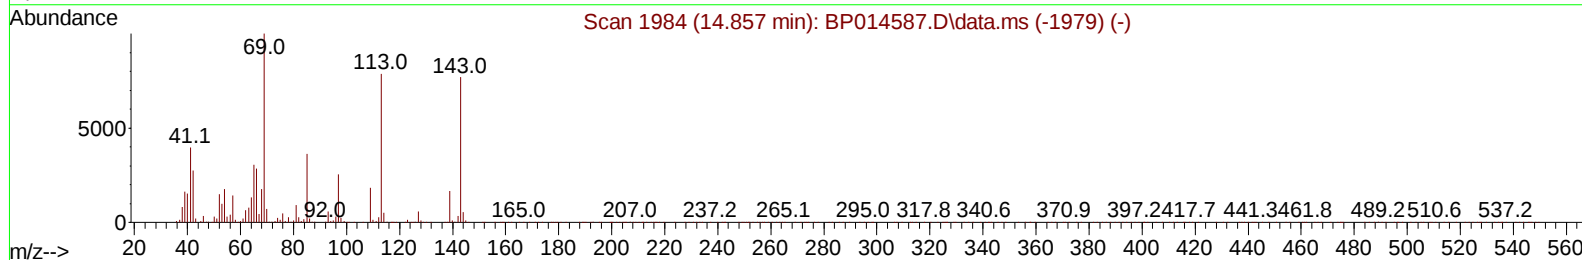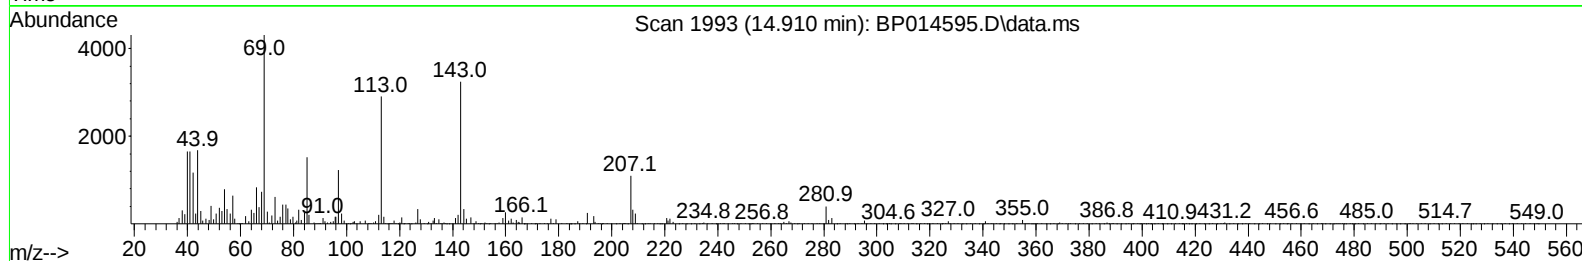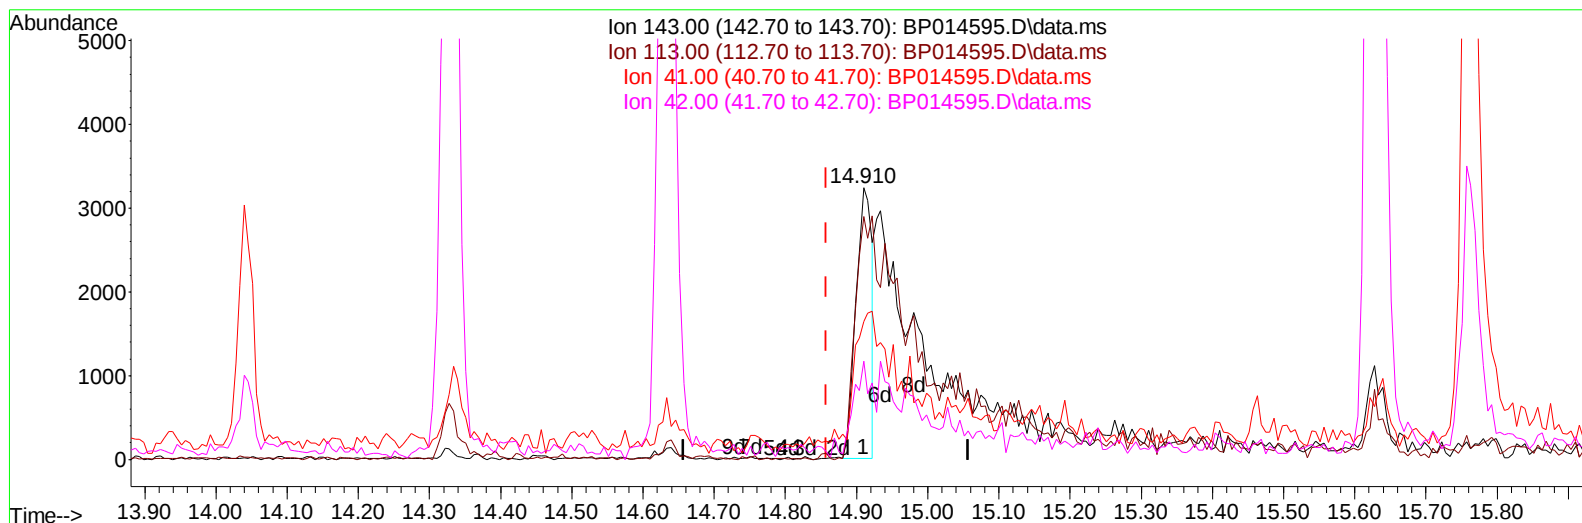

TIC: BP014595.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.053) 0.91 ng/u1

response 5046

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	89.51
41.00	44.20	50.74
42.00	31.50	36.24




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014595.D
Acq On : 06 Apr 2023 19:31
Operator : CG/JU
Sample : 02194-09
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDW6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/07/2023
Supervised By :Jagrut Upadhyay 04/07/2023

Quant Time: Apr 07 00:47:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

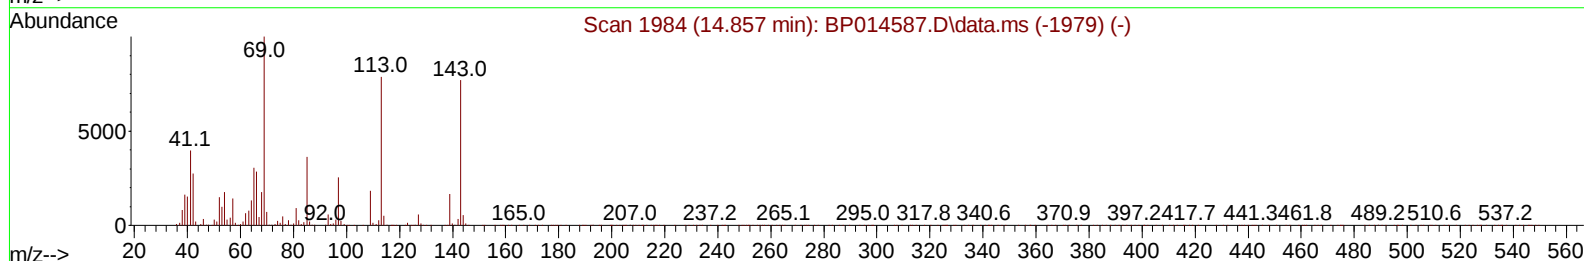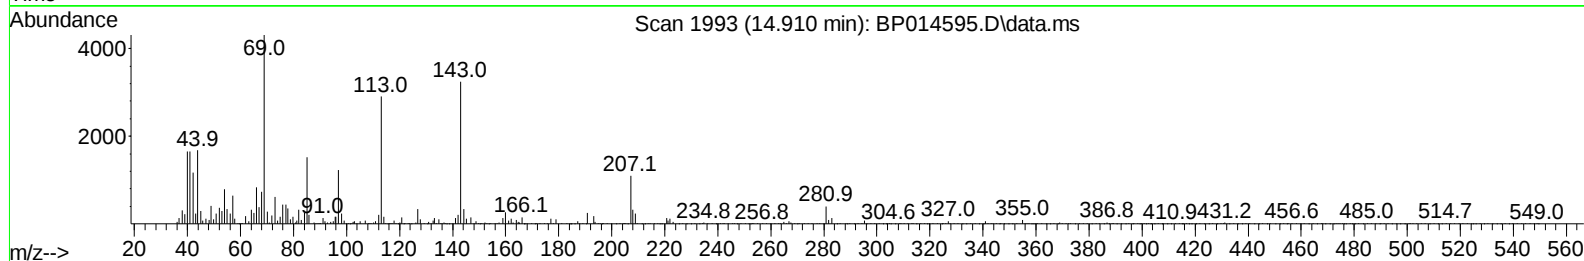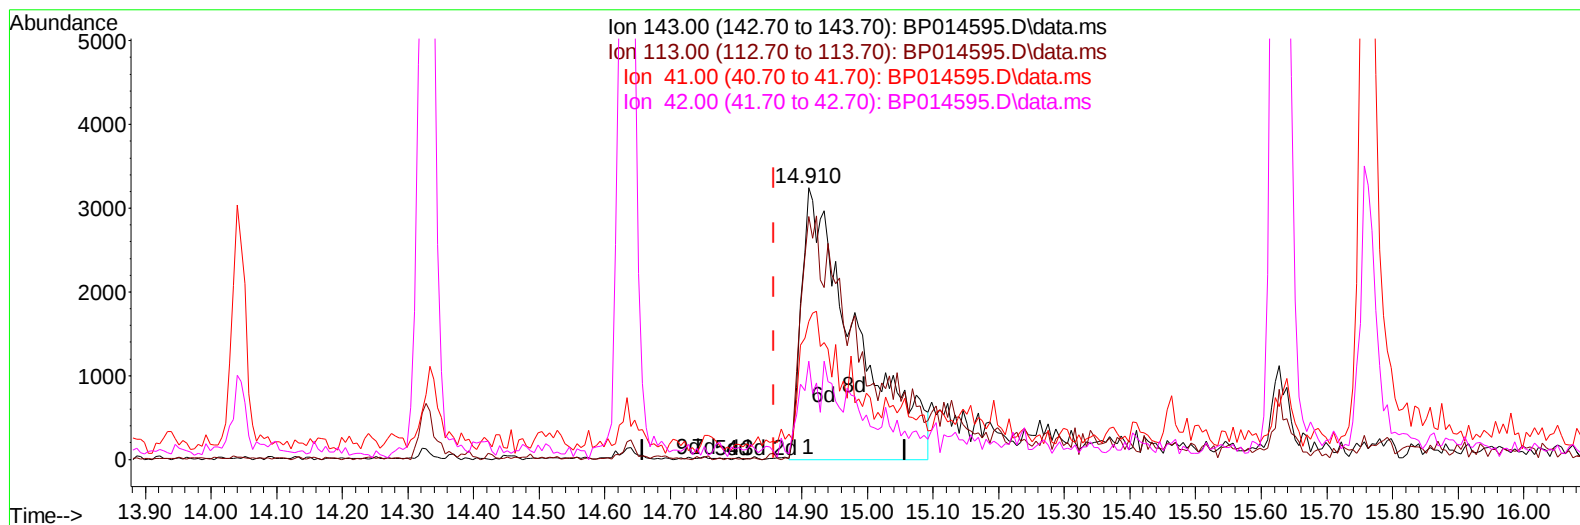

TIC: BP014595.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.053) 3.34 ng/ul m

response 18463

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	89.51
41.00	44.20	50.74
42.00	31.50	36.24

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014595.D
 Acq On : 06 Apr 2023 19:31
 Operator : CG/JU
 Sample : 02194-09
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDW6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/07/2023
 Supervised By :Jagrut Upadhyay 04/07/2023

Quant Time: Apr 07 00:47:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 07 00:45:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.981	152	145590	20.000	ng/ul	0.00
20) Naphthalene-d8	10.804	136	659514	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.634	164	451124	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.398	188	1009895	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	795507	20.000	ng/ul	0.00
88) Perylene-d12	23.980	264	709041	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	16157	4.304	ng/uL	0.00
4) Pyridine-d5	3.811	84	49584	5.154	ng/ul	0.02
7) Phenol-d5	7.158	99	63644	4.740	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.310	67	237277	27.543	ng/ul	0.00
11) 2-Chlorophenol-d4	7.516	132	196312	20.229	ng/ul	0.00
15) 4-Methylphenol-d8	8.705	113	130934	12.089	ng/ul	0.00
21) Nitrobenzene-d5	9.163	128	130745	24.557	ng/ul	0.00
24) 2-Nitrophenol-d4	9.887	143	146301	23.997	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	223477	20.128	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	227032	15.524	ng/ul	0.00
46) Dimethylphthalate-d6	14.045	166	1011912	27.665	ng/ul	0.00
49) Acenaphthylene-d8	14.328	160	1080152	26.613	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	18463m	3.341	ng/ul	0.05
60) Fluorene-d10	15.628	176	862237	28.267	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.763	200	165839	22.317	ng/ul	0.00
73) Anthracene-d10	17.498	188	1468690	30.050	ng/ul	0.00
81) Pyrene-d10	19.727	212	1721306	32.214	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.821	264	1191864	31.639	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014595.D
Acq On : 06 Apr 2023 19:31
Operator : CG/JU
Sample : 02194-09
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDW6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/07/2023
Supervised By :Jagrut Upadhyay 04/07/2023

Quant Time: Apr 07 00:47:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

