




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014600.D
Acq On : 06 Apr 2023 22:21
Operator : CG/JU
Sample : 02225-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB8

Manual IntegrationsAPPROVED

Quant Time: Apr 07 00:48:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/07/2023
Supervised By :Jagrut Upadhyay 04/07/2023

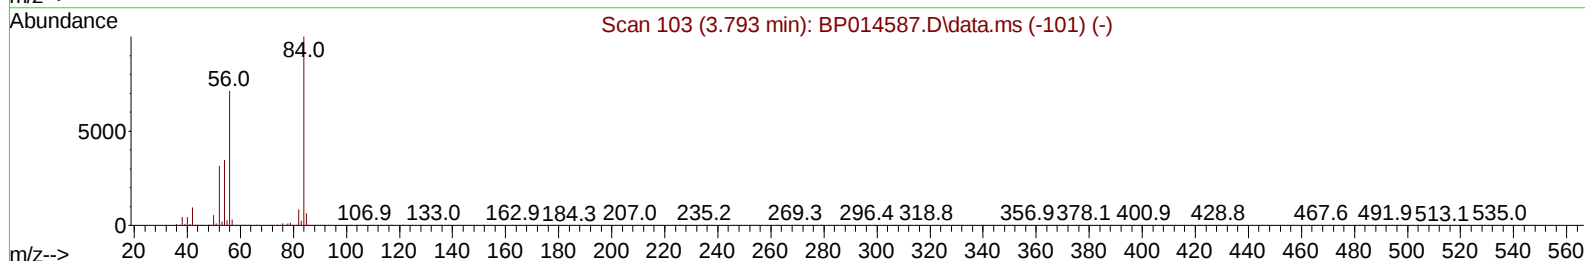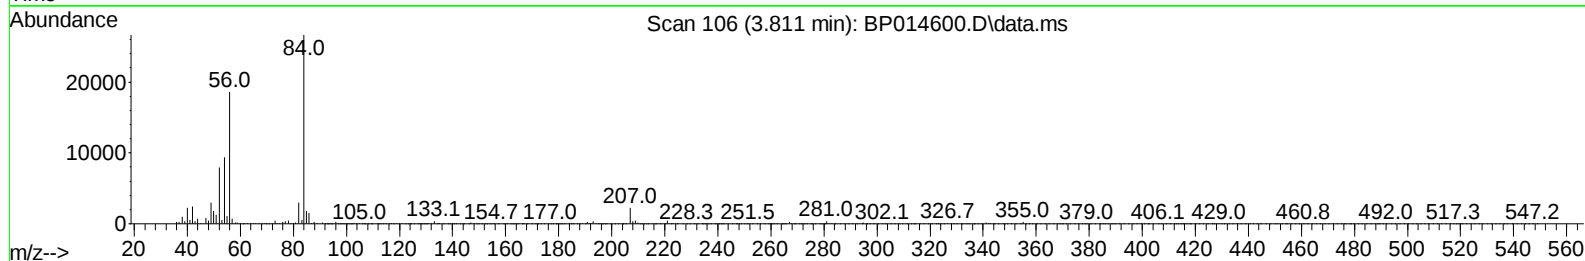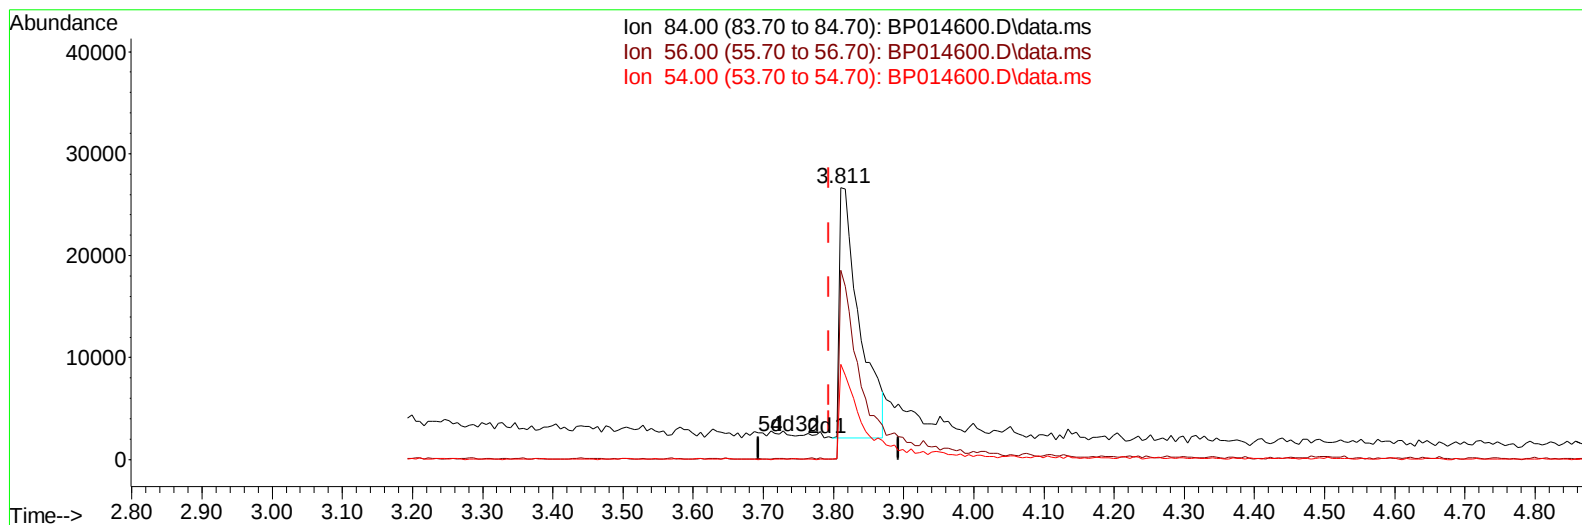

TIC: BP014600.D\data.ms

(4) Pyridine-d5 (S)

3.811min (+ 0.017) 4.48 ng/u1

response 48509

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	69.79
54.00	32.60	35.13
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014600.D
 Acq On : 06 Apr 2023 22:21
 Operator : CG/JU
 Sample : 02225-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB8

Manual IntegrationsAPPROVED

Quant Time: Apr 07 00:48:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 07 00:45:34 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/07/2023
 Supervised By :Jagrut Upadhyay 04/07/2023

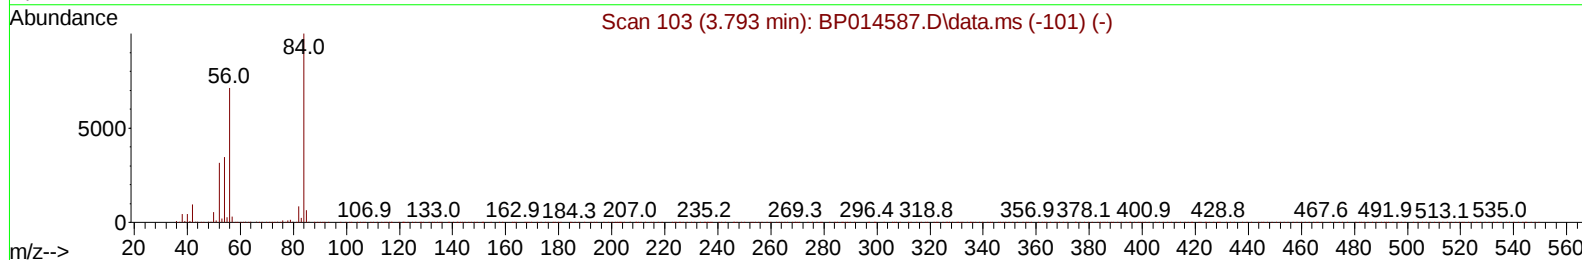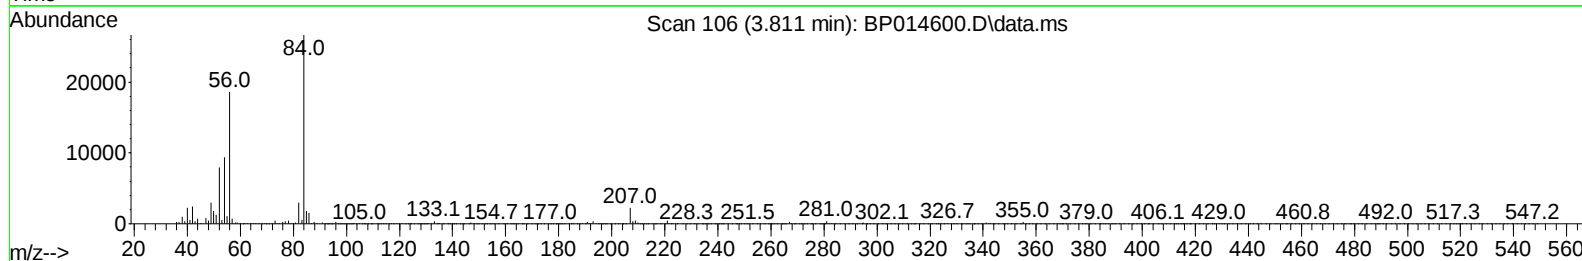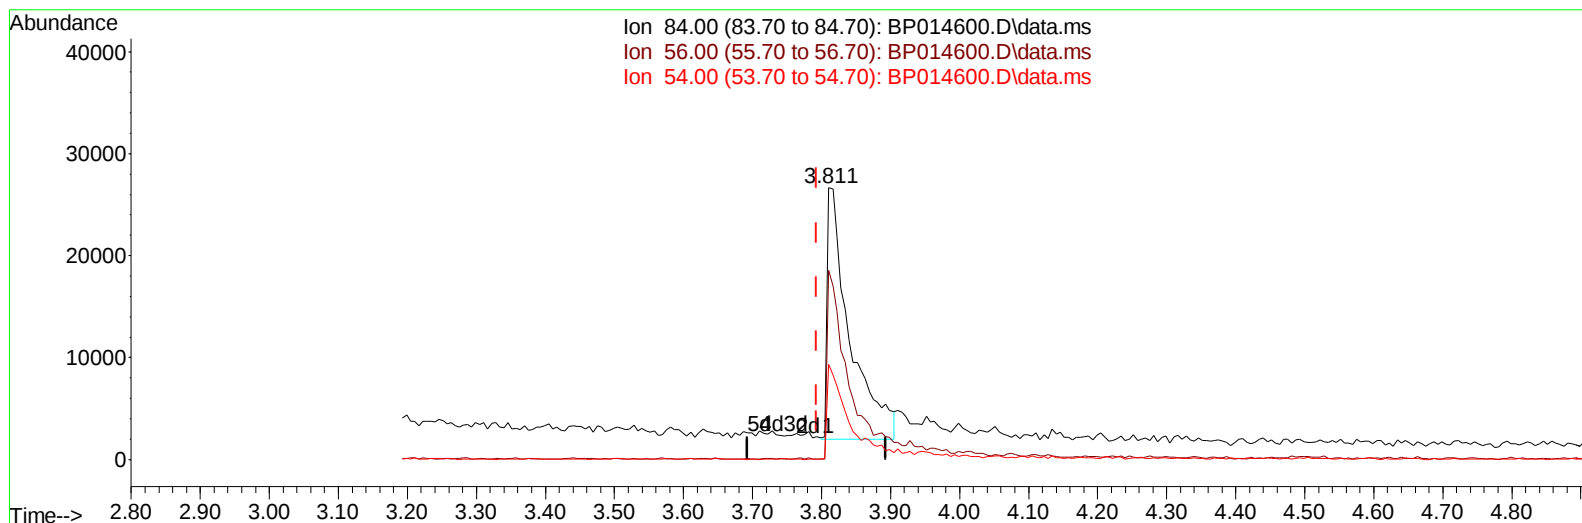

TIC: BP014600.D\data.ms

(4) Pyridine-d5 (S)

3.811min (+ 0.017) 5.16 ng/ul m

response 55907

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	69.79
54.00	32.60	35.13
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014600.D
Acq On : 06 Apr 2023 22:21
Operator : CG/JU
Sample : 02225-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB8

Manual IntegrationsAPPROVED

Quant Time: Apr 07 00:48:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/07/2023
Supervised By :Jagrut Upadhyay 04/07/2023

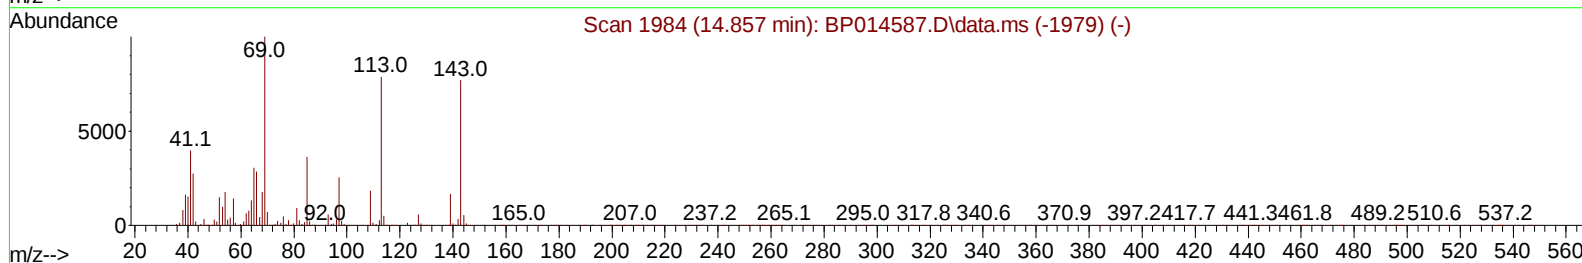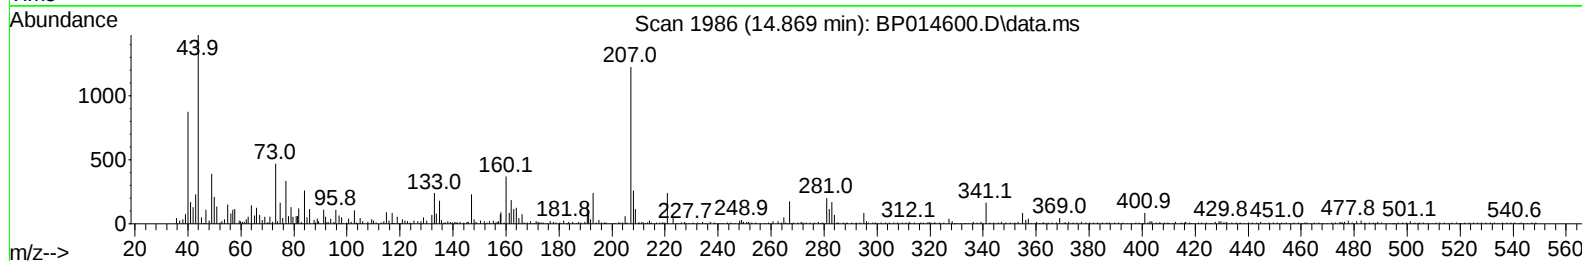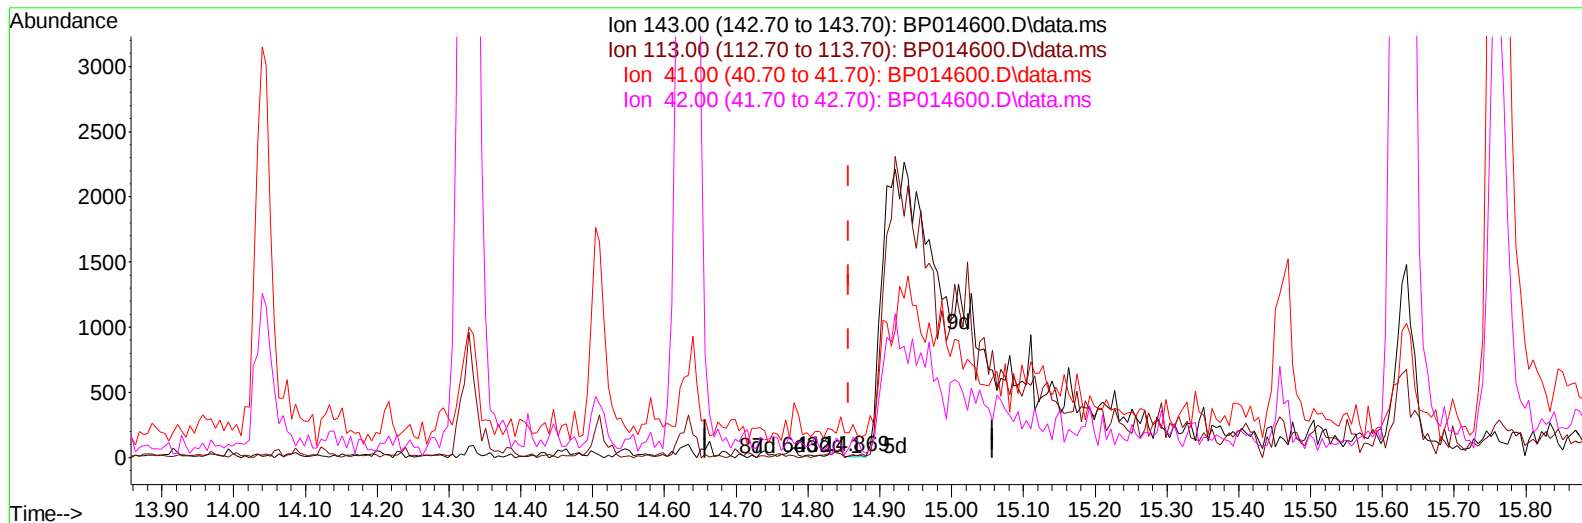

TIC: BP014600.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.869min (+ 0.012) 0.00 ng/u1

response 12

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	85.71
41.00	44.20	1207.14#
42.00	31.50	921.43#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014600.D
Acq On : 06 Apr 2023 22:21
Operator : CG/JU
Sample : 02225-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB8

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/07/2023
Supervised By :Jagrut Upadhyay 04/07/2023

Quant Time: Apr 07 00:48:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

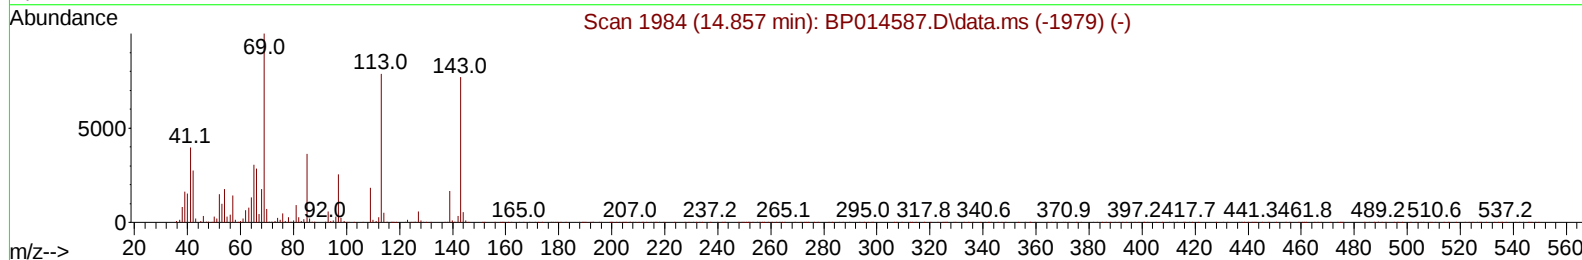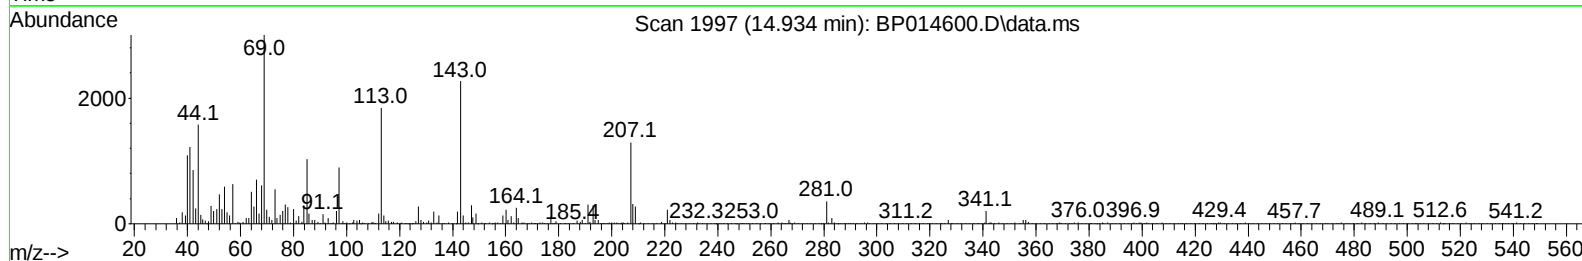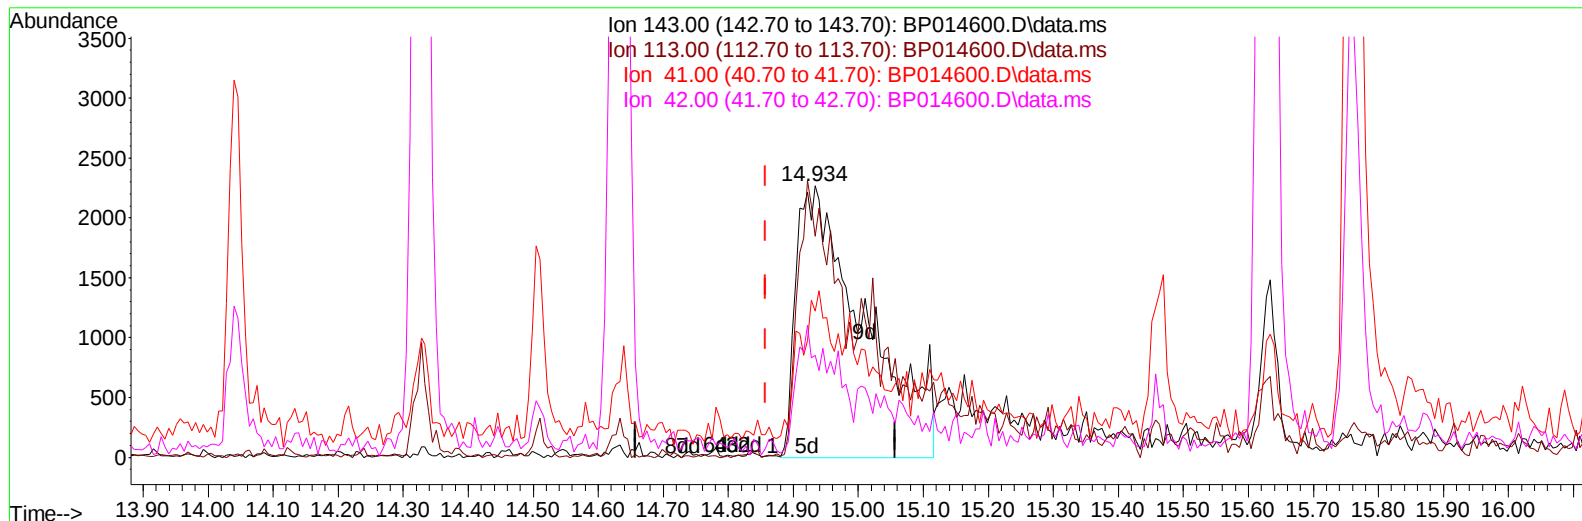

TIC: BP014600.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.934min (+ 0.076) 2.60 ng/u1 m

response 16512

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	81.52
41.00	44.20	53.90#
42.00	31.50	37.67

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014600.D
 Acq On : 06 Apr 2023 22:21
 Operator : CG/JU
 Sample : 02225-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB8

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/07/2023
 Supervised By :Jagrut Upadhyay 04/07/2023

Quant Time: Apr 07 00:48:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 07 00:45:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.981	152	163992	20.000	ng/ul	0.00
20) Naphthalene-d8	10.798	136	754608	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.634	164	518486	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.392	188	1183098	20.000	ng/ul	0.00
79) Chrysene-d12	21.480	240	977795	20.000	ng/ul	0.00
88) Perylene-d12	23.980	264	857826	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	15045	3.558	ng/uL	0.00
4) Pyridine-d5	3.811	84	55907m	5.159	ng/ul	0.02
7) Phenol-d5	7.157	99	62274	4.118	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.310	67	264573	27.265	ng/ul	0.00
11) 2-Chlorophenol-d4	7.516	132	209719	19.185	ng/ul	0.00
15) 4-Methylphenol-d8	8.704	113	133376	10.933	ng/ul	0.00
21) Nitrobenzene-d5	9.157	128	148399	24.360	ng/ul	0.00
24) 2-Nitrophenol-d4	9.887	143	161284	23.121	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.428	165	253754	19.975	ng/ul	0.00
31) 4-Chloroaniline-d4	10.951	131	258967	15.476	ng/ul	0.00
46) Dimethylphthalate-d6	14.045	166	1127947	26.830	ng/ul	0.00
49) Acenaphthylene-d8	14.328	160	1206328	25.861	ng/ul	0.00
54) 4-Nitrophenol-d4	14.934	143	16512m	2.600	ng/ul	0.08
60) Fluorene-d10	15.628	176	965312	27.535	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.763	200	186955	21.476	ng/ul	0.00
73) Anthracene-d10	17.492	188	1716542	29.980	ng/ul	0.00
81) Pyrene-d10	19.727	212	1993439	30.352	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.815	264	1413839	31.022	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014600.D
Acq On : 06 Apr 2023 22:21
Operator : CG/JU
Sample : 02225-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB8

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/07/2023
Supervised By :Jagrut Upadhyay 04/07/2023

Quant Time: Apr 07 00:48:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 07 00:45:34 2023
Response via : Initial Calibration

