

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014553.D
 Acq On : 05 Apr 2023 12:35
 Operator : CG/JU
 Sample : PB151829BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK829

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014553.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	37	rVB	44251	53386	1.27%	0.130%
2	3.799	102	104	125	rBV	396409	729848	17.34%	1.782%
3	4.122	156	159	166	rVB2	10953	15690	0.37%	0.038%
4	7.157	669	675	694	rBV	519353	1031280	24.50%	2.518%
5	7.316	696	702	714	rVB	502929	827492	19.66%	2.021%
6	7.522	730	737	755	rBV	587618	1070415	25.43%	2.614%
7	7.987	809	816	824	rBV	527275	867632	20.61%	2.119%
8	8.710	932	939	957	rBV	669413	1318174	31.32%	3.219%
9	9.163	1009	1016	1030	rBV	612126	1110527	26.39%	2.712%
10	9.893	1132	1140	1150	rBV	458309	830194	19.72%	2.027%
11	10.081	1165	1172	1182	rVB2	30780	72648	1.73%	0.177%
12	10.440	1226	1233	1254	rBV	520079	1137809	27.03%	2.778%
13	10.810	1288	1296	1311	rBV	654768	1109249	26.35%	2.709%
14	10.963	1314	1322	1346	rBV	436490	1038272	24.67%	2.535%
15	12.416	1562	1569	1576	rBV5	10006	24098	0.57%	0.059%
16	13.528	1752	1758	1764	rVB5	4012	7976	0.19%	0.019%
17	13.622	1771	1774	1779	rVB6	2785	4785	0.11%	0.012%
18	14.051	1839	1847	1863	rBV	1647587	2424973	57.62%	5.921%
19	14.334	1888	1895	1911	rBV2	1655603	2600244	61.78%	6.349%
20	14.451	1914	1915	1921	rVB6	4474	4933	0.12%	0.012%
21	14.639	1940	1947	1962	rBV	1238107	1885620	44.80%	4.604%
22	14.881	1981	1988	2015	rBV2	255753	893014	21.22%	2.181%
23	15.639	2110	2117	2133	rBV	2223782	3297099	78.34%	8.051%
24	15.769	2133	2139	2155	rBV	321362	700801	16.65%	1.711%
25	16.428	2249	2251	2256	rVB6	4587	6328	0.15%	0.015%
26	17.198	2377	2382	2387	rVB8	4458	8867	0.21%	0.022%
27	17.404	2410	2417	2427	rBV	1587870	2326452	55.27%	5.681%
28	17.504	2427	2434	2454	rVV	2469751	3653954	86.81%	8.922%
29	17.916	2502	2504	2509	rBV6	3717	4286	0.10%	0.010%
30	19.310	2738	2741	2745	rVB3	29354	36519	0.87%	0.089%
31	19.386	2750	2754	2756	rBV2	26070	36019	0.86%	0.088%
32	19.733	2807	2813	2829	rBV	3129265	4208921	100.00%	10.277%
33	21.492	3107	3112	3125	rBV	1363874	2216907	52.67%	5.413%
34	23.833	3503	3510	3526	rVB2	1587529	3439812	81.73%	8.399%
35	23.998	3531	3538	3553	rVB2	867448	1958777	46.54%	4.783%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014553.D
Acq On : 05 Apr 2023 12:35
Operator : CG/JU
Sample : PB151829BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK829

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION




Sum of corrected areas: 40953001

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014553.D
Acq On : 05 Apr 2023 12:35
Operator : CG/JU
Sample : PB151829BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK829

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

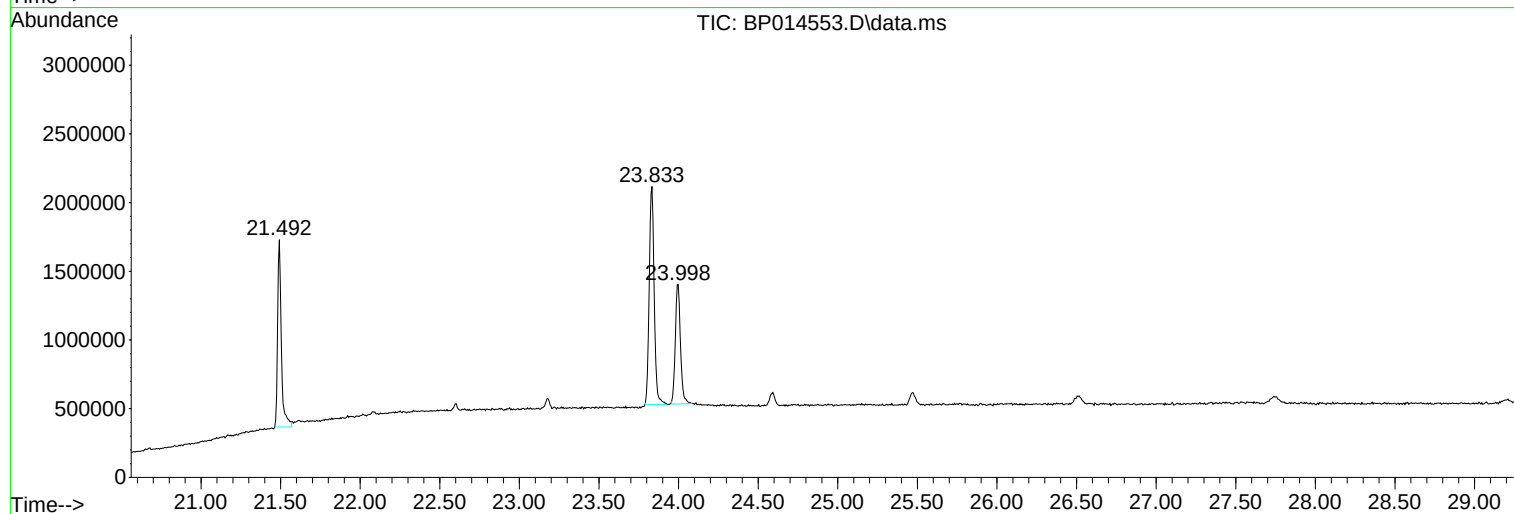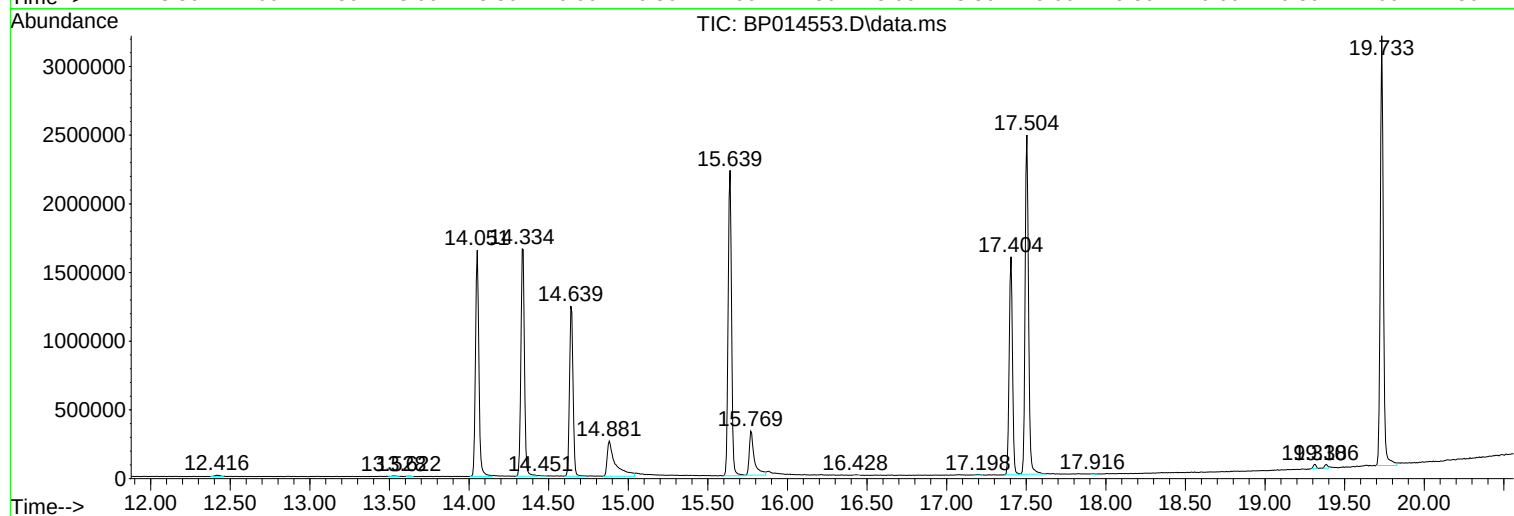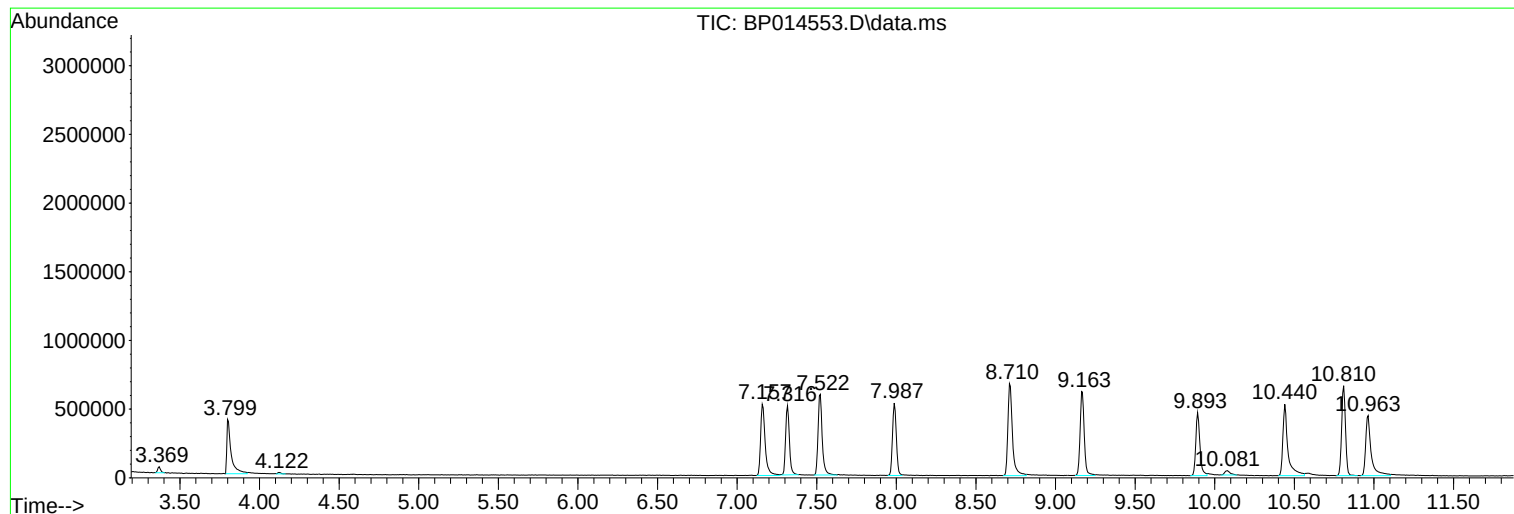

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014553.D
Acq On : 05 Apr 2023 12:35
Operator : CG/JU
Sample : PB151829BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK829

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014553.D
Acq On : 05 Apr 2023 12:35
Operator : CG/JU
Sample : PB151829BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK829

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc