

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014554.D
 Acq On : 05 Apr 2023 13:09
 Operator : CG/JU
 Sample : PB151827BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK827

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014554.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	27	31	38	rVB	34893	46174	1.33%	0.148%
2	3.805	102	105	122	rBV	285594	517373	14.92%	1.661%
3	4.122	156	159	167	rVB2	10459	13147	0.38%	0.042%
4	6.105	492	496	498	rBV5	2683	3771	0.11%	0.012%
5	6.605	576	581	582	rBV5	2468	3740	0.11%	0.012%
6	7.081	658	662	668	rBV8	2389	4766	0.14%	0.015%
7	7.158	669	675	692	rVV	345232	715382	20.63%	2.297%
8	7.316	696	702	714	rVB	350704	572874	16.52%	1.839%
9	7.522	730	737	757	rBV	397356	766009	22.09%	2.459%
10	7.987	809	816	825	rBV	423129	696536	20.09%	2.236%
11	8.716	933	940	961	rBV	421956	892035	25.72%	2.864%
12	8.928	974	976	980	rVB5	2908	3523	0.10%	0.011%
13	9.169	1009	1017	1028	rBV	411085	746358	21.52%	2.396%
14	9.893	1133	1140	1150	rBV	267523	511684	14.75%	1.643%
15	10.075	1165	1171	1186	rVB5	23714	71798	2.07%	0.230%
16	10.446	1227	1234	1249	rBV	325010	803467	23.17%	2.579%
17	10.587	1256	1258	1270	rVB10	16534	41195	1.19%	0.132%
18	10.810	1288	1296	1308	rBV	584026	999767	28.83%	3.210%
19	10.963	1315	1322	1349	rBV	315287	804910	23.21%	2.584%
20	12.428	1565	1571	1576	rVV5	6125	13685	0.39%	0.044%
21	14.051	1839	1847	1865	rBV	1008532	1614789	46.56%	5.184%
22	14.334	1889	1895	1912	rBV	1112426	1744223	50.30%	5.599%
23	14.640	1940	1947	1958	rBV	917945	1394549	40.21%	4.477%
24	14.892	1982	1990	2014	rBV2	125700	537815	15.51%	1.727%
25	15.639	2110	2117	2129	rBV	1473781	2232121	64.36%	7.166%
26	15.775	2134	2140	2154	rBV	139566	334103	9.63%	1.073%
27	16.422	2247	2250	2256	rVB7	3310	6689	0.19%	0.021%
28	17.404	2410	2417	2427	rBV	1215347	1766754	50.95%	5.672%
29	17.504	2428	2434	2450	rVV2	1605460	2480202	71.52%	7.962%
30	19.316	2738	2742	2745	rBV3	22027	30292	0.87%	0.097%
31	19.386	2750	2754	2756	rBV2	20680	27743	0.80%	0.089%
32	19.733	2807	2813	2829	rBV	2197325	3105198	89.54%	9.969%
33	21.492	3107	3112	3125	rBV	1269089	2096916	60.47%	6.732%
34	23.827	3503	3509	3526	rVB2	1633237	3467912	100.00%	11.133%
35	23.992	3531	3537	3548	rVB2	931884	2082522	60.05%	6.685%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014554.D
Acq On : 05 Apr 2023 13:09
Operator : CG/JU
Sample : PB151827BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK827

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION




Sum of corrected areas: 31150022

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014554.D
Acq On : 05 Apr 2023 13:09
Operator : CG/JU
Sample : PB151827BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK827

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

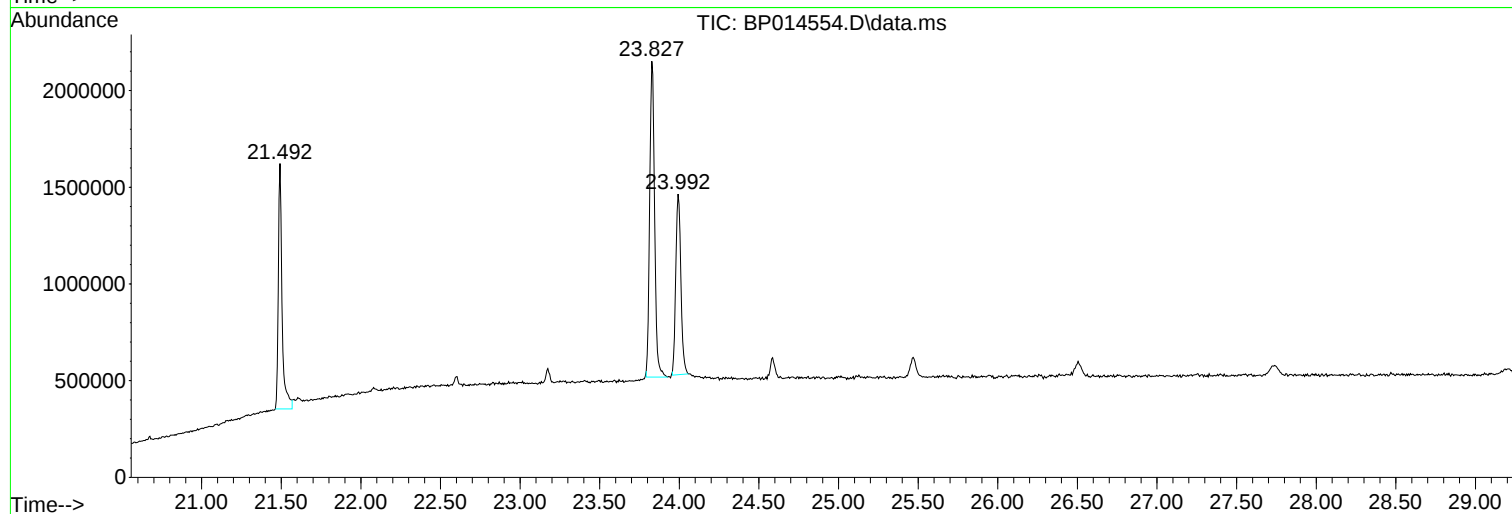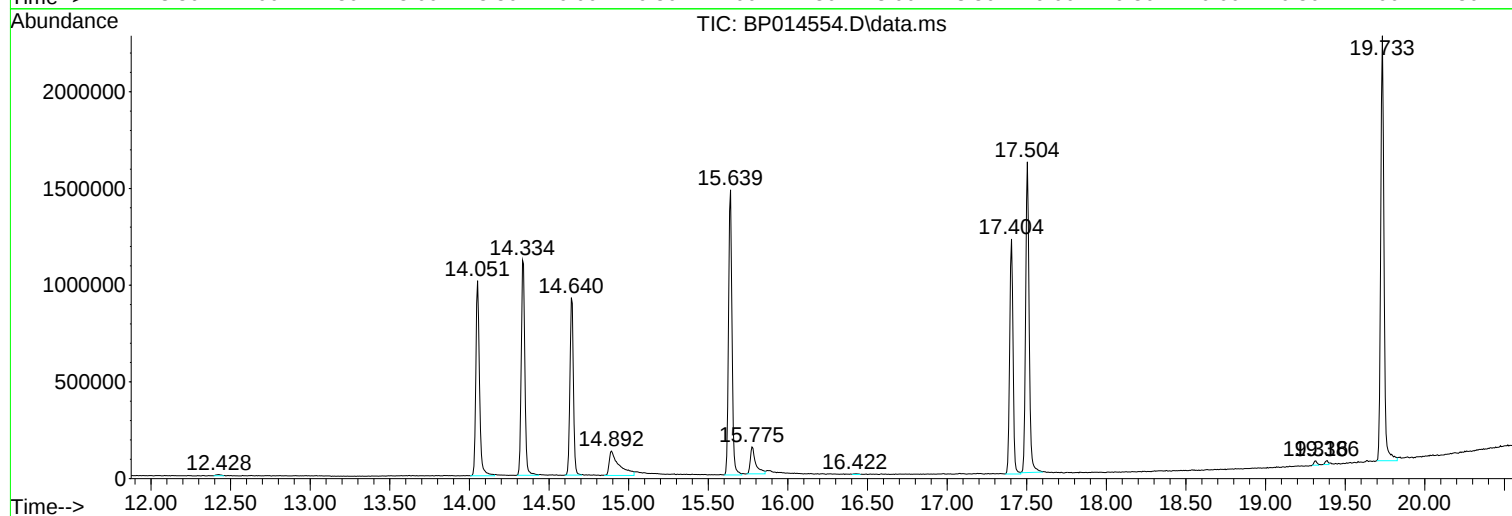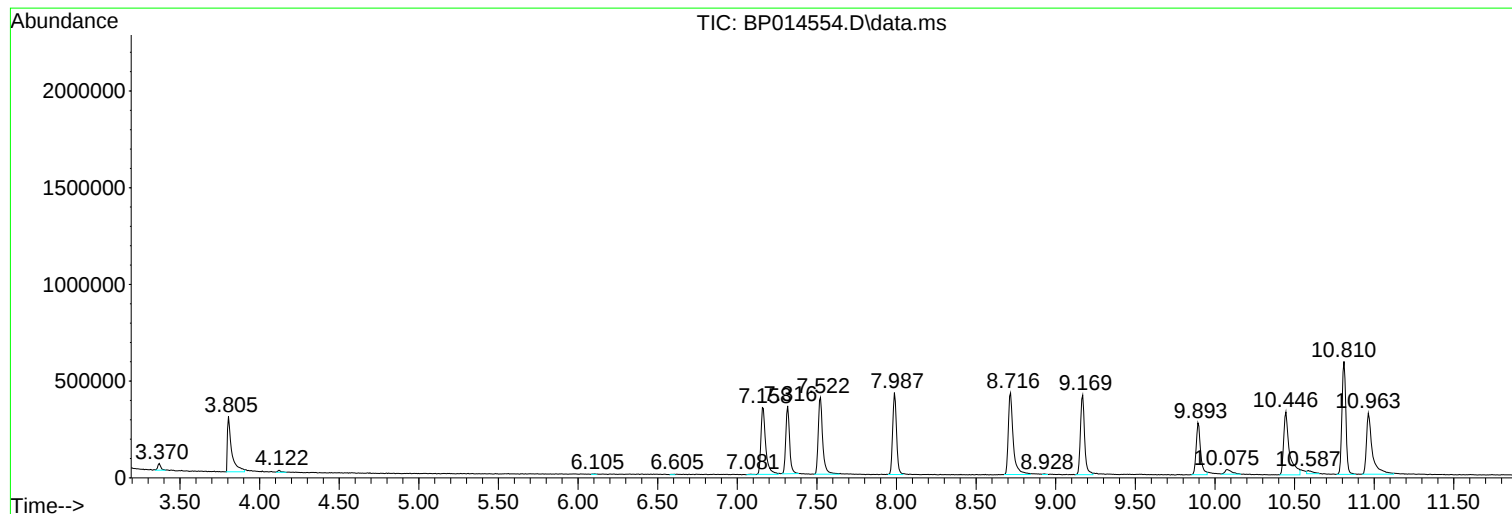

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014554.D
Acq On : 05 Apr 2023 13:09
Operator : CG/JU
Sample : PB151827BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK827

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014554.D
Acq On : 05 Apr 2023 13:09
Operator : CG/JU
Sample : PB151827BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK827

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc