

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014558.D
 Acq On : 05 Apr 2023 15:24
 Operator : CG/JU
 Sample : 02122-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9B0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014558.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	27	31	36	rVB	27150	33605	0.92%	0.114%
2	3.828	107	109	119	rBV	31667	70437	1.94%	0.238%
3	4.016	138	141	148	rVB3	11463	18728	0.52%	0.063%
4	4.122	155	159	162	rVB4	8373	11579	0.32%	0.039%
5	4.234	174	178	181	rBV6	6830	7840	0.22%	0.026%
6	4.687	253	255	261	rVB7	2817	4318	0.12%	0.015%
7	5.057	313	318	322	rBV	5812	10124	0.28%	0.034%
8	6.363	535	540	545	rBV8	5414	9422	0.26%	0.032%
9	7.081	660	662	668	rVB7	3018	4553	0.13%	0.015%
10	7.169	668	677	691	rBV	62892	163653	4.50%	0.553%
11	7.316	695	702	714	rBV	366773	621586	17.10%	2.100%
12	7.522	731	737	757	rBV	321868	631821	17.38%	2.134%
13	7.987	809	816	828	rBV	359493	605524	16.66%	2.046%
14	8.716	932	940	957	rBV2	221173	498702	13.72%	1.685%
15	9.169	1009	1017	1036	rBV	455315	851360	23.42%	2.876%
16	9.528	1073	1078	1087	rVB8	6816	15417	0.42%	0.052%
17	9.892	1131	1140	1160	rBV	321130	643954	17.72%	2.175%
18	10.063	1163	1169	1170	rBV6	13456	16925	0.47%	0.057%
19	10.439	1226	1233	1253	rBV	338670	907691	24.97%	3.066%
20	10.810	1288	1296	1313	rVB	503853	887604	24.42%	2.999%
21	10.969	1313	1323	1343	rBV	177841	490115	13.48%	1.656%
22	12.216	1531	1535	1540	rVB8	3561	6645	0.18%	0.022%
23	12.410	1563	1568	1575	rBV7	7078	15485	0.43%	0.052%
24	13.239	1705	1709	1717	rBV7	2725	7028	0.19%	0.024%
25	13.439	1739	1743	1747	rBV6	5838	8210	0.23%	0.028%
26	13.610	1770	1772	1778	rVB6	2602	4294	0.12%	0.015%
27	14.045	1838	1846	1862	rBV	1119748	1766144	48.59%	5.966%
28	14.151	1862	1864	1871	rVB8	5683	11274	0.31%	0.038%
29	14.333	1883	1895	1908	rBV	1276165	1942004	53.43%	6.560%
30	14.510	1921	1925	1929	rVB6	5290	7893	0.22%	0.027%
31	14.639	1939	1947	1958	rBV	808940	1197905	32.96%	4.047%
32	14.933	1990	1997	2000	rBV6	19256	46119	1.27%	0.156%
33	15.239	2045	2049	2054	rVB6	9330	16141	0.44%	0.055%
34	15.463	2083	2087	2092	rVB2	17634	21713	0.60%	0.073%
35	15.633	2110	2116	2129	rBV	1622829	2497251	68.71%	8.436%
36	15.769	2134	2139	2148	rBV	282577	561945	15.46%	1.898%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014558.D
 Acq On : 05 Apr 2023 15:24
 Operator : CG/JU
 Sample : 02122-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9B0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	16.004	2175	2179	2190	rVB	54601	98673	2.71%	0.333%
38	16.086	2191	2193	2199	rVB7	5616	7335	0.20%	0.025%
39	16.210	2212	2214	2220	rVB7	4680	4569	0.13%	0.015%
40	16.333	2231	2235	2246	rBV	31444	56032	1.54%	0.189%
41	16.733	2301	2303	2309	rVB7	3917	5080	0.14%	0.017%
42	16.798	2312	2314	2317	rVV4	4283	5074	0.14%	0.017%
43	16.827	2317	2319	2326	rVB7	4509	8896	0.24%	0.030%
44	17.133	2366	2371	2374	rBV2	17715	25310	0.70%	0.086%
45	17.398	2410	2416	2427	rBV	948988	1453419	39.99%	4.910%
46	17.498	2427	2433	2447	rVV	1757701	2731992	75.16%	9.229%
47	17.680	2462	2464	2470	rVB7	7272	9807	0.27%	0.033%
48	17.874	2493	2497	2500	rVB4	10661	13137	0.36%	0.044%
49	18.045	2524	2526	2531	rBV5	8233	9837	0.27%	0.033%
50	18.280	2561	2566	2572	rBV7	30044	71186	1.96%	0.240%
51	19.310	2737	2741	2746	rBV4	31622	45064	1.24%	0.152%
52	19.380	2749	2753	2761	rVV2	26800	55221	1.52%	0.187%
53	19.733	2807	2813	2820	rBV	2350272	3313686	91.17%	11.194%
54	21.162	3053	3056	3064	rBV3	171283	273215	7.52%	0.923%
55	21.486	3107	3111	3121	rBV	990962	1556976	42.84%	5.260%
56	23.827	3502	3509	3524	rVB	1785918	3634740	100.00%	12.279%
57	23.992	3531	3537	3546	rVB2	769973	1607250	44.22%	5.430%




Sum of corrected areas: 29601508

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014558.D
Acq On : 05 Apr 2023 15:24
Operator : CG/JU
Sample : 02122-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9B0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

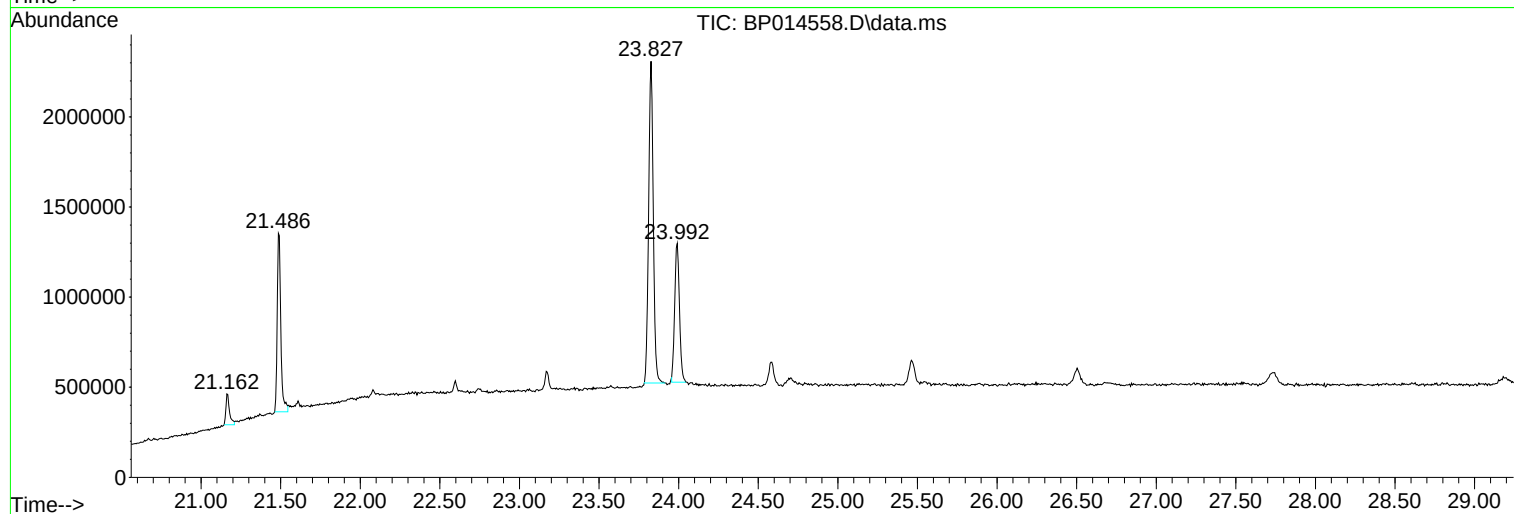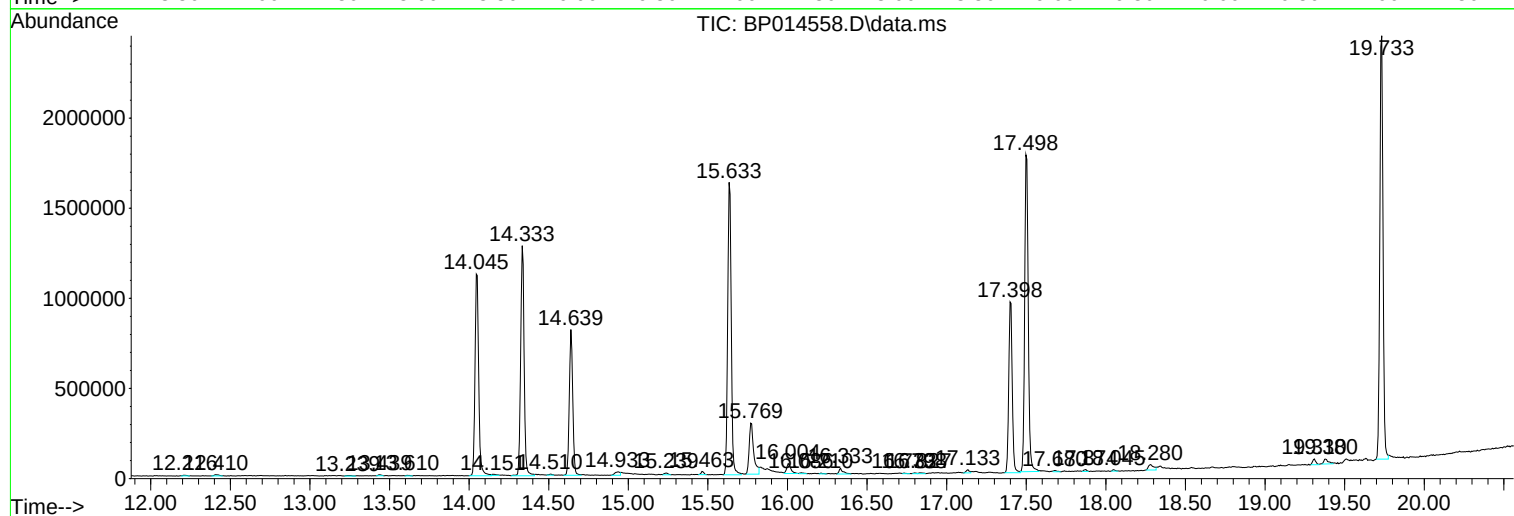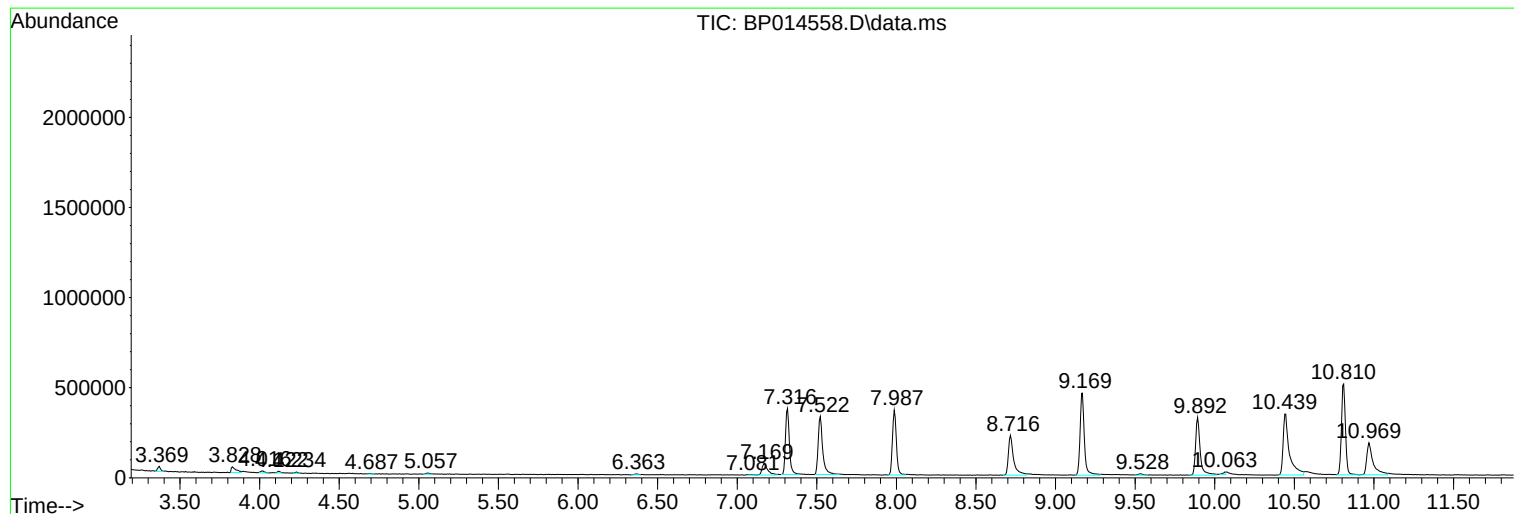

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014558.D
Acq On : 05 Apr 2023 15:24
Operator : CG/JU
Sample : 02122-07
Misc :
ALS Vial : 8 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
CB9B0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.162	3.51 ng/ul	273215	Chrysene-d12		21.486	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	1-Tetracosene		336	C24H48	010192-32-2	99
2	3-Eicosene, (E)-		280	C20H40	074685-33-9	95
3	Behenic alcohol		326	C22H46O	000661-19-8	93
4	1-Eicosene		280	C20H40	003452-07-1	91
5	Heptadecyl heptafluorobutyrate		452	C21H35F7O2	959085-66-6	90

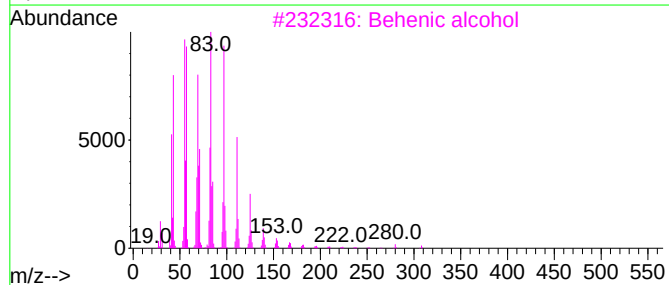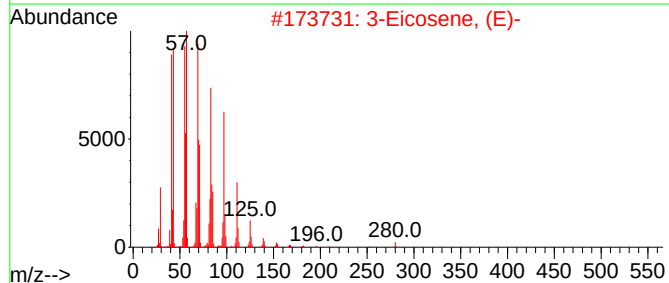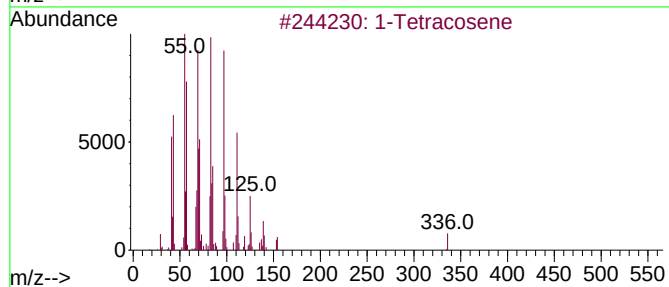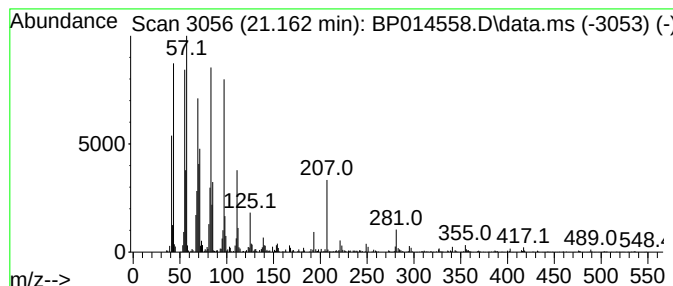

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014558.D
Acq On : 05 Apr 2023 15:24
Operator : CG/JU
Sample : 02122-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9B0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.162	3.5	ng/u1	273215	5	21.486	1556980	20.0