

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014561.D
 Acq On : 05 Apr 2023 17:10
 Operator : CG/JU
 Sample : 02122-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014561.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.369	28	31	38	rVB	27964	38409	0.99%	0.115%
2	3.846	109	112	122	rBV	18910	44869	1.16%	0.134%
3	4.028	137	143	148	rVB	12629	23042	0.60%	0.069%
4	4.122	156	159	165	rVB4	10068	13617	0.35%	0.041%
5	4.240	176	179	183	rVB6	6401	9250	0.24%	0.028%
6	5.058	315	318	324	rBV3	7728	13620	0.35%	0.041%
7	5.246	348	350	356	rVB7	2757	4038	0.10%	0.012%
8	6.369	537	541	547	rVB7	4869	8347	0.22%	0.025%
9	7.005	645	649	655	rVB9	2689	5667	0.15%	0.017%
10	7.175	672	678	690	rBV2	65817	160901	4.16%	0.482%
11	7.322	697	703	717	rBV	426243	699606	18.09%	2.094%
12	7.528	731	738	759	rBV	355025	707041	18.29%	2.116%
13	7.993	810	817	831	rBV	465653	766733	19.83%	2.295%
14	8.722	934	941	961	rBV	232282	531973	13.76%	1.592%
15	9.175	1010	1018	1030	rBV	517297	941868	24.36%	2.819%
16	9.540	1076	1080	1084	rVB6	5661	6995	0.18%	0.021%
17	9.899	1134	1141	1161	rBV	384693	731645	18.92%	2.190%
18	10.081	1166	1172	1178	rBV10	5953	15738	0.41%	0.047%
19	10.446	1227	1234	1257	rBV	359617	997555	25.80%	2.986%
20	10.816	1289	1297	1309	rBV	641202	1101701	28.49%	3.298%
21	10.975	1316	1324	1345	rBV	142064	431987	11.17%	1.293%
22	12.416	1564	1569	1576	rBV4	7852	15177	0.39%	0.045%
23	13.445	1740	1744	1748	rBV6	3354	5760	0.15%	0.017%
24	14.057	1837	1848	1862	rBV	1281632	2024884	52.37%	6.061%
25	14.339	1889	1896	1914	rBV	1462249	2231149	57.70%	6.678%
26	14.516	1922	1926	1929	rVB6	3465	5074	0.13%	0.015%
27	14.645	1941	1948	1957	rBV	1006393	1493753	38.63%	4.471%
28	14.945	1991	1999	2013	rBV10	17192	84994	2.20%	0.254%
29	15.469	2085	2088	2091	rBV5	4440	6640	0.17%	0.020%
30	15.581	2103	2107	2111	rBV7	2638	4957	0.13%	0.015%
31	15.639	2111	2117	2131	rBV	1847348	2787848	72.10%	8.345%
32	15.775	2134	2140	2149	rBV	369992	695165	17.98%	2.081%
33	16.016	2177	2181	2190	rVB	27282	47920	1.24%	0.143%
34	17.092	2358	2364	2368	rBV8	6152	12290	0.32%	0.037%
35	17.198	2380	2382	2386	rVB5	4384	4223	0.11%	0.013%
36	17.298	2396	2399	2401	rBV4	3492	4600	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014561.D
 Acq On : 05 Apr 2023 17:10
 Operator : CG/JU
 Sample : 02122-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9B8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	17.404	2410	2417	2428	rBV	1205061	1768480	45.74%	5.294%
38	17.504	2428	2434	2450	rVV	2060206	3130536	80.96%	9.371%
39	18.280	2561	2566	2574	rBV4	50147	108122	2.80%	0.324%
40	19.316	2738	2742	2747	rBV3	31303	41923	1.08%	0.125%
41	19.386	2750	2754	2760	rBV3	27329	53809	1.39%	0.161%
42	19.504	2771	2774	2781	rBV4	37069	66745	1.73%	0.200%
43	19.733	2808	2813	2821	rBV	2657677	3604971	93.23%	10.791%
44	21.169	3054	3057	3063	rBV5	66619	105908	2.74%	0.317%
45	21.492	3107	3112	3127	rBV	1243322	2001280	51.76%	5.990%
46	23.833	3503	3510	3525	rVB2	1900819	3866678	100.00%	11.574%
47	23.998	3532	3538	3556	rVB2	914253	1980547	51.22%	5.928%




Sum of corrected areas: 33408035

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014561.D
Acq On : 05 Apr 2023 17:10
Operator : CG/JU
Sample : 02122-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9B8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

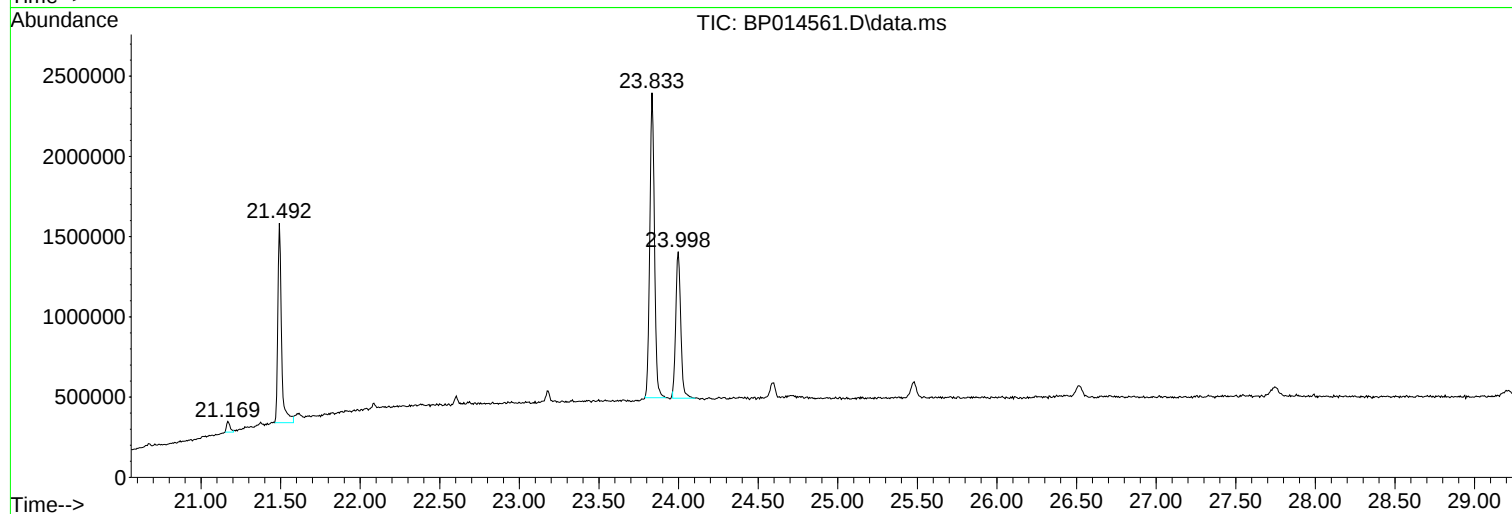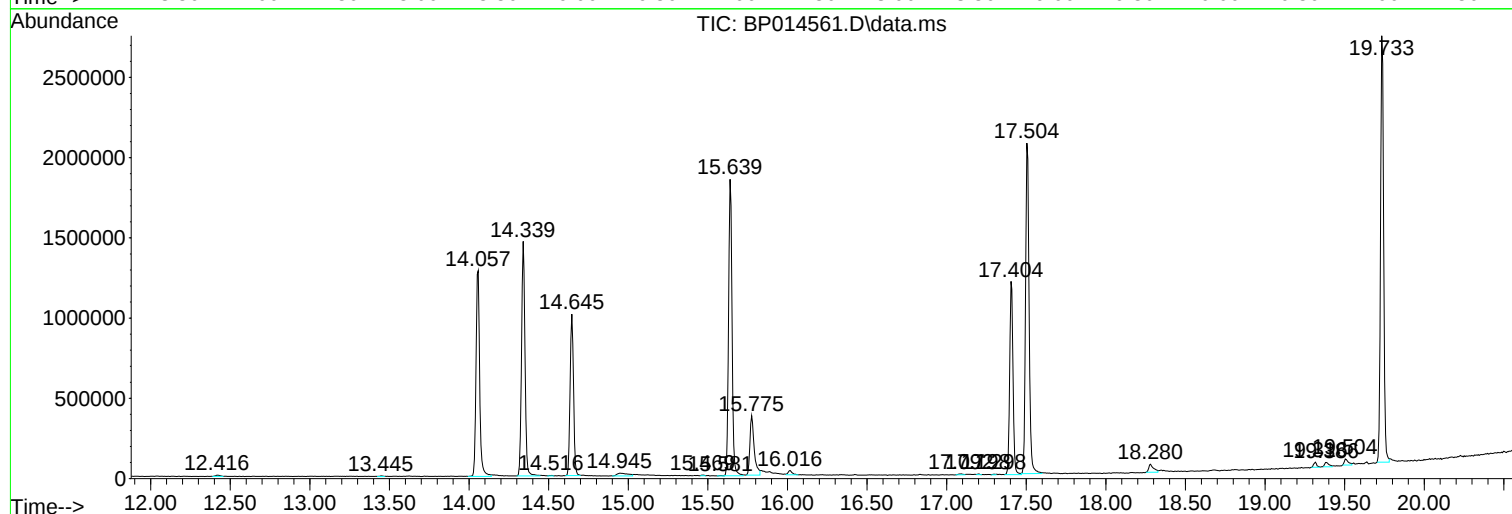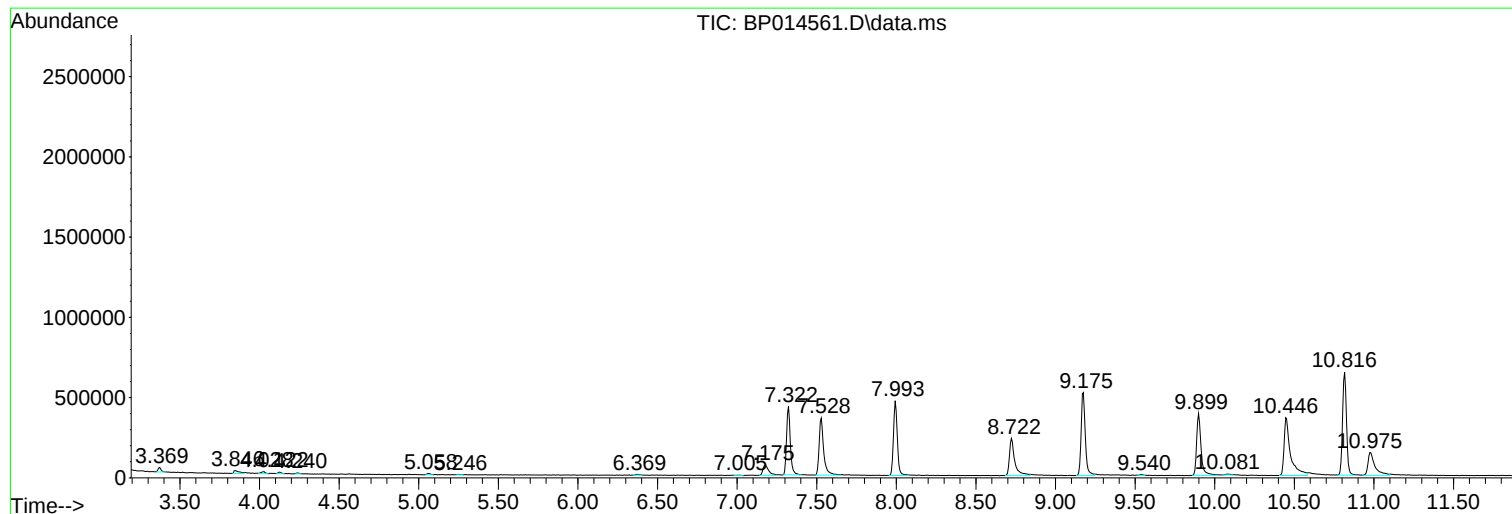

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014561.D
Acq On : 05 Apr 2023 17:10
Operator : CG/JU
Sample : 02122-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9B8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014561.D
Acq On : 05 Apr 2023 17:10
Operator : CG/JU
Sample : 02122-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9B8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
