

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014562.D
 Acq On : 05 Apr 2023 17:44
 Operator : CG/JU
 Sample : 02122-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9A8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014562.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	35	rBV	23022	29619	0.80%	0.094%
2	3.834	108	110	121	rBV	21175	44807	1.21%	0.142%
3	4.017	137	141	148	rVB2	12693	21427	0.58%	0.068%
4	4.123	156	159	166	rVB2	8500	13075	0.35%	0.041%
5	4.234	176	178	181	rVB3	5669	6249	0.17%	0.020%
6	5.058	314	318	324	rVB5	6861	10659	0.29%	0.034%
7	6.369	535	541	545	rBV7	5904	9982	0.27%	0.032%
8	7.069	658	660	667	rVB8	2497	4268	0.12%	0.014%
9	7.169	670	677	690	rBV	66739	165956	4.49%	0.525%
10	7.316	695	702	715	rBV	429274	730322	19.77%	2.311%
11	7.522	729	737	758	rBV	364851	744175	20.15%	2.355%
12	7.987	809	816	827	rBV	403849	678180	18.36%	2.146%
13	8.058	827	828	833	rVB4	3747	3866	0.10%	0.012%
14	8.716	932	940	960	rBV	232761	540076	14.62%	1.709%
15	8.875	965	967	972	rVB6	2762	3999	0.11%	0.013%
16	9.163	1008	1016	1033	rBV	537960	984837	26.66%	3.117%
17	9.528	1074	1078	1083	rVB3	7539	12305	0.33%	0.039%
18	9.893	1132	1140	1158	rBV	398263	771360	20.88%	2.441%
19	10.069	1167	1170	1172	rBV4	5002	6568	0.18%	0.021%
20	10.440	1226	1233	1255	rBV	379603	1016824	27.53%	3.218%
21	10.810	1289	1296	1311	rVB	563602	981493	26.57%	3.106%
22	10.969	1316	1323	1347	rBV2	147627	437290	11.84%	1.384%
23	11.210	1363	1364	1370	rVB6	2625	4078	0.11%	0.013%
24	12.216	1531	1535	1539	rBV6	2850	4885	0.13%	0.015%
25	12.416	1563	1569	1579	rBV7	8236	19862	0.54%	0.063%
26	13.099	1681	1685	1690	rBV7	2050	3972	0.11%	0.013%
27	13.440	1740	1743	1750	rVB8	4858	8049	0.22%	0.025%
28	13.610	1767	1772	1775	rBV6	3248	4741	0.13%	0.015%
29	14.046	1837	1846	1862	rBV	1200986	1950983	52.82%	6.174%
30	14.334	1888	1895	1914	rBV	1435373	2166115	58.64%	6.855%
31	14.510	1922	1925	1928	rVB5	2875	3969	0.11%	0.013%
32	14.640	1940	1947	1961	rBV	910247	1327115	35.93%	4.200%
33	14.951	1993	2000	2003	rBV7	14188	37100	1.00%	0.117%
34	15.463	2084	2087	2091	rBV6	3176	5037	0.14%	0.016%
35	15.634	2110	2116	2131	rBV	1753549	2722962	73.72%	8.617%
36	15.769	2133	2139	2154	rBV	360028	708668	19.19%	2.243%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014562.D
 Acq On : 05 Apr 2023 17:44
 Operator : CG/JU
 Sample : 02122-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9A8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	16.010	2175	2180	2189	rVB	27429	48655	1.32%	0.154%
38	16.528	2263	2268	2271	rBV7	4142	7482	0.20%	0.024%
39	17.081	2358	2362	2364	rBV5	3972	5070	0.14%	0.016%
40	17.187	2375	2380	2382	rBV6	3768	7558	0.20%	0.024%
41	17.398	2410	2416	2426	rBV	1049924	1560816	42.26%	4.939%
42	17.504	2427	2434	2458	rVV	2005784	3062200	82.90%	9.691%
43	18.281	2562	2566	2572	rBV7	22594	52148	1.41%	0.165%
44	19.310	2738	2741	2745	rVB4	27624	37443	1.01%	0.118%
45	19.381	2750	2753	2758	rVV3	19686	29449	0.80%	0.093%
46	19.733	2807	2813	2823	rBV	2514082	3502843	94.83%	11.085%
47	21.163	3053	3056	3065	rBV7	75516	161326	4.37%	0.511%
48	21.486	3107	3111	3123	rBV	989145	1606437	43.49%	5.084%
49	23.827	3502	3509	3523	rVB2	1770676	3693799	100.00%	11.689%
50	23.992	3531	3537	3548	rVB2	741686	1639843	44.39%	5.189%




Sum of corrected areas: 31599942

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014562.D
Acq On : 05 Apr 2023 17:44
Operator : CG/JU
Sample : 02122-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

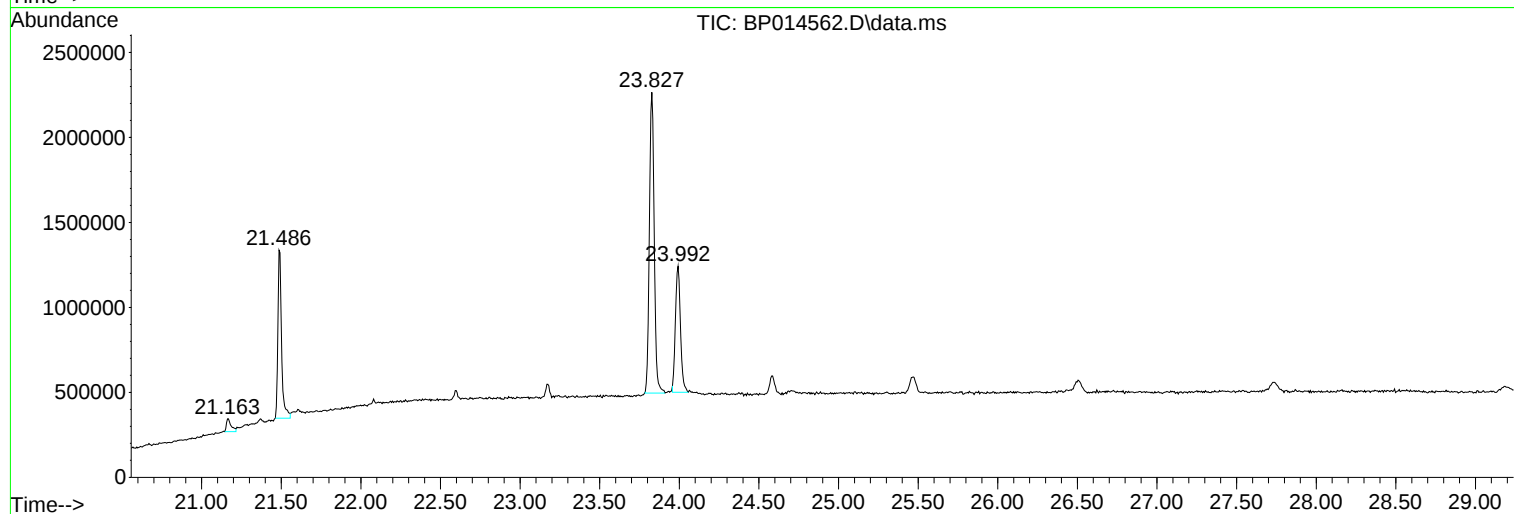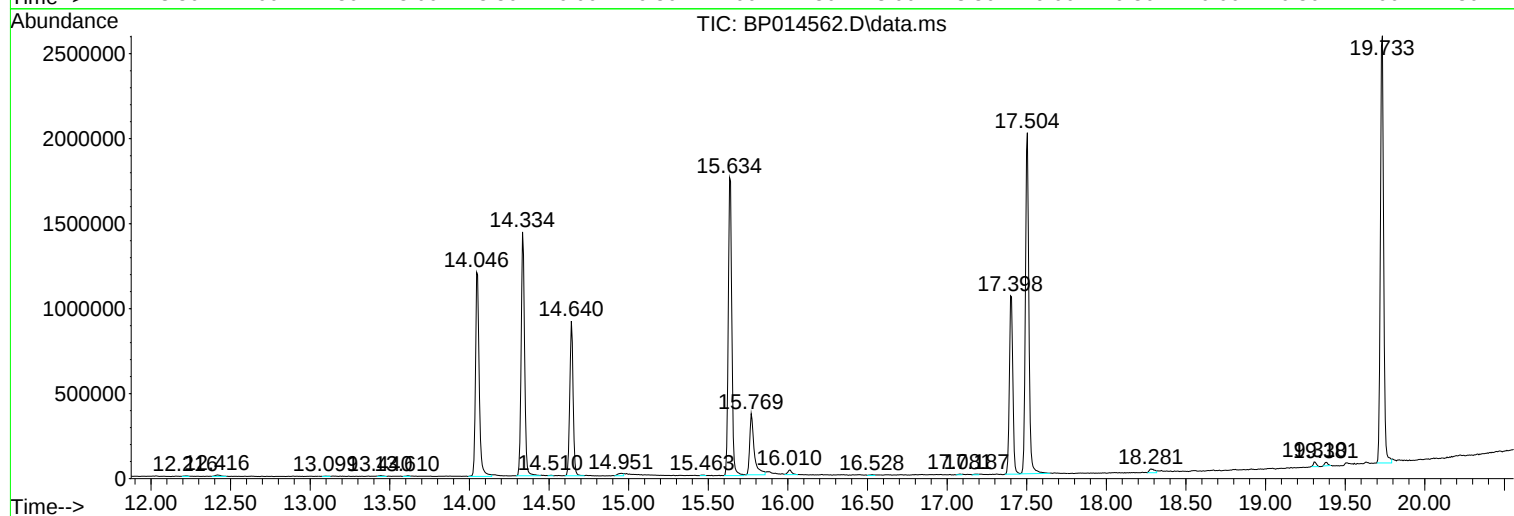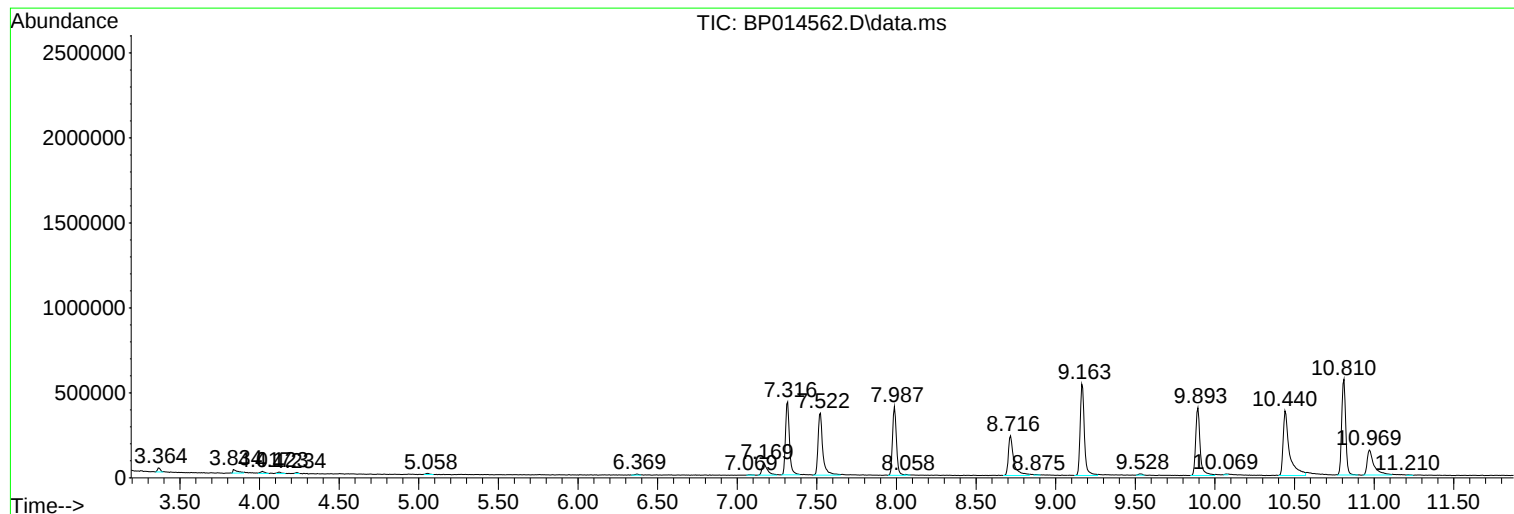

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014562.D
Acq On : 05 Apr 2023 17:44
Operator : CG/JU
Sample : 02122-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A8










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic21.163 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.163	2.01 ng/ul	161326	Chrysene-d12	21.486

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Cyclotetracosane	336	C24H48	000297-03-0	98
2		2- Chloropropionic acid, octadec...	360	C21H41ClO2	088104-31-8	94
3		Cyclotriacontane	420	C30H60	000297-35-8	93
4		Pentacos-1-ene	350	C25H50	016980-85-1	90
5		Triacontyl acetate	480	C32H64O2	041755-58-2	90

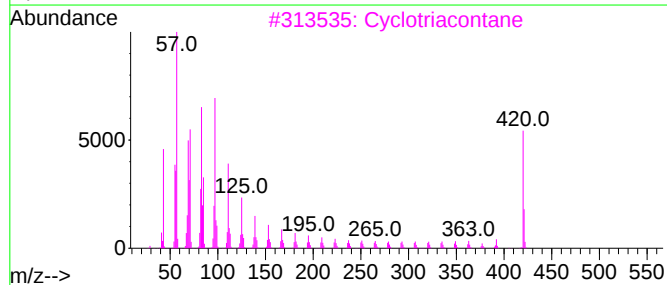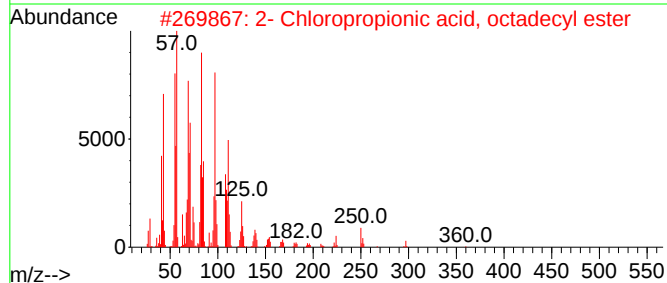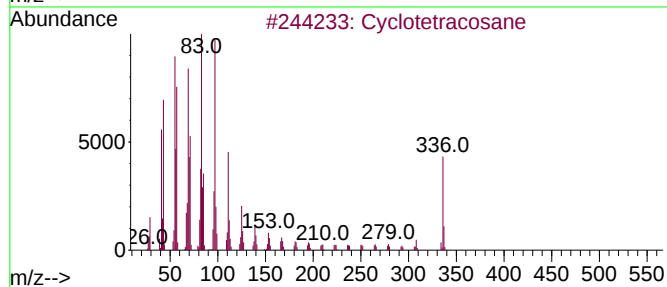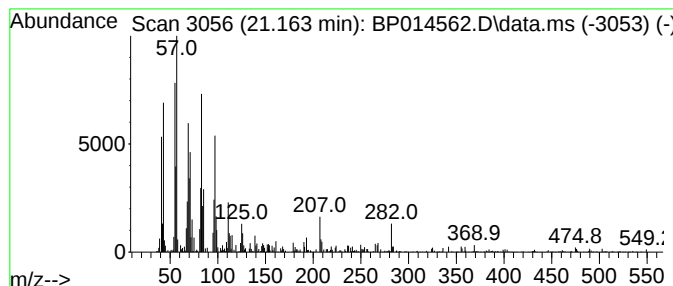

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014562.D
Acq On : 05 Apr 2023 17:44
Operator : CG/JU
Sample : 02122-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9A8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	21.163	2.0	ng/u1	161326	5	21.486	1606440	20.0