

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014563.D
 Acq On : 05 Apr 2023 18:18
 Operator : CG/JU
 Sample : 02122-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9B2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014563.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	27	31	39	rVB	26365	35377	1.26%	0.132%
2	3.817	105	107	126	rBV	67957	150964	5.39%	0.563%
3	4.017	137	141	147	rVB2	13473	20135	0.72%	0.075%
4	4.122	155	159	166	rVB4	9910	16919	0.60%	0.063%
5	4.234	175	178	184	rVB7	6594	9333	0.33%	0.035%
6	4.393	202	205	208	rBV5	2646	3514	0.13%	0.013%
7	4.734	259	263	264	rBV4	2249	2880	0.10%	0.011%
8	5.052	313	317	321	rBV	6732	8946	0.32%	0.033%
9	5.169	334	337	339	rVB3	2961	3217	0.11%	0.012%
10	6.375	536	542	547	rVB9	5636	11347	0.40%	0.042%
11	6.587	575	578	585	rVB8	2017	3758	0.13%	0.014%
12	7.169	671	677	689	rBV2	39167	105399	3.76%	0.393%
13	7.316	696	702	718	rBV	315766	541138	19.31%	2.017%
14	7.522	731	737	758	rBV	239464	496229	17.70%	1.849%
15	7.987	808	816	828	rBV	430720	716921	25.58%	2.672%
16	8.722	934	941	964	rBV	143717	366829	13.09%	1.367%
17	8.899	970	971	976	rVB5	2756	2867	0.10%	0.011%
18	9.169	1009	1017	1031	rBV	374914	714221	25.48%	2.662%
19	9.534	1074	1079	1085	rVB5	6546	11394	0.41%	0.042%
20	9.893	1133	1140	1159	rBV	259494	519425	18.53%	1.936%
21	10.105	1172	1176	1181	rVB8	2675	5788	0.21%	0.022%
22	10.446	1226	1234	1255	rBV	255895	712721	25.43%	2.656%
23	10.810	1288	1296	1309	rBV	582810	1048372	37.40%	3.907%
24	10.963	1315	1322	1348	rBV	215774	630338	22.49%	2.349%
25	11.163	1355	1356	1363	rVB7	2382	3056	0.11%	0.011%
26	12.216	1530	1535	1540	rBV9	4130	7670	0.27%	0.029%
27	12.357	1554	1559	1560	rBV5	7291	8892	0.32%	0.033%
28	12.410	1565	1568	1576	rVV8	7958	19365	0.69%	0.072%
29	13.446	1738	1744	1749	rBV8	5512	10471	0.37%	0.039%
30	14.045	1838	1846	1874	rBV	909072	1554575	55.46%	5.793%
31	14.334	1887	1895	1910	rBV	1109506	1673615	59.71%	6.237%
32	14.640	1938	1947	1966	rBV	970676	1434953	51.19%	5.347%
33	14.963	1997	2002	2006	rBV7	8676	21093	0.75%	0.079%
34	15.463	2083	2087	2091	rBV4	6932	11330	0.40%	0.042%
35	15.569	2102	2105	2108	rBV5	2493	3568	0.13%	0.013%
36	15.634	2110	2116	2133	rBV	1333027	2107682	75.19%	7.854%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014563.D
 Acq On : 05 Apr 2023 18:18
 Operator : CG/JU
 Sample : 02122-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9B2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	15.775	2134	2140	2155	rBV2	218963	479262	17.10%	1.786%
38	16.010	2175	2180	2189	rVB2	23508	44133	1.57%	0.164%
39	16.204	2211	2213	2220	rVB8	2680	4444	0.16%	0.017%
40	16.916	2330	2334	2335	rBV4	2545	2955	0.11%	0.011%
41	17.075	2359	2361	2365	rBV5	3501	5091	0.18%	0.019%
42	17.192	2379	2381	2384	rVB4	3074	3335	0.12%	0.012%
43	17.404	2410	2417	2427	rBV	1095148	1652112	58.94%	6.157%
44	17.504	2427	2434	2448	rVV	1494537	2373982	84.69%	8.847%
45	18.281	2562	2566	2573	rBV8	19527	44265	1.58%	0.165%
46	19.310	2738	2741	2746	rVB4	20577	25779	0.92%	0.096%
47	19.733	2807	2813	2827	rBV	1948702	2782219	99.26%	10.368%
48	21.163	3053	3056	3064	rBV4	108841	173423	6.19%	0.646%
49	21.486	3106	3111	3124	rBV	1069542	1781535	63.56%	6.639%
50	23.827	3502	3509	3524	rVB	1318883	2802991	100.00%	10.445%
51	23.986	3530	3536	3549	rVB2	763284	1664663	59.39%	6.203%




Sum of corrected areas: 26834491

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014563.D
Acq On : 05 Apr 2023 18:18
Operator : CG/JU
Sample : 02122-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9B2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

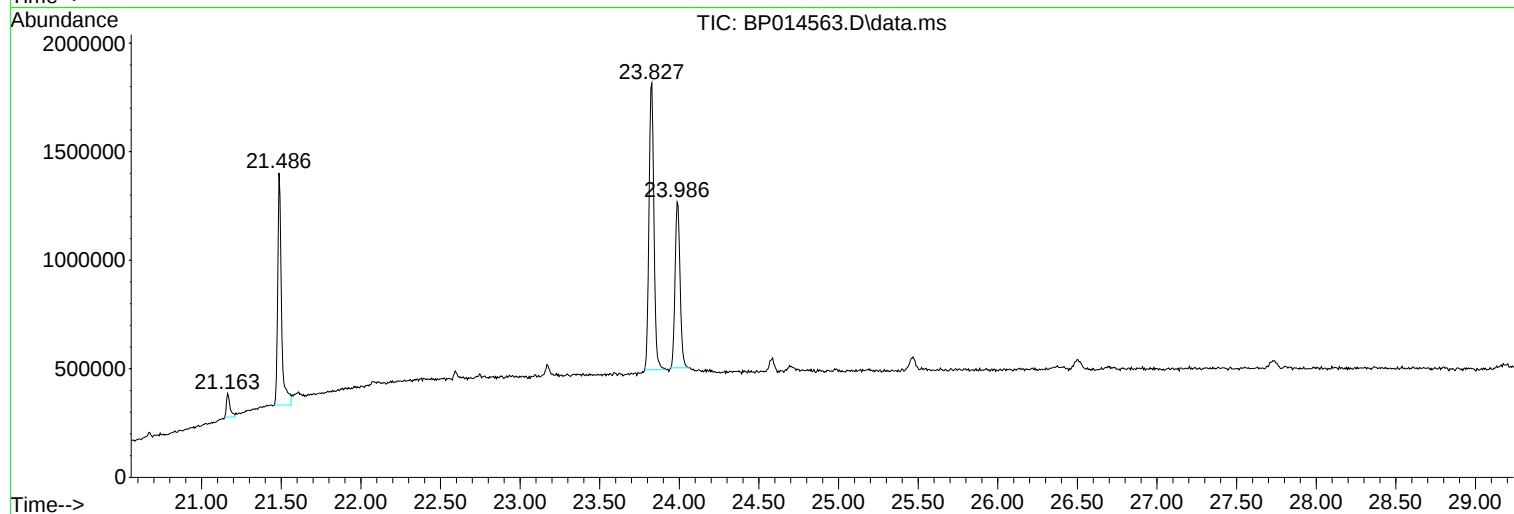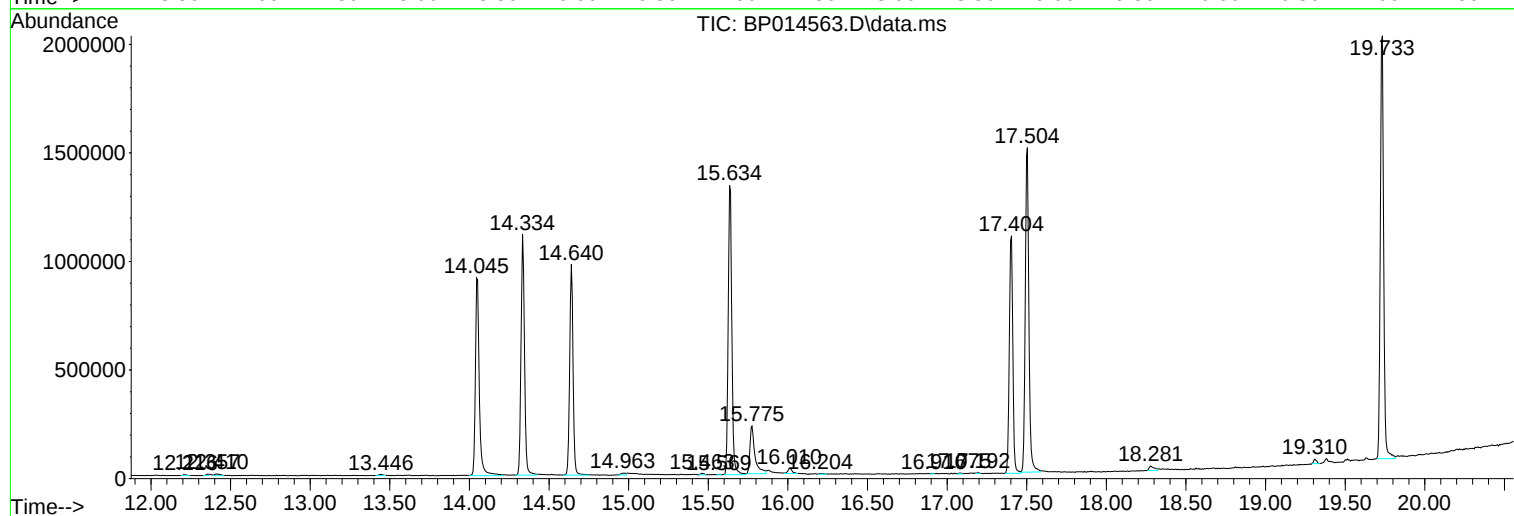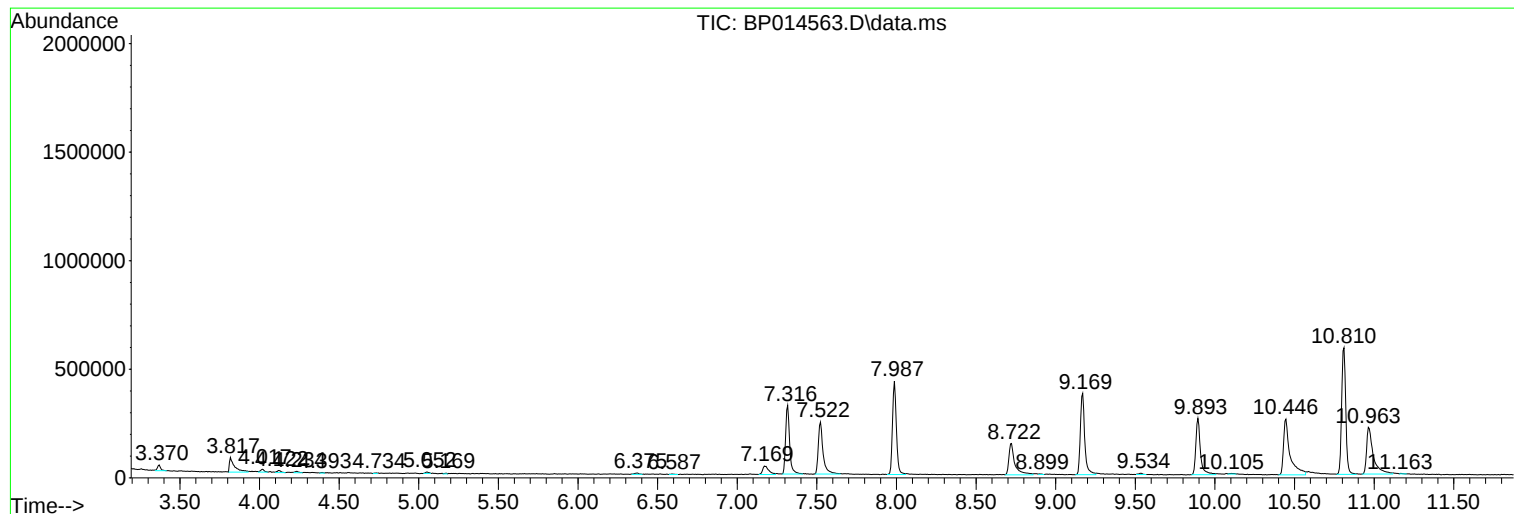

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014563.D
Acq On : 05 Apr 2023 18:18
Operator : CG/JU
Sample : 02122-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9B2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014563.D
Acq On : 05 Apr 2023 18:18
Operator : CG/JU
Sample : 02122-10
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9B2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc