

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014564.D
 Acq On : 05 Apr 2023 18:51
 Operator : CG/JU
 Sample : 02122-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9C8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014564.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	39	rVB	36637	48049	1.46%	0.155%
2	3.817	105	107	124	rBV	58818	125890	3.82%	0.405%
3	4.017	137	141	147	rVB2	14143	22827	0.69%	0.073%
4	4.123	156	159	162	rVB3	8370	11025	0.33%	0.035%
5	4.228	174	177	183	rVB5	8406	12368	0.38%	0.040%
6	5.052	313	317	323	rVB3	10334	15967	0.48%	0.051%
7	5.228	345	347	350	rBV3	2544	3510	0.11%	0.011%
8	5.340	362	366	371	rBV8	2660	3520	0.11%	0.011%
9	5.617	409	413	415	rBV4	3113	4252	0.13%	0.014%
10	6.375	538	542	550	rVB8	6779	14449	0.44%	0.046%
11	7.081	658	662	666	rVB6	2387	4305	0.13%	0.014%
12	7.169	671	677	694	rBV3	58205	152622	4.63%	0.491%
13	7.317	695	702	716	rVV	411772	700728	21.26%	2.254%
14	7.522	730	737	759	rBV	321469	654002	19.84%	2.104%
15	7.987	809	816	826	rBV	457922	754309	22.88%	2.427%
16	8.058	826	828	831	rVB4	3559	3705	0.11%	0.012%
17	8.158	843	845	849	rBV4	2537	3620	0.11%	0.012%
18	8.716	933	940	963	rBV	208408	496850	15.07%	1.599%
19	9.163	1008	1016	1037	rBV	493002	943068	28.61%	3.034%
20	9.528	1072	1078	1083	rVB7	6654	14190	0.43%	0.046%
21	9.893	1129	1140	1155	rBV	332105	633301	19.21%	2.038%
22	10.069	1165	1170	1171	rBV5	3587	4197	0.13%	0.014%
23	10.440	1225	1233	1263	rBV	366421	952505	28.90%	3.065%
24	10.810	1289	1296	1311	rVB	627530	1114604	33.82%	3.586%
25	10.963	1314	1322	1347	rBV	332109	886325	26.89%	2.852%
26	12.422	1563	1570	1573	rBV5	6471	13823	0.42%	0.044%
27	13.616	1770	1773	1779	rBV7	2931	4065	0.12%	0.013%
28	14.046	1838	1846	1865	rBV	1138721	1876353	56.93%	6.037%
29	14.334	1888	1895	1907	rBV	1398880	2099755	63.70%	6.756%
30	14.640	1940	1947	1959	rBV	1030687	1512243	45.88%	4.865%
31	14.963	1997	2002	2003	rBV5	9143	13089	0.40%	0.042%
32	15.463	2084	2087	2092	rVB7	3439	4684	0.14%	0.015%
33	15.634	2110	2116	2132	rBV	1679478	2627472	79.71%	8.453%
34	15.775	2134	2140	2155	rBV	237291	521392	15.82%	1.677%
35	16.422	2247	2250	2254	rBV6	2753	3916	0.12%	0.013%
36	17.081	2359	2362	2367	rVB7	4757	6604	0.20%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014564.D
 Acq On : 05 Apr 2023 18:51
 Operator : CG/JU
 Sample : 02122-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9C8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	17.204	2377	2383	2386	rVB8	3129	5519	0.17%	0.018%
38	17.398	2410	2416	2426	rBV	1155922	1738524	52.74%	5.593%
39	17.498	2427	2433	2453	rVV	1913483	2968592	90.06%	9.551%
40	18.287	2564	2567	2575	rBV8	13226	30883	0.94%	0.099%
41	19.310	2738	2741	2746	rVB3	23138	30970	0.94%	0.100%
42	19.381	2750	2753	2760	rVB2	19303	35471	1.08%	0.114%
43	19.733	2807	2813	2827	rBV	2281407	3279756	99.50%	10.552%
44	21.486	3107	3111	3125	rBV	1027224	1642786	49.84%	5.285%
45	23.827	3502	3509	3523	rVB2	1590300	3296121	100.00%	10.605%
46	23.992	3531	3537	3551	rVB2	803525	1789525	54.29%	5.757%




Sum of corrected areas: 31081731

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014564.D
Acq On : 05 Apr 2023 18:51
Operator : CG/JU
Sample : 02122-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9C8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

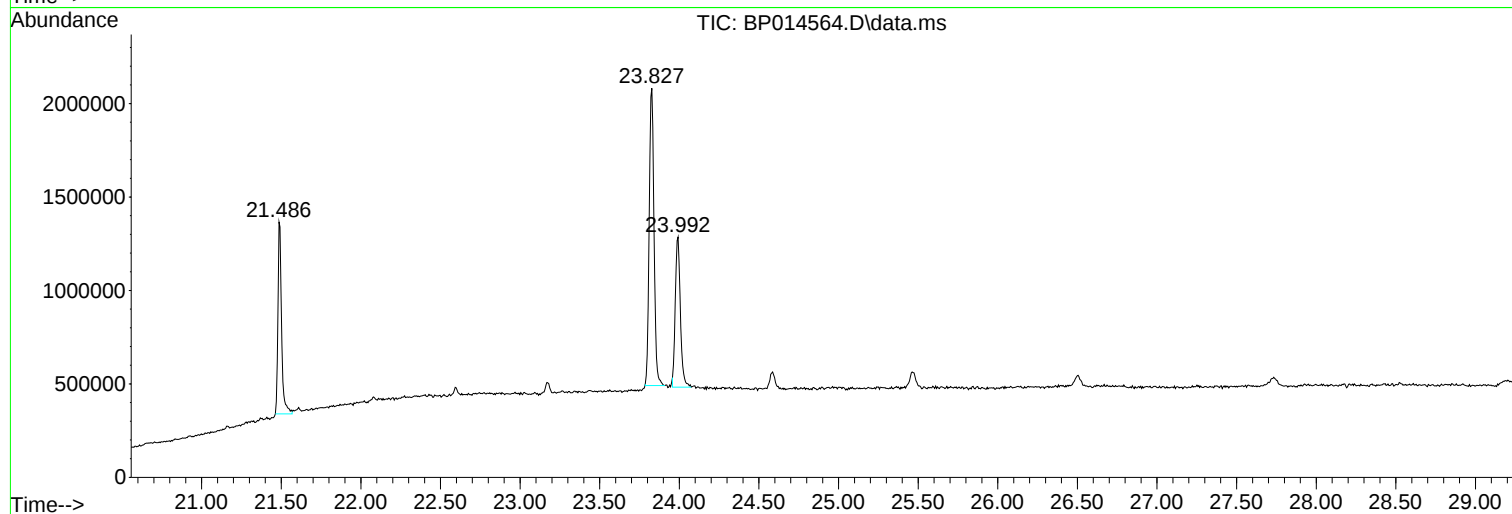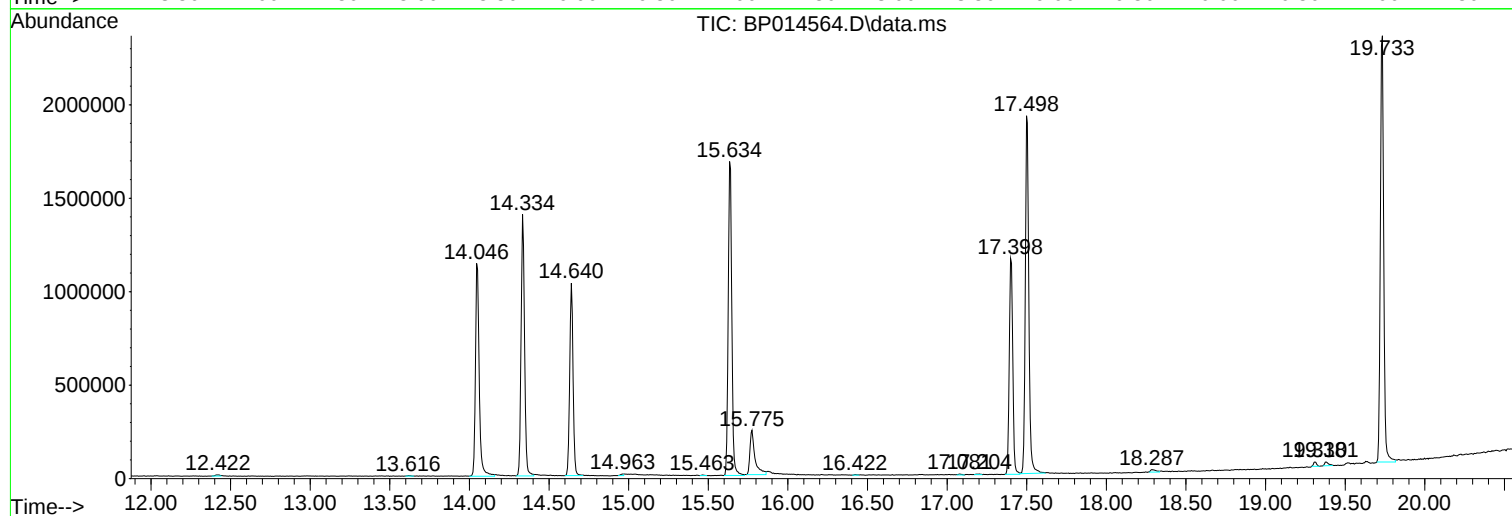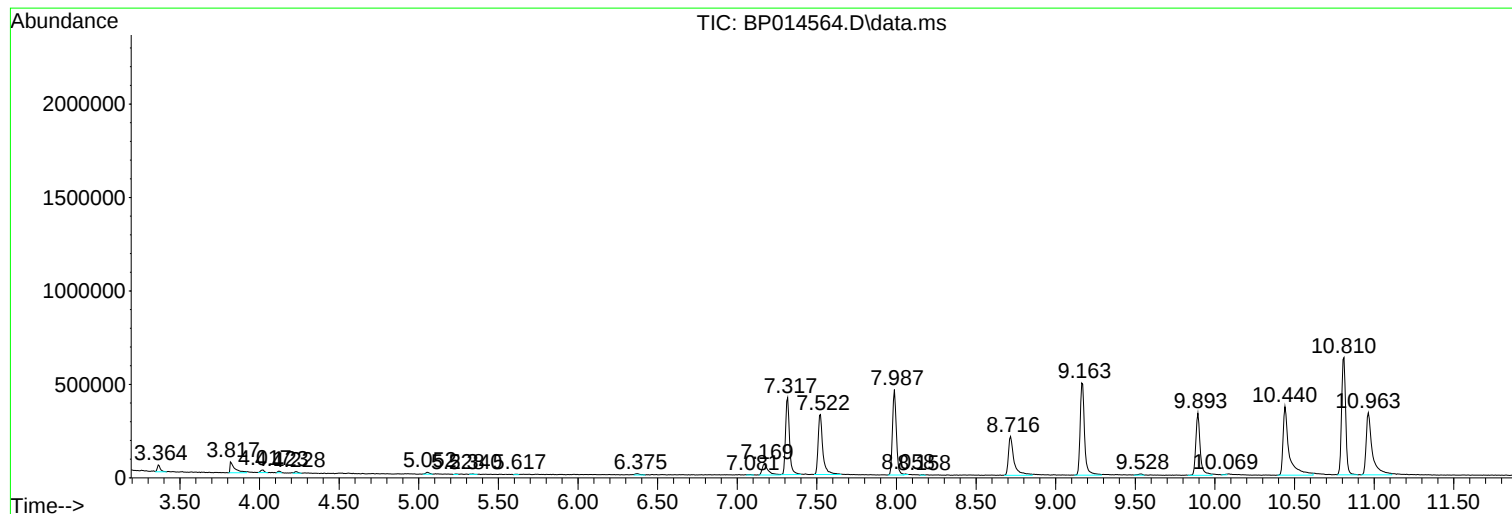

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014564.D
Acq On : 05 Apr 2023 18:51
Operator : CG/JU
Sample : 02122-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9C8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014564.D
Acq On : 05 Apr 2023 18:51
Operator : CG/JU
Sample : 02122-14
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9C8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc