

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014565.D
 Acq On : 05 Apr 2023 19:25
 Operator : CG/JU
 Sample : 02122-15
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB9C9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014565.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	27	31	40	rVB	34010	52138	1.18%	0.133%
2	3.828	108	109	121	rBV	29794	66954	1.51%	0.171%
3	4.017	137	141	149	rVB2	18140	29909	0.68%	0.076%
4	4.123	155	159	169	rVB2	11058	14992	0.34%	0.038%
5	4.228	174	177	182	rVB4	9706	14904	0.34%	0.038%
6	5.052	313	317	324	rBV2	11476	17891	0.40%	0.046%
7	6.375	535	542	546	rVB5	6915	12245	0.28%	0.031%
8	7.164	670	676	693	rBV	81877	203409	4.60%	0.518%
9	7.316	695	702	717	rVV	502761	853112	19.27%	2.173%
10	7.516	730	736	755	rBV	437329	841352	19.01%	2.143%
11	7.987	809	816	830	rBV	518126	873044	19.72%	2.224%
12	8.275	858	865	869	rBV9	4683	10224	0.23%	0.026%
13	8.711	932	939	954	rBV	289871	630090	14.23%	1.605%
14	9.163	1009	1016	1035	rBV	651259	1163808	26.29%	2.965%
15	9.528	1075	1078	1083	rVB6	4685	6584	0.15%	0.017%
16	9.893	1133	1140	1158	rBV	480253	921603	20.82%	2.348%
17	10.087	1171	1173	1180	rVB8	4490	7707	0.17%	0.020%
18	10.440	1224	1233	1257	rBV	501621	1241690	28.05%	3.163%
19	10.805	1288	1295	1307	rBV	748259	1322297	29.87%	3.368%
20	10.963	1314	1322	1345	rBV	253843	670967	15.16%	1.709%
21	12.416	1563	1569	1582	rVB	9687	25983	0.59%	0.066%
22	14.046	1838	1846	1869	rBV	1532858	2425409	54.79%	6.178%
23	14.334	1885	1895	1913	rBV	1780289	2703200	61.07%	6.886%
24	14.640	1939	1947	1959	rBV	1253261	1887342	42.64%	4.808%
25	14.940	1991	1998	2000	rBV6	16581	36589	0.83%	0.093%
26	15.634	2110	2116	2131	rBV	2267156	3397858	76.76%	8.656%
27	15.769	2133	2139	2155	rVV	522125	990588	22.38%	2.523%
28	15.875	2155	2157	2169	rVB8	17994	39179	0.89%	0.100%
29	16.428	2246	2251	2253	rBV6	3979	4878	0.11%	0.012%
30	17.028	2351	2353	2357	rBV4	3346	4681	0.11%	0.012%
31	17.081	2360	2362	2365	rVB4	4410	4460	0.10%	0.011%
32	17.192	2377	2381	2386	rBV7	4500	7886	0.18%	0.020%
33	17.398	2407	2416	2427	rBV	1621457	2294088	51.83%	5.844%
34	17.498	2427	2433	2451	rVV2	2601438	3934951	88.90%	10.024%
35	18.051	2524	2527	2533	rVB7	6587	10459	0.24%	0.027%
36	19.304	2737	2740	2747	rBV2	33987	50630	1.14%	0.129%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014565.D
Acq On : 05 Apr 2023 19:25
Operator : CG/JU
Sample : 02122-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9C9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION

37	19.381	2749	2753	2761	rVV2	28874	48601	1.10%	0.124%
38	19.733	2807	2813	2825	rBV	3050794	4426356	100.00%	11.276%
39	21.486	3106	3111	3125	rBV	1288650	2226317	50.30%	5.671%
40	23.827	3502	3509	3527	rVB	1795156	3841523	86.79%	9.786%
41	23.992	3530	3537	3548	rVV2	875527	1940045	43.83%	4.942%




Sum of corrected areas: 39255943

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014565.D
Acq On : 05 Apr 2023 19:25
Operator : CG/JU
Sample : 02122-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9C9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

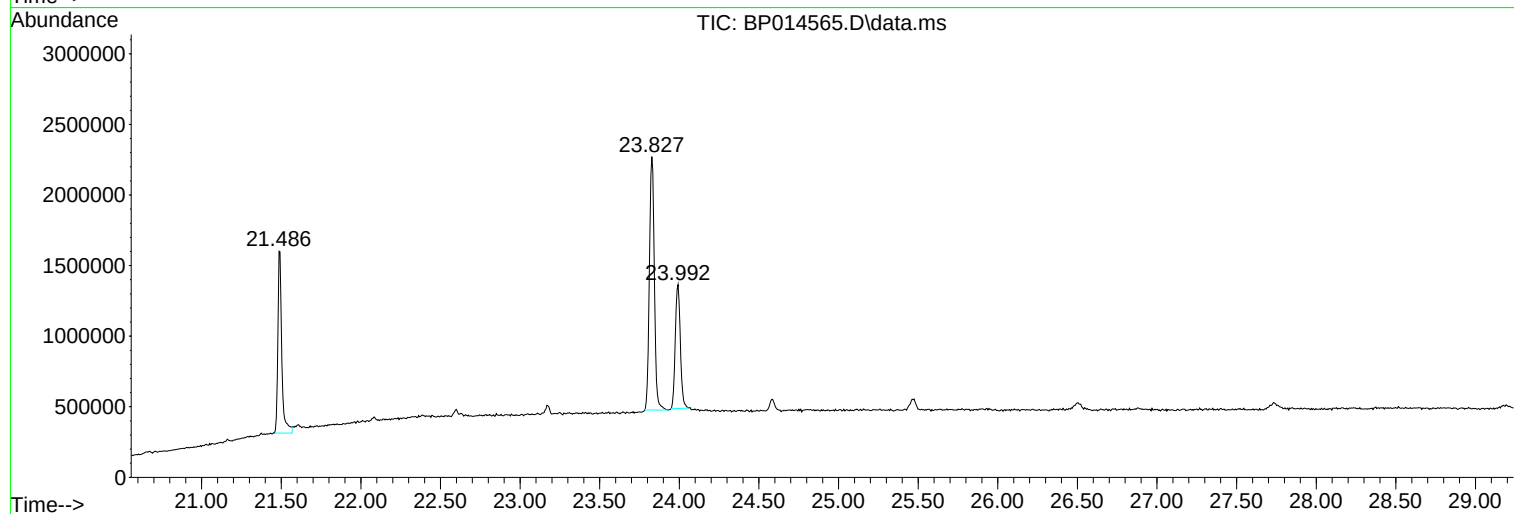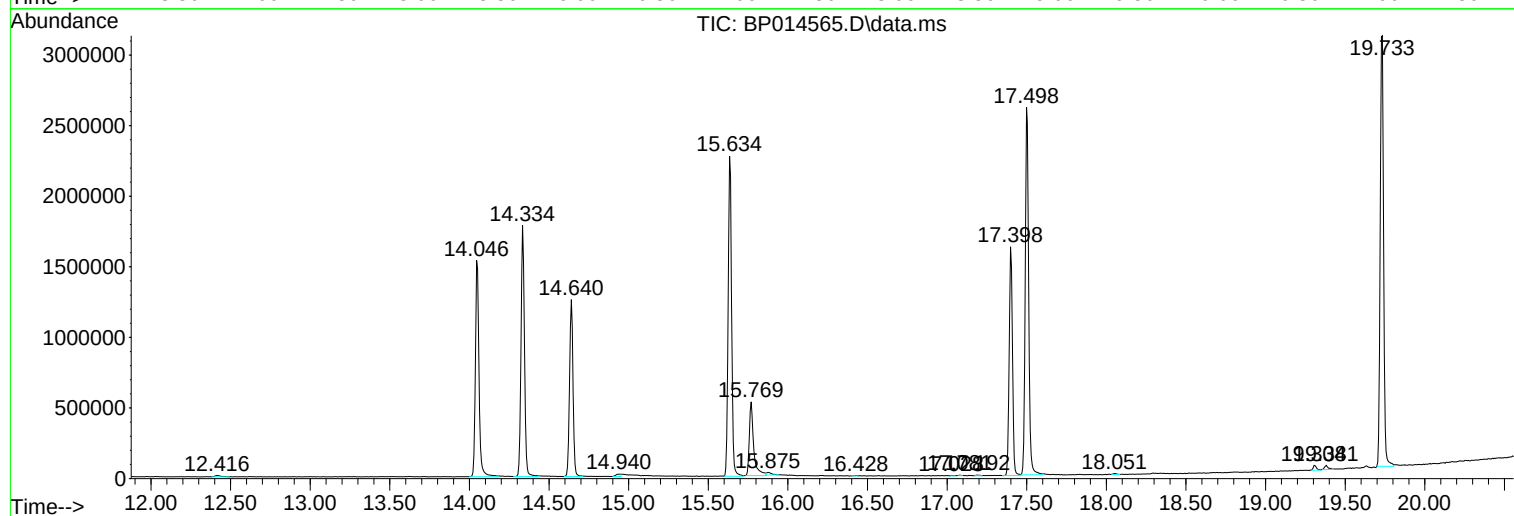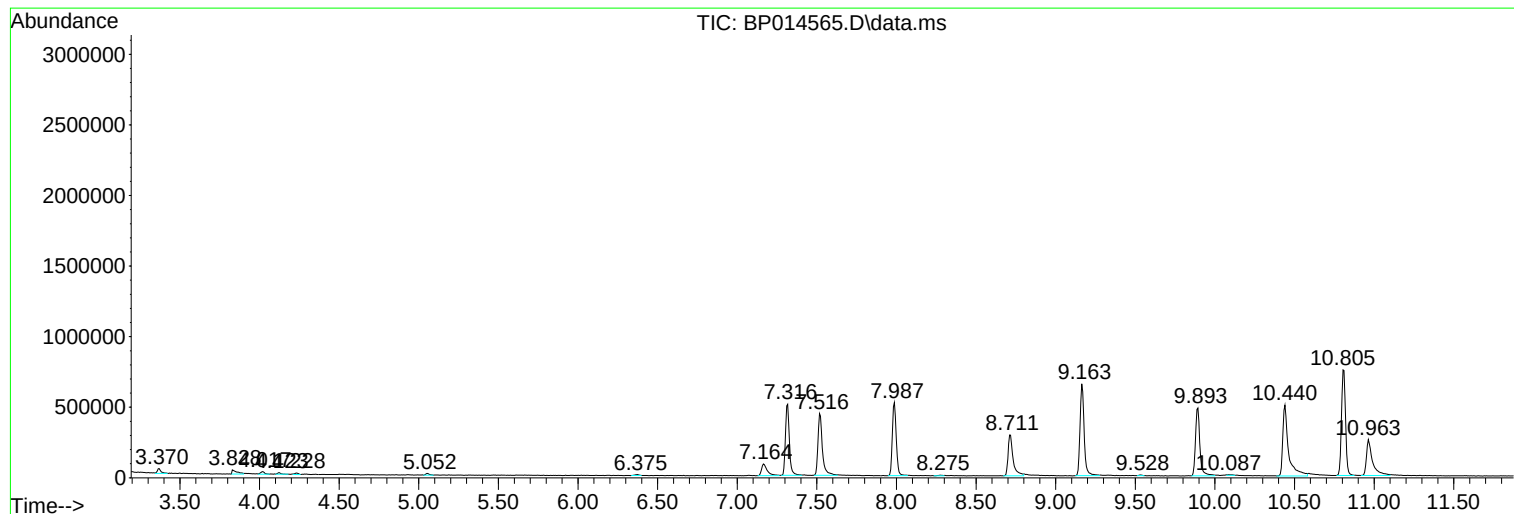

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014565.D
Acq On : 05 Apr 2023 19:25
Operator : CG/JU
Sample : 02122-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9C9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014565.D
Acq On : 05 Apr 2023 19:25
Operator : CG/JU
Sample : 02122-15
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB9C9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc