

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014571.D
 Acq On : 05 Apr 2023 23:21
 Operator : CG/JU
 Sample : PB151872BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK872

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014571.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	38	rVB	42747	61662	1.91%	0.177%
2	3.799	102	104	125	rBV	365659	642235	19.90%	1.847%
3	4.123	155	159	164	rVB2	10417	14752	0.46%	0.042%
4	5.687	423	425	429	rVB4	2936	3508	0.11%	0.010%
5	7.152	668	674	695	rVV	469324	964561	29.89%	2.774%
6	7.311	695	701	720	rVB	477521	797174	24.70%	2.293%
7	7.516	729	736	757	rBV	559888	993256	30.78%	2.856%
8	7.775	778	780	786	rVB7	2103	3901	0.12%	0.011%
9	7.987	809	816	828	rBV	449210	761133	23.58%	2.189%
10	8.711	932	939	952	rBV	568208	1134955	35.17%	3.264%
11	9.163	1009	1016	1031	rBV	555641	1007736	31.22%	2.898%
12	9.887	1130	1139	1166	rBV	448523	853350	26.44%	2.454%
13	10.434	1226	1232	1256	rBV	484254	1144001	35.45%	3.290%
14	10.805	1288	1295	1308	rVB	638274	1101183	34.12%	3.167%
15	10.957	1312	1321	1346	rBV	406347	1068096	33.09%	3.072%
16	12.416	1564	1569	1577	rBV10	7521	20137	0.62%	0.058%
17	13.516	1754	1756	1760	rBV5	3226	3835	0.12%	0.011%
18	14.046	1840	1846	1861	rBV	1159676	1870492	57.96%	5.379%
19	14.187	1868	1870	1875	rVB6	3417	4309	0.13%	0.012%
20	14.334	1888	1895	1912	rBV2	1370159	2147448	66.54%	6.176%
21	14.640	1940	1947	1957	rBV	948193	1459715	45.23%	4.198%
22	14.887	1983	1989	2014	rBV2	123569	579425	17.95%	1.666%
23	15.634	2109	2116	2129	rBV	1763927	2640498	81.82%	7.594%
24	15.763	2133	2138	2154	rBV	413272	746865	23.14%	2.148%
25	17.069	2358	2360	2366	rVB7	4091	6908	0.21%	0.020%
26	17.398	2410	2416	2426	rBV	1176246	1711586	53.03%	4.922%
27	17.498	2427	2433	2457	rVB2	1802513	2838547	87.95%	8.163%
28	18.339	2574	2576	2579	rBV4	5140	4993	0.15%	0.014%
29	19.304	2737	2740	2747	rBV5	24495	35854	1.11%	0.103%
30	19.381	2750	2753	2762	rVB3	16670	28957	0.90%	0.083%
31	19.728	2806	2812	2826	rBV	2287791	3227398	100.00%	9.281%
32	21.486	3106	3111	3125	rBV	1057736	1863845	57.75%	5.360%
33	23.827	3502	3509	3522	rVB	1529620	3209685	99.45%	9.231%
34	23.986	3530	3536	3549	rVB2	824700	1820450	56.41%	5.235%

Sum of corrected areas: 34772450




Instrument :
BNA_P
ClientSampleId :
SBLK872

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014571.D
Acq On : 05 Apr 2023 23:21
Operator : CG/JU
Sample : PB151872BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK872

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

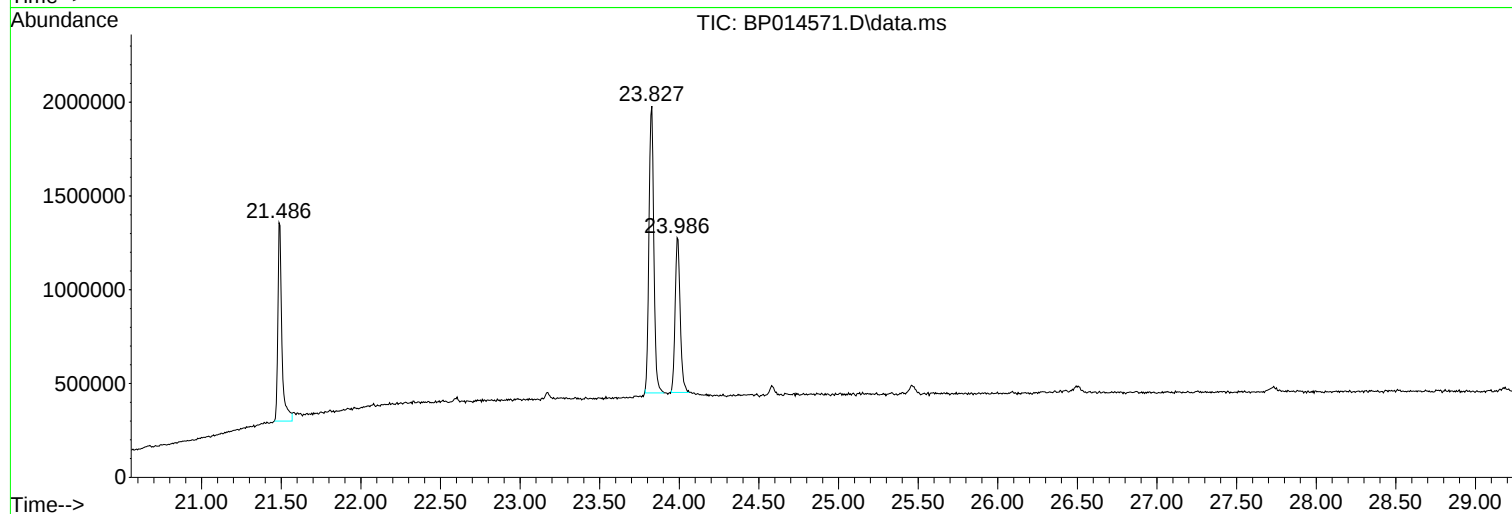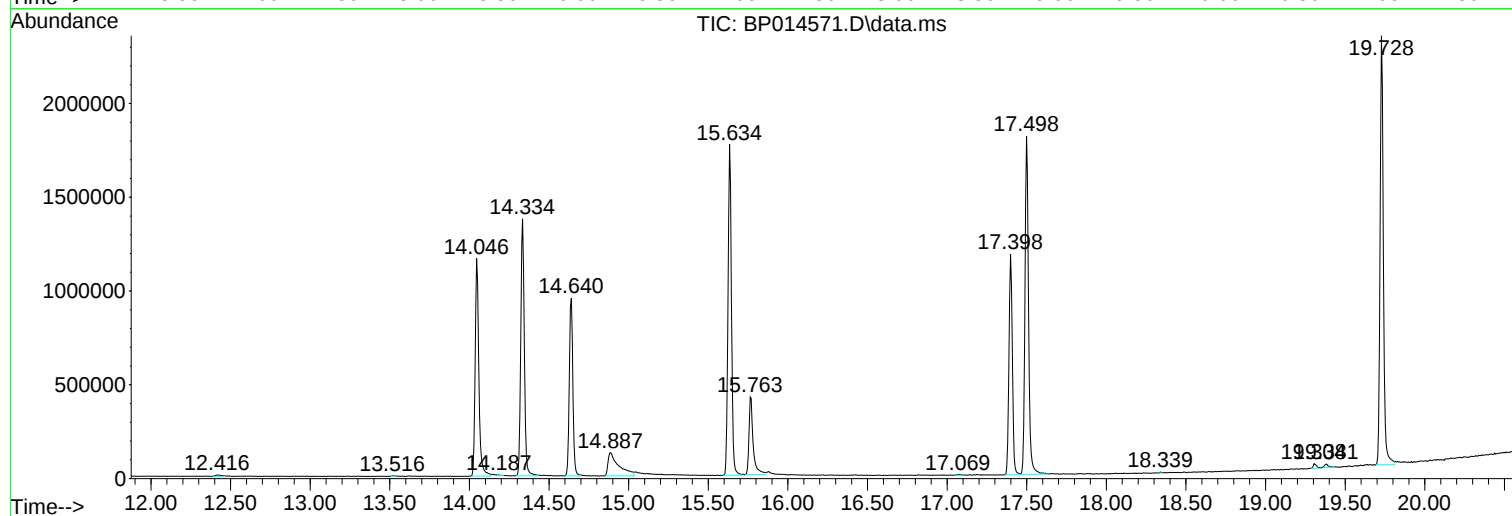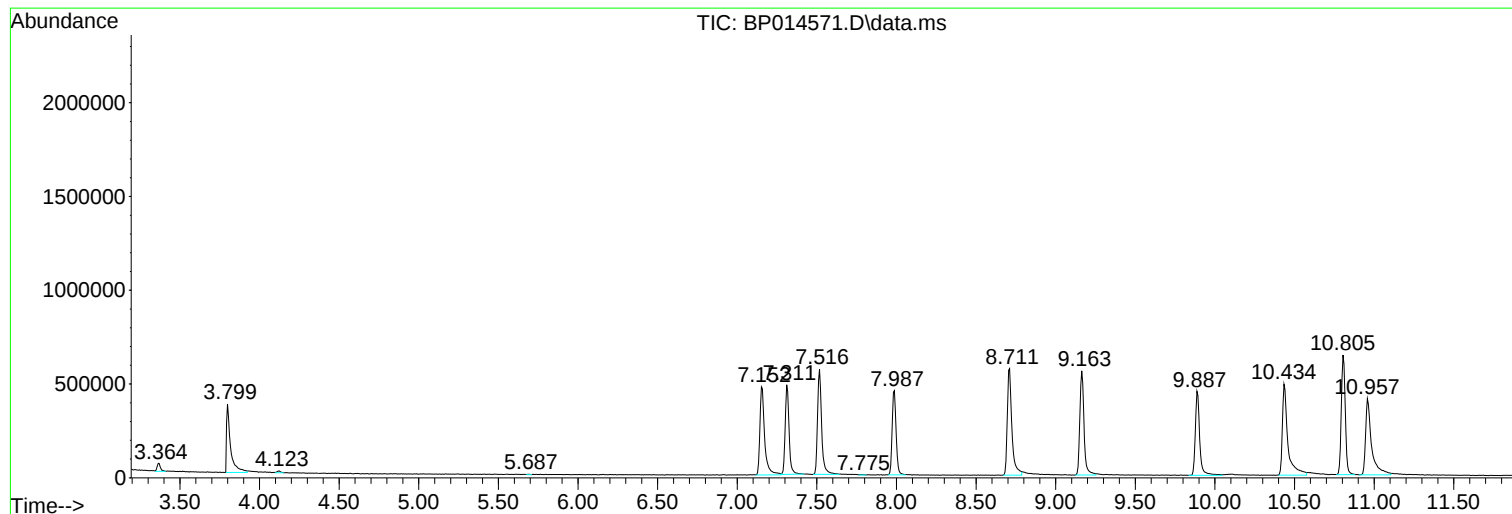

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014571.D
Acq On : 05 Apr 2023 23:21
Operator : CG/JU
Sample : PB151872BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK872

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014571.D
Acq On : 05 Apr 2023 23:21
Operator : CG/JU
Sample : PB151872BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK872

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc