

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014573.D
 Acq On : 06 Apr 2023 00:28
 Operator : CG/JU
 Sample : PB151910BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK910

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014573.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	35	rBV	42976	56788	1.23%	0.123%
2	3.799	101	104	121	rBV	399913	696016	15.08%	1.505%
3	4.122	156	159	165	rVB	10864	15060	0.33%	0.033%
4	7.152	668	674	695	rBV	568158	1122951	24.33%	2.428%
5	7.310	695	701	721	rVB	563409	947358	20.52%	2.048%
6	7.516	729	736	751	rBV	673392	1168153	25.31%	2.526%
7	7.987	809	816	828	rBV	551551	924110	20.02%	1.998%
8	8.704	932	938	961	rBV	719909	1424954	30.87%	3.081%
9	9.163	1009	1016	1039	rBV	692989	1244164	26.95%	2.690%
10	9.887	1131	1139	1161	rBV	566575	1047396	22.69%	2.265%
11	10.434	1225	1232	1259	rBV	654907	1449658	31.40%	3.134%
12	10.804	1287	1295	1307	rBV	816273	1416045	30.68%	3.062%
13	10.957	1313	1321	1350	rBV	799609	1860394	40.30%	4.022%
14	12.422	1561	1570	1579	rBV6	9216	24808	0.54%	0.054%
15	13.528	1752	1758	1762	rVB8	4815	9583	0.21%	0.021%
16	13.622	1767	1774	1778	rBV10	2725	6809	0.15%	0.015%
17	14.045	1839	1846	1864	rBV	1666170	2577827	55.84%	5.574%
18	14.334	1888	1895	1915	rBV	1852602	2828587	61.28%	6.116%
19	14.639	1940	1947	1959	rBV	1384283	1995734	43.23%	4.315%
20	14.875	1980	1987	2022	rBV	249541	974313	21.11%	2.107%
21	15.633	2109	2116	2131	rBV	2396796	3552828	76.96%	7.682%
22	15.763	2132	2138	2154	rVV	734049	1208536	26.18%	2.613%
23	15.881	2154	2158	2166	rVB3	15501	32901	0.71%	0.071%
24	16.210	2211	2214	2218	rBV6	3237	5363	0.12%	0.012%
25	16.422	2247	2250	2253	rBV5	4572	5710	0.12%	0.012%
26	17.069	2358	2360	2365	rBV6	3712	6299	0.14%	0.014%
27	17.186	2378	2380	2383	rBV4	5009	4913	0.11%	0.011%
28	17.398	2409	2416	2426	rBV	1777239	2493032	54.01%	5.390%
29	17.498	2427	2433	2451	rVB	2576171	3884616	84.15%	8.399%
30	18.339	2572	2576	2583	rBV5	8731	22272	0.48%	0.048%
31	19.310	2737	2741	2745	rBV2	36485	44795	0.97%	0.097%
32	19.380	2749	2753	2757	rBV	27644	40153	0.87%	0.087%
33	19.727	2806	2812	2828	rBV	3206670	4616217	100.00%	9.981%
34	21.486	3106	3111	3121	rBV	1607572	2591185	56.13%	5.603%
35	23.827	3502	3509	3521	rVB2	1856047	3754700	81.34%	8.118%
36	23.986	3530	3536	3552	rVB3	961203	2196179	47.58%	4.748%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014573.D
Acq On : 06 Apr 2023 00:28
Operator : CG/JU
Sample : PB151910BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK910

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Title : SVOA CALIBRATION




Sum of corrected areas: 46250407

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014573.D
Acq On : 06 Apr 2023 00:28
Operator : CG/JU
Sample : PB151910BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK910

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

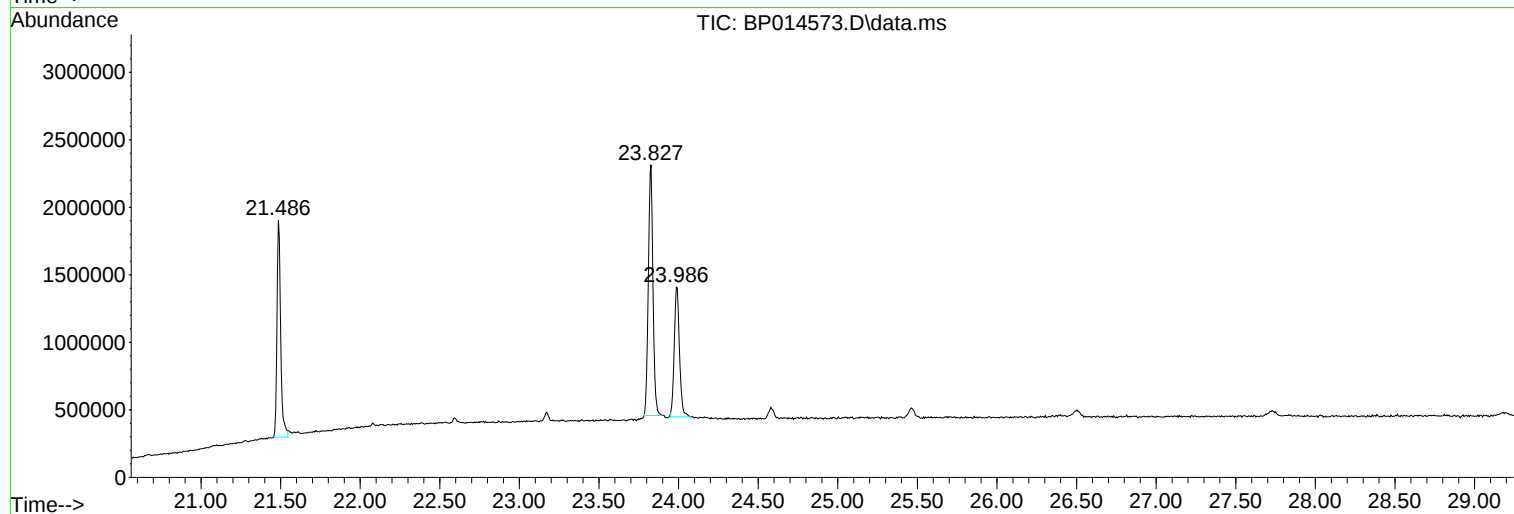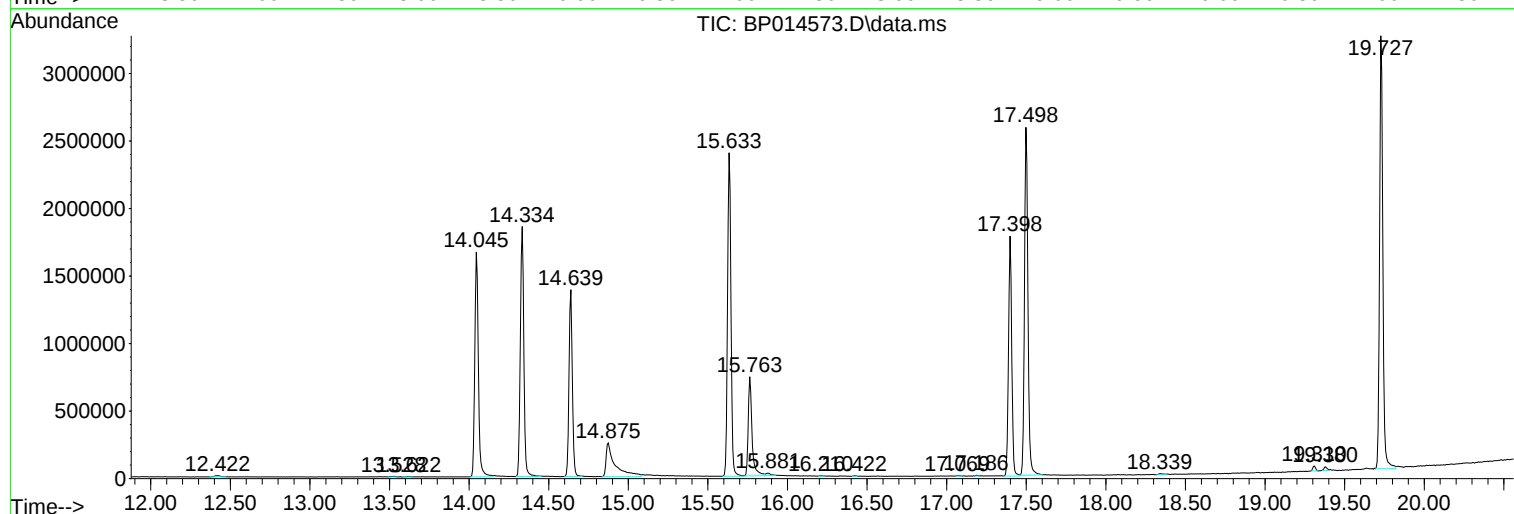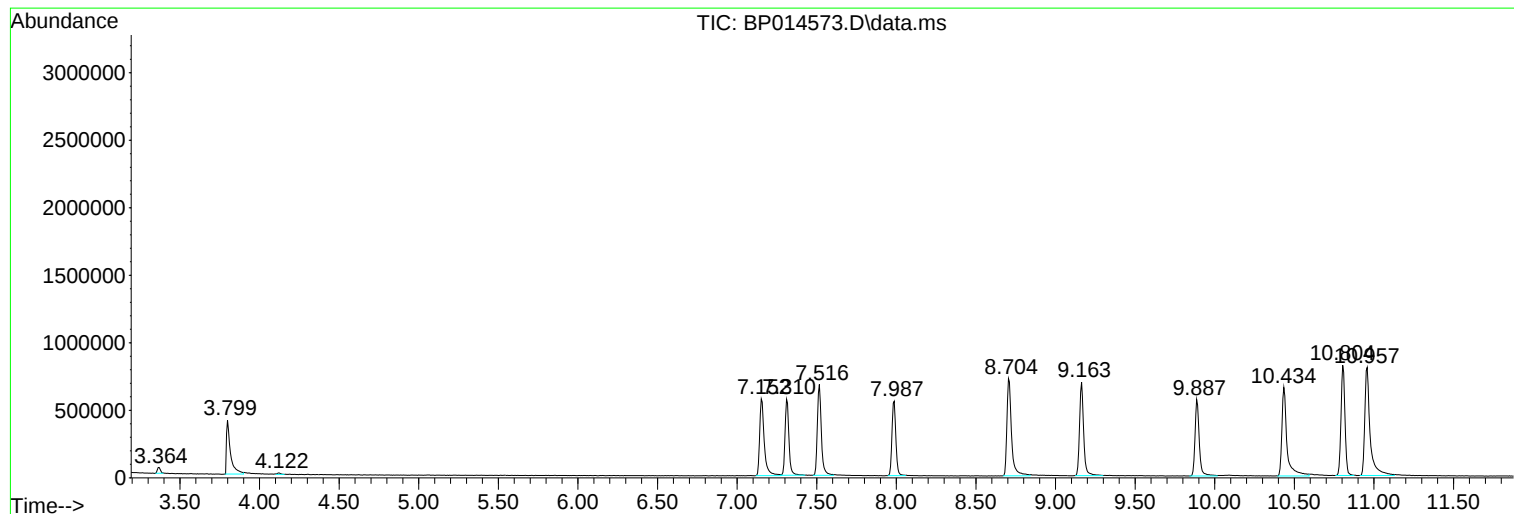

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014573.D
Acq On : 06 Apr 2023 00:28
Operator : CG/JU
Sample : PB151910BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK910

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014573.D
Acq On : 06 Apr 2023 00:28
Operator : CG/JU
Sample : PB151910BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK910

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc