

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014579.D
 Acq On : 06 Apr 2023 04:23
 Operator : CG/JU
 Sample : 02194-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	8	10	13	rBV3	4137	4469	0.13%	0.014%
2	3.364	27	30	35	rBV	27409	31735	0.94%	0.097%
3	3.834	107	110	117	rBV	23645	46806	1.38%	0.143%
4	4.016	137	141	147	rVB2	14445	22918	0.68%	0.070%
5	4.122	155	159	164	rVB3	9275	12993	0.38%	0.040%
6	4.228	174	177	183	rVB4	7187	10029	0.30%	0.031%
7	4.652	243	249	258	rVB	29656	47977	1.42%	0.146%
8	5.052	313	317	324	rVB2	12670	19625	0.58%	0.060%
9	5.240	344	349	355	rBV8	5877	11585	0.34%	0.035%
10	6.363	535	540	545	rBV8	6322	11147	0.33%	0.034%
11	7.163	670	676	693	rBV2	62468	168763	4.99%	0.515%
12	7.310	695	701	716	rVV	387522	652624	19.30%	1.991%
13	7.516	728	736	757	rBV	340592	652286	19.29%	1.990%
14	7.981	809	815	828	rBV	461599	792276	23.43%	2.417%
15	8.710	930	939	951	rBV	233350	482218	14.26%	1.471%
16	9.163	1008	1016	1030	rBV	456984	840751	24.86%	2.565%
17	9.534	1075	1079	1083	rVB4	6393	9550	0.28%	0.029%
18	9.887	1132	1139	1154	rBV	364030	680263	20.11%	2.075%
19	10.081	1169	1172	1176	rVB6	2629	3830	0.11%	0.012%
20	10.434	1226	1232	1258	rBV	381420	951951	28.15%	2.904%
21	10.804	1287	1295	1309	rBV	668300	1163049	34.39%	3.548%
22	10.963	1315	1322	1347	rBV	195913	541240	16.00%	1.651%
23	11.363	1387	1390	1397	rVB9	3196	4411	0.13%	0.013%
24	11.675	1440	1443	1444	rBV3	3672	3926	0.12%	0.012%
25	12.416	1562	1569	1573	rBV5	7423	13949	0.41%	0.043%
26	12.587	1596	1598	1601	rBV3	2814	3513	0.10%	0.011%
27	12.981	1663	1665	1670	rBV6	2509	4254	0.13%	0.013%
28	13.151	1690	1694	1698	rVB7	3200	4352	0.13%	0.013%
29	13.234	1704	1708	1713	rVB8	4128	6978	0.21%	0.021%
30	13.439	1739	1743	1751	rVB8	3421	7711	0.23%	0.024%
31	13.516	1751	1756	1764	rVB9	7523	15794	0.47%	0.048%
32	13.610	1768	1772	1775	rBV5	3227	4953	0.15%	0.015%
33	14.045	1837	1846	1859	rBV	1244984	1904251	56.31%	5.809%
34	14.151	1861	1864	1869	rVV7	9401	15992	0.47%	0.049%
35	14.228	1873	1877	1881	rVB	10445	14817	0.44%	0.045%
36	14.334	1888	1895	1912	rBV	1274458	1985900	58.72%	6.058%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014579.D
 Acq On : 06 Apr 2023 04:23
 Operator : CG/JU
 Sample : 02194-05
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDW3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	14.510	1920	1925	1930	rVB8	6490	11020	0.33%	0.034%
38	14.634	1940	1946	1962	rVB	1009803	1543099	45.63%	4.708%
39	14.875	1981	1987	1990	rBV6	4910	9466	0.28%	0.029%
40	14.928	1990	1996	2006	rBV8	15262	54526	1.61%	0.166%
41	15.416	2076	2079	2083	rVB2	4591	4843	0.14%	0.015%
42	15.463	2083	2087	2096	rVB3	18945	27241	0.81%	0.083%
43	15.633	2109	2116	2133	rBV	1688332	2590192	76.59%	7.902%
44	15.763	2133	2138	2150	rBV	496241	834254	24.67%	2.545%
45	15.998	2172	2178	2190	rBV	440928	679591	20.09%	2.073%
46	16.328	2230	2234	2245	rVB	44624	76080	2.25%	0.232%
47	16.569	2269	2275	2279	rBV	68983	102948	3.04%	0.314%
48	16.680	2290	2294	2296	rVV5	4089	5517	0.16%	0.017%
49	17.128	2366	2370	2375	rBV	41089	52818	1.56%	0.161%
50	17.180	2375	2379	2382	rVB3	11908	17601	0.52%	0.054%
51	17.286	2395	2397	2400	rVB4	5348	4662	0.14%	0.014%
52	17.398	2409	2416	2426	rBV	1277427	1831331	54.15%	5.587%
53	17.498	2426	2433	2449	rVV2	1950911	2962784	87.61%	9.039%
54	17.675	2459	2463	2469	rVB9	10688	20375	0.60%	0.062%
55	17.863	2492	2495	2499	rVB2	26020	32719	0.97%	0.100%
56	18.045	2522	2526	2530	rBV5	24438	32641	0.97%	0.100%
57	18.263	2559	2563	2572	rBV	63720	125058	3.70%	0.382%
58	18.533	2606	2609	2613	rBV3	20257	22607	0.67%	0.069%
59	19.304	2736	2740	2745	rBV2	31719	50612	1.50%	0.154%
60	19.374	2749	2752	2759	rVV3	27574	50130	1.48%	0.153%
61	19.498	2769	2773	2779	rBV5	39298	70381	2.08%	0.215%
62	19.727	2806	2812	2825	rBV	2414458	3381969	100.00%	10.317%
63	21.163	3053	3056	3064	rBV4	89668	154803	4.58%	0.472%
64	21.486	3106	3111	3124	rBV	1168923	1890975	55.91%	5.769%
65	23.821	3501	3508	3522	rBV2	1533807	3219709	95.20%	9.822%
66	23.986	3530	3536	3549	rVB2	804029	1770585	52.35%	5.402%




Sum of corrected areas: 32779423

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014579.D
Acq On : 06 Apr 2023 04:23
Operator : CG/JU
Sample : 02194-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDW3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

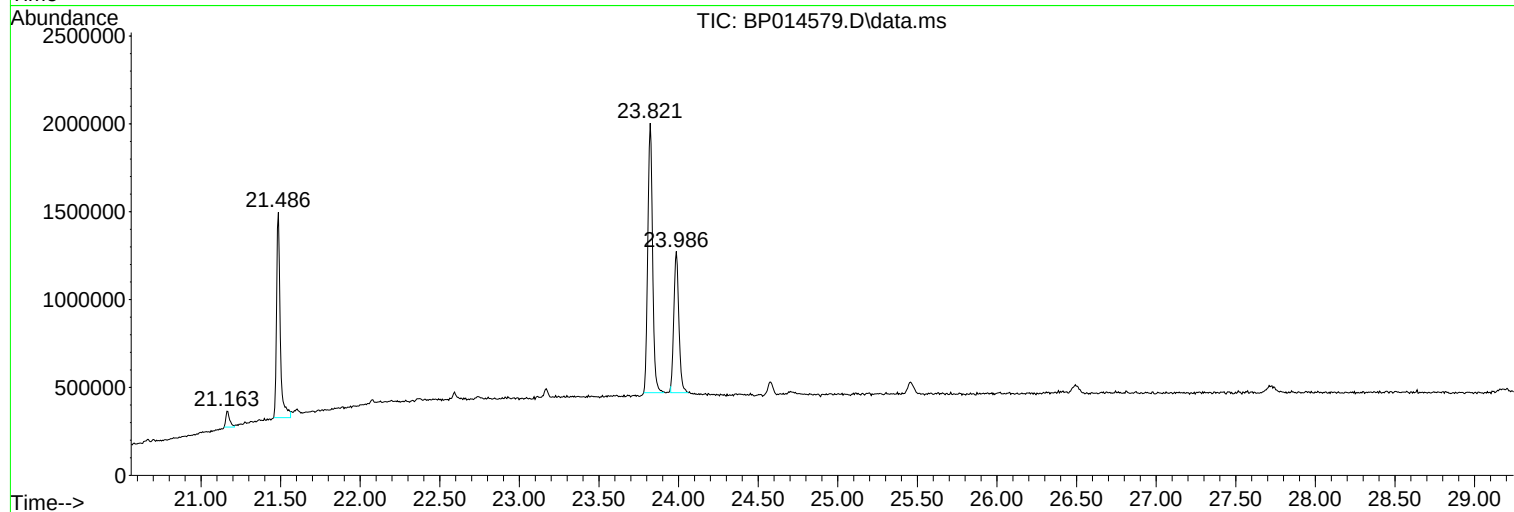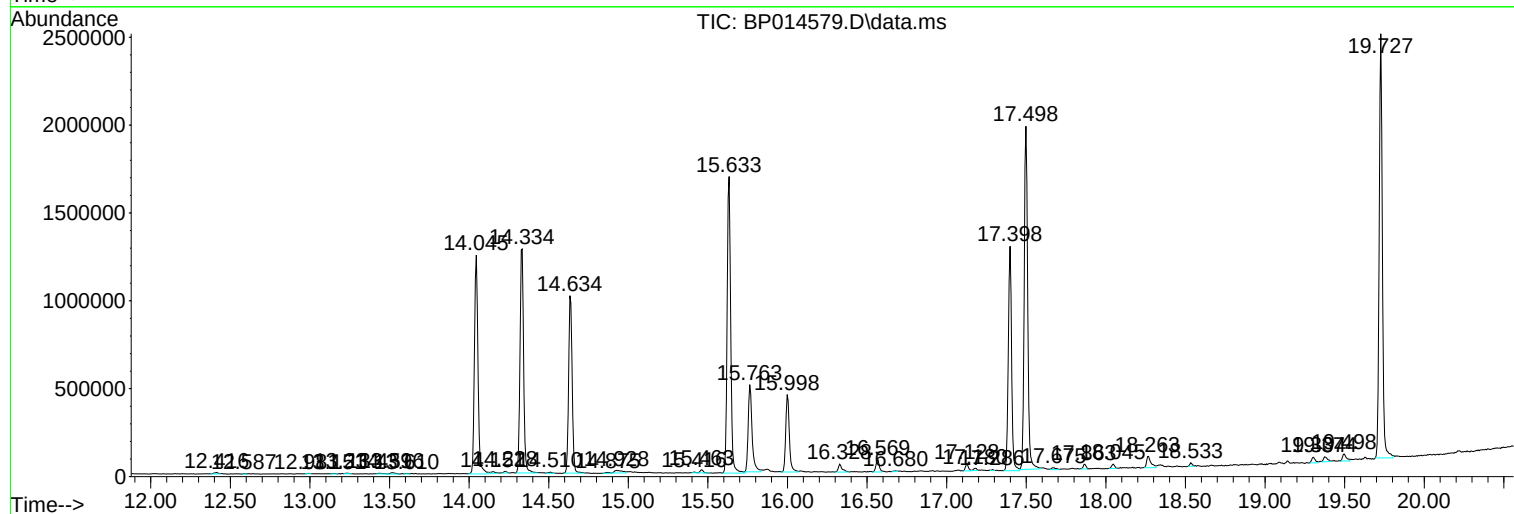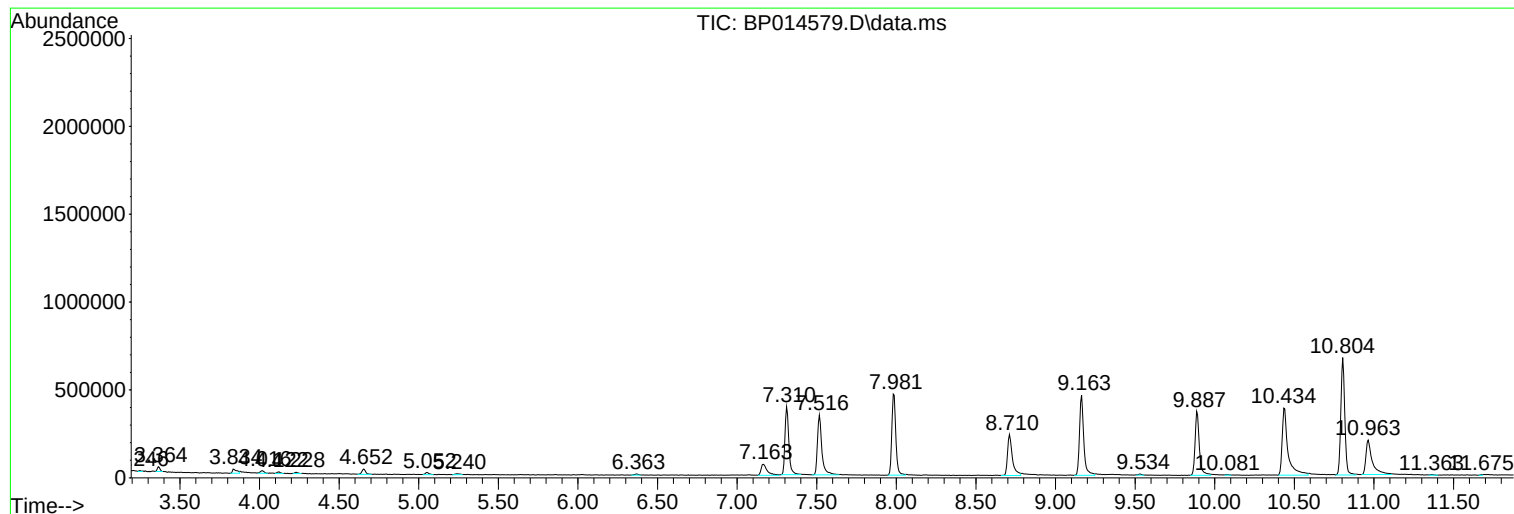

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014579.D
Acq On : 06 Apr 2023 04:23
Operator : CG/JU
Sample : 02194-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDW3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.998	8.81 ng/ul	679591	Acenaphthene-d10	14.634

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	95
4			Benzophenone	182	C13H10O	000119-61-9	91
5			Benzophenone	182	C13H10O	000119-61-9	78

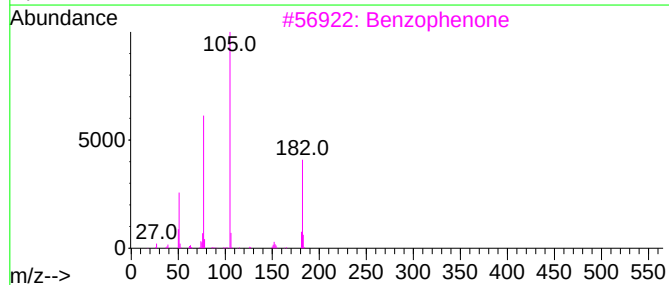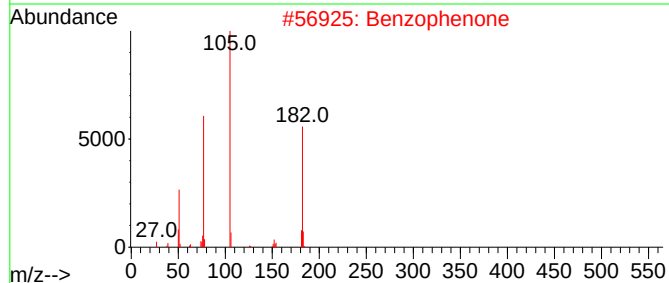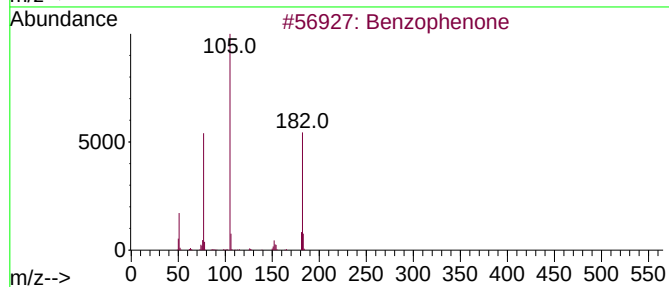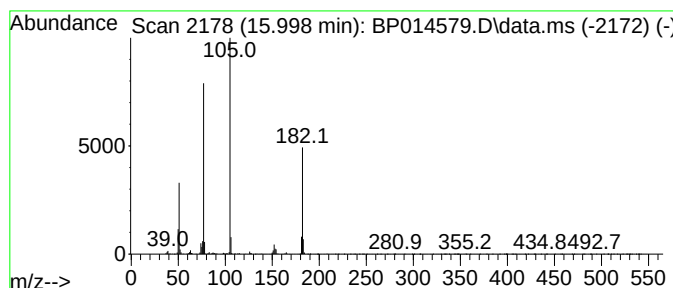

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014579.D
Acq On : 06 Apr 2023 04:23
Operator : CG/JU
Sample : 02194-05
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDW3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.998	8.8	ng/u1	679591	3	14.634	1543100	20.0