

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014590.D
 Acq On : 06 Apr 2023 11:10
 Operator : CG/JU
 Sample : 02192-01DL2 25X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG2DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014590.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.117	154	158	164	rBV	11753	17298	0.55%	0.116%
2	4.322	191	193	196	rVB4	4359	3935	0.13%	0.026%
3	5.458	382	386	391	rBV7	2863	3757	0.12%	0.025%
4	5.599	403	410	413	rBV8	6198	12141	0.39%	0.081%
5	5.969	466	473	478	rVB5	7143	13773	0.44%	0.092%
6	6.852	620	623	629	rBV8	2343	3825	0.12%	0.026%
7	7.063	652	659	663	rBV2	6789	11979	0.38%	0.080%
8	7.122	665	669	673	rVB6	3010	4583	0.15%	0.031%
9	7.193	676	681	685	rBV3	7814	12859	0.41%	0.086%
10	7.322	698	703	707	rBV2	10309	19210	0.61%	0.129%
11	7.540	734	740	743	rBV7	7154	14949	0.48%	0.100%
12	7.569	743	745	749	rVV5	5754	9562	0.31%	0.064%
13	7.622	749	754	763	rVB2	32040	55997	1.79%	0.375%
14	7.705	765	768	771	rBV5	2922	4244	0.14%	0.028%
15	7.981	806	815	828	rBV	491498	876972	28.07%	5.872%
16	8.093	830	834	840	rVB	21823	39267	1.26%	0.263%
17	8.357	872	879	887	rBV5	13087	27562	0.88%	0.185%
18	8.528	903	908	916	rBV3	23973	44602	1.43%	0.299%
19	8.622	918	924	928	rVB6	8291	13415	0.43%	0.090%
20	8.799	949	954	958	rVB8	3434	6405	0.21%	0.043%
21	8.934	974	977	978	rBV3	3372	3882	0.12%	0.026%
22	8.987	982	986	991	rVB6	5705	10009	0.32%	0.067%
23	9.093	1000	1004	1012	rBV2	9355	17730	0.57%	0.119%
24	9.181	1012	1019	1029	rBV6	11641	31607	1.01%	0.212%
25	9.422	1057	1060	1066	rBV7	5026	11374	0.36%	0.076%
26	9.622	1088	1094	1097	rBV3	7267	11446	0.37%	0.077%
27	9.681	1097	1104	1114	rVB3	11223	21026	0.67%	0.141%
28	9.851	1128	1133	1135	rBV5	2207	3622	0.12%	0.024%
29	9.916	1139	1144	1146	rBV6	4317	7265	0.23%	0.049%
30	10.046	1159	1166	1172	rBV3	6635	10266	0.33%	0.069%
31	10.199	1185	1192	1200	rBV6	14838	27198	0.87%	0.182%
32	10.428	1225	1231	1238	rBV7	6773	12608	0.40%	0.084%
33	10.504	1238	1244	1254	rBV7	9106	25945	0.83%	0.174%
34	10.804	1286	1295	1299	rBV	716771	1230413	39.38%	8.238%
35	10.851	1299	1303	1318	rVV	367736	719800	23.04%	4.820%
36	10.981	1321	1325	1328	rVB3	5418	9177	0.29%	0.061%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014590.D
 Acq On : 06 Apr 2023 11:10
 Operator : CG/JU
 Sample : 02192-01DL2 25X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG2DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	11.193	1357	1361	1366	rVB8	2646	5115	0.16%	0.034%
38	12.375	1559	1562	1569	rBV8	2253	4130	0.13%	0.028%
39	12.475	1572	1579	1588	rBV	31930	76429	2.45%	0.512%
40	12.687	1606	1615	1626	rBV	41934	91103	2.92%	0.610%
41	13.481	1745	1750	1756	rBV7	8042	18327	0.59%	0.123%
42	13.522	1756	1757	1762	rVB5	4279	3910	0.13%	0.026%
43	13.681	1779	1784	1785	rVV5	4679	6695	0.21%	0.045%
44	13.692	1785	1786	1791	rVB4	5296	5883	0.19%	0.039%
45	13.822	1801	1808	1811	rBV6	7670	17088	0.55%	0.114%
46	13.957	1825	1831	1836	rBV3	15825	30143	0.96%	0.202%
47	14.010	1836	1840	1843	rVV5	10702	18259	0.58%	0.122%
48	14.057	1843	1848	1862	rVV	42260	88416	2.83%	0.592%
49	14.192	1866	1871	1875	rVV8	8377	17785	0.57%	0.119%
50	14.222	1875	1876	1884	rVB7	5733	6177	0.20%	0.041%
51	14.334	1888	1895	1905	rBV	52652	103120	3.30%	0.690%
52	14.634	1939	1946	1955	rBV	1090416	1713302	54.84%	11.472%
53	14.863	1983	1985	1991	rVB7	3042	4184	0.13%	0.028%
54	15.045	2012	2016	2023	rVB10	5132	11715	0.37%	0.078%
55	15.110	2023	2027	2036	rVB10	3494	8552	0.27%	0.057%
56	15.222	2040	2046	2047	rBV6	6176	9364	0.30%	0.063%
57	15.287	2051	2057	2072	rVB2	63417	153466	4.91%	1.028%
58	15.469	2086	2088	2092	rVB5	3954	4219	0.14%	0.028%
59	15.634	2110	2116	2123	rBV2	58061	113665	3.64%	0.761%
60	15.798	2139	2144	2147	rBV7	7398	16657	0.53%	0.112%
61	16.686	2290	2295	2296	rBV4	3726	5438	0.17%	0.036%
62	16.751	2304	2306	2309	rVB4	3356	3646	0.12%	0.024%
63	17.045	2349	2356	2377	rBV	1879983	3124134	100.00%	20.918%
64	17.398	2409	2416	2428	rBV	1250119	1930817	61.80%	12.928%
65	17.498	2428	2433	2442	rVB2	69556	128302	4.11%	0.859%
66	18.004	2515	2519	2523	rBV7	4729	7337	0.23%	0.049%
67	19.733	2808	2813	2819	rBV	77495	131492	4.21%	0.880%
68	21.486	3106	3111	3124	rBV	1140209	1864005	59.66%	12.481%
69	23.986	3529	3536	3547	rVB2	852703	1862564	59.62%	12.471%




Sum of corrected areas: 14935142

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014590.D
Acq On : 06 Apr 2023 11:10
Operator : CG/JU
Sample : 02192-01DL2 25X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG2DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

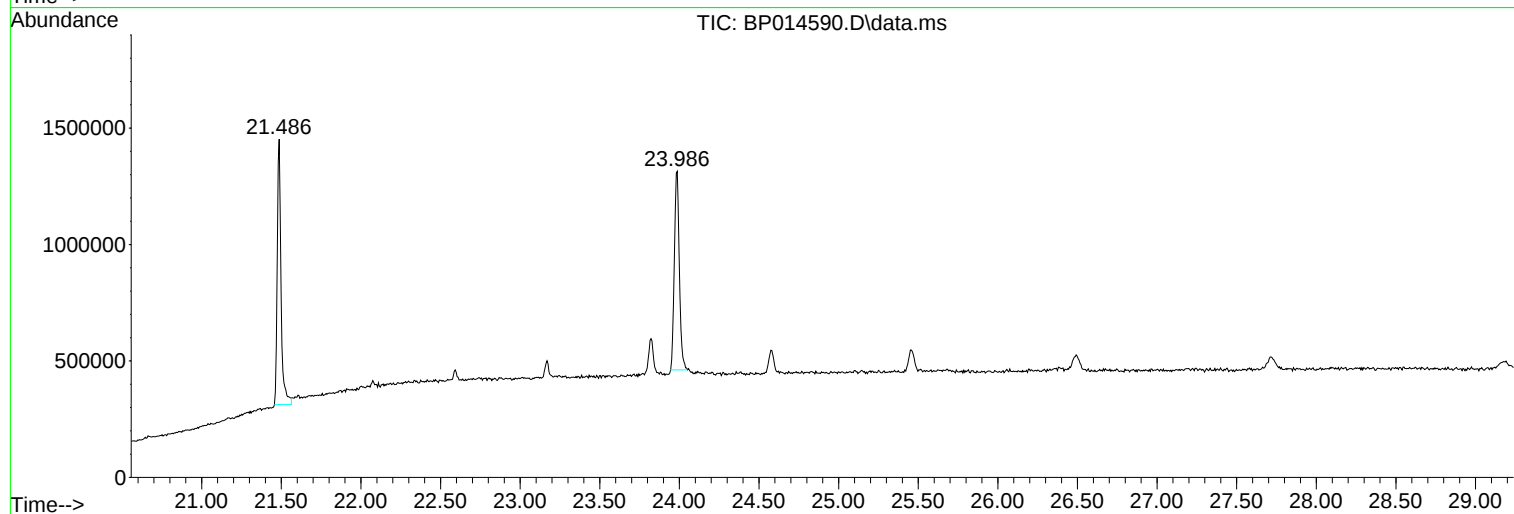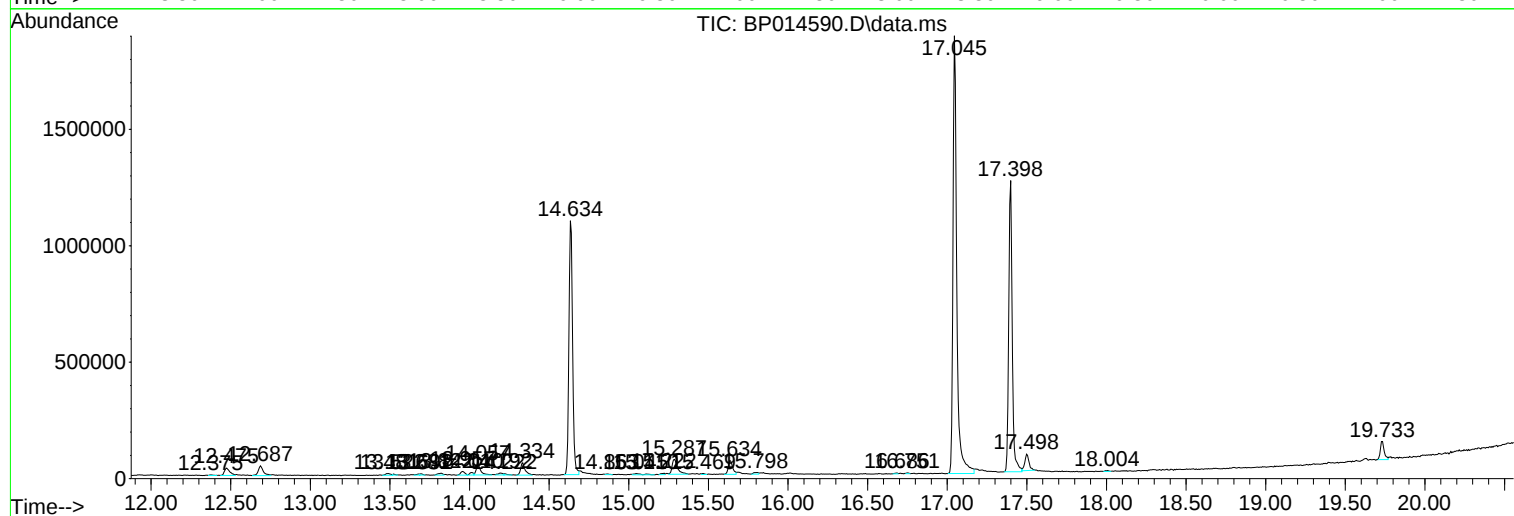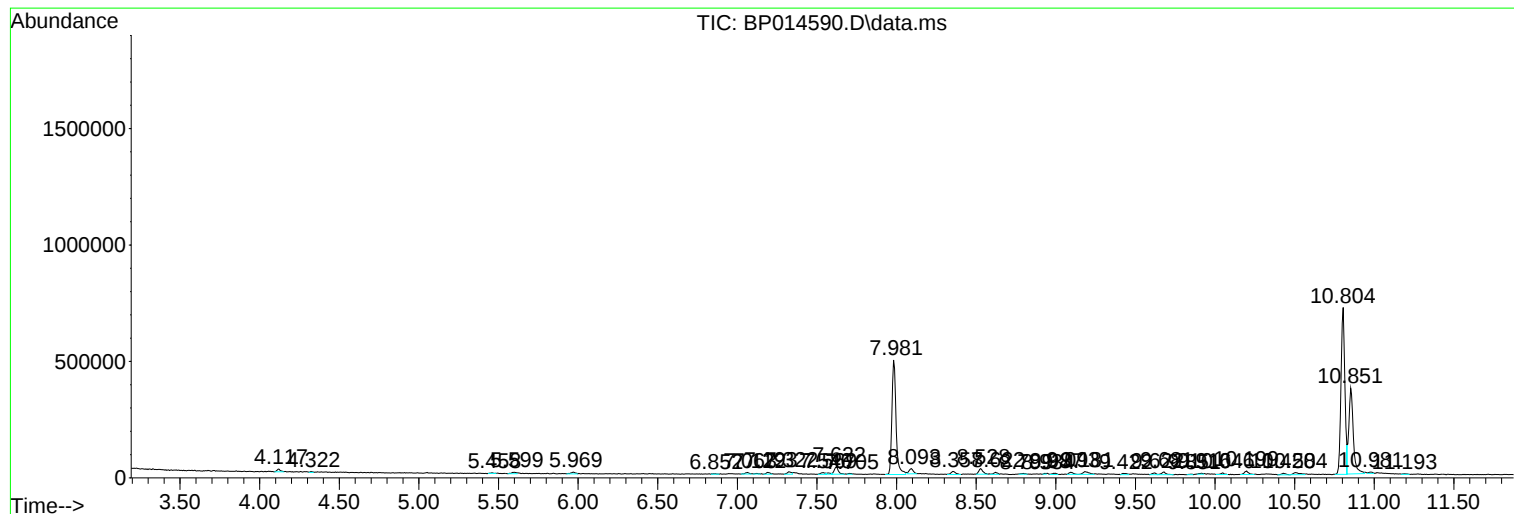

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014590.D
Acq On : 06 Apr 2023 11:10
Operator : CG/JU
Sample : 02192-01DL2 25X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG2DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014590.D
Acq On : 06 Apr 2023 11:10
Operator : CG/JU
Sample : 02192-01DL2 25X
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG2DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc