

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014593.D
 Acq On : 06 Apr 2023 18:22
 Operator : CG/JU
 Sample : PB151949BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK949

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014593.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	38	rBV	44920	60966	1.50%	0.146%
2	3.799	101	104	129	rBV	348021	630268	15.47%	1.510%
3	4.123	155	159	165	rVB2	11974	18769	0.46%	0.045%
4	7.152	668	674	692	rBV	543155	1033879	25.38%	2.477%
5	7.311	695	701	714	rVV	495593	819287	20.11%	1.963%
6	7.516	729	736	754	rBV	615579	1053424	25.86%	2.524%
7	7.981	809	815	826	rBV	581185	964481	23.68%	2.311%
8	8.705	931	938	958	rBV	694887	1309371	32.14%	3.137%
9	9.163	1009	1016	1029	rBV	633924	1108741	27.22%	2.656%
10	9.887	1127	1139	1156	rBV	527997	987274	24.23%	2.365%
11	10.434	1224	1232	1261	rBV	623220	1374291	33.73%	3.292%
12	10.805	1287	1295	1305	rBV	870722	1476802	36.25%	3.538%
13	10.957	1313	1321	1350	rBV	467371	1113065	27.32%	2.667%
14	12.410	1562	1568	1579	rBV5	8813	25856	0.63%	0.062%
15	14.046	1837	1846	1861	rBV	1551787	2279144	55.95%	5.460%
16	14.328	1886	1894	1907	rBV	1673516	2547922	62.54%	6.104%
17	14.634	1938	1946	1962	rBV	1391813	2105896	51.69%	5.045%
18	14.869	1980	1986	2013	rBV2	213173	792410	19.45%	1.898%
19	15.634	2109	2116	2131	rBV	2101994	3219721	79.03%	7.714%
20	15.763	2132	2138	2154	rVV	702331	1160281	28.48%	2.780%
21	15.875	2154	2157	2164	rVB6	13697	23825	0.58%	0.057%
22	17.398	2409	2416	2426	rBV	1874925	2623854	64.41%	6.286%
23	17.498	2426	2433	2452	rVV	2404586	3580169	87.88%	8.577%
24	19.304	2736	2740	2747	rBV4	34725	56275	1.38%	0.135%
25	19.375	2749	2752	2759	rVB2	24777	41826	1.03%	0.100%
26	19.728	2806	2812	2827	rBV	2998798	4073795	100.00%	9.760%
27	21.486	3106	3111	3122	rBV	1524661	2383388	58.51%	5.710%
28	23.821	3501	3508	3522	rBV2	1405473	2959122	72.64%	7.089%
29	23.986	3529	3536	3548	rVB2	858826	1916821	47.05%	4.592%




Sum of corrected areas: 41740923

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014593.D
Acq On : 06 Apr 2023 18:22
Operator : CG/JU
Sample : PB151949BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK949

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

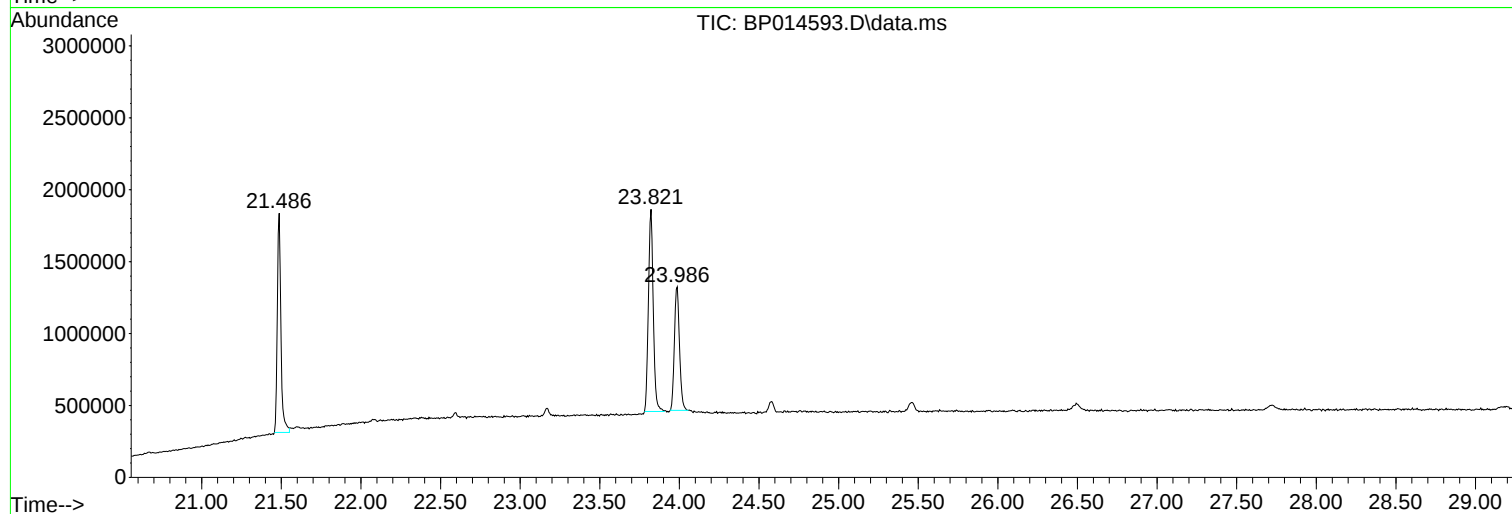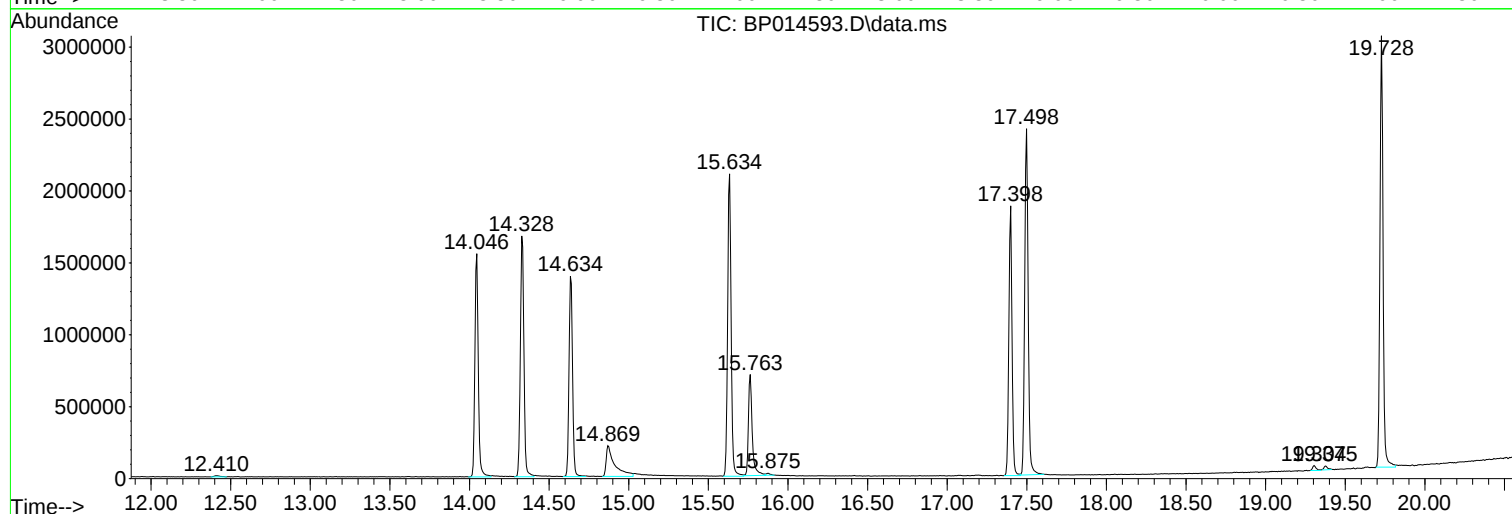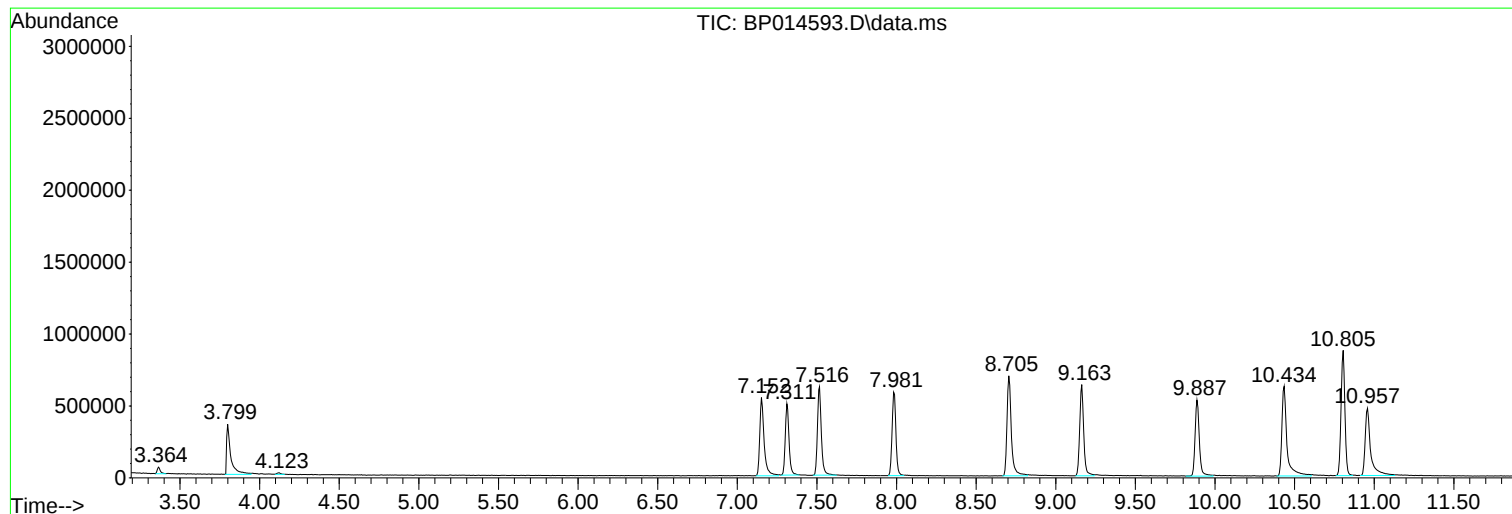

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014593.D
Acq On : 06 Apr 2023 18:22
Operator : CG/JU
Sample : PB151949BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK949

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014593.D
Acq On : 06 Apr 2023 18:22
Operator : CG/JU
Sample : PB151949BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK949

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------