

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014594.D
 Acq On : 06 Apr 2023 18:57
 Operator : CG/JU
 Sample : 02194-06
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	35	rVB	33015	39769	0.80%	0.093%
2	3.834	107	110	120	rBV	25702	59960	1.21%	0.140%
3	4.016	136	141	148	rBV	15965	26501	0.54%	0.062%
4	4.116	155	158	164	rVB2	10513	17111	0.35%	0.040%
5	4.234	174	178	181	rVB4	7429	9394	0.19%	0.022%
6	4.652	244	249	261	rVB	34259	60111	1.22%	0.140%
7	5.052	312	317	323	rBV	12305	21078	0.43%	0.049%
8	5.246	346	350	353	rBV4	4935	7735	0.16%	0.018%
9	6.369	536	541	546	rVB4	7583	13264	0.27%	0.031%
10	7.069	656	660	665	rBV7	3156	5356	0.11%	0.013%
11	7.157	668	675	694	rVV	84175	205033	4.15%	0.479%
12	7.310	695	701	720	rVV	480390	795961	16.10%	1.859%
13	7.516	729	736	756	rBV	427834	773015	15.64%	1.806%
14	7.981	808	815	829	rBV	525118	882100	17.85%	2.061%
15	8.704	931	938	957	rBV	321229	651000	13.17%	1.521%
16	9.163	1008	1016	1031	rBV	611307	1095802	22.17%	2.560%
17	9.528	1073	1078	1085	rBV9	5755	9943	0.20%	0.023%
18	9.887	1132	1139	1154	rBV	493769	895634	18.12%	2.092%
19	10.434	1223	1232	1255	rBV	567010	1241006	25.11%	2.899%
20	10.804	1288	1295	1311	rBV	783002	1360162	27.52%	3.177%
21	10.957	1315	1321	1342	rBV	235486	589829	11.93%	1.378%
22	11.675	1437	1443	1444	rBV6	5292	7966	0.16%	0.019%
23	12.034	1501	1504	1509	rVB6	3612	5906	0.12%	0.014%
24	12.404	1562	1567	1575	rBV5	10396	27454	0.56%	0.064%
25	12.981	1658	1665	1667	rBV7	5212	8652	0.18%	0.020%
26	13.234	1706	1708	1714	rVB4	7040	8499	0.17%	0.020%
27	13.434	1738	1742	1747	rBV7	4805	7633	0.15%	0.018%
28	13.516	1753	1756	1762	rVB8	5022	9780	0.20%	0.023%
29	13.869	1808	1816	1818	rBV9	4756	11088	0.22%	0.026%
30	14.039	1836	1845	1860	rBV	1758952	2543463	51.46%	5.942%
31	14.151	1860	1864	1871	rVV8	11302	21105	0.43%	0.049%
32	14.222	1871	1876	1881	rVV	13512	19869	0.40%	0.046%
33	14.328	1888	1894	1907	rBV	1789318	2670004	54.02%	6.237%
34	14.510	1920	1925	1928	rVB6	8072	10758	0.22%	0.025%
35	14.634	1940	1946	1955	rBV	1352884	1947338	39.40%	4.549%
36	14.904	1986	1992	2005	rVV3	26736	98056	1.98%	0.229%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014594.D
 Acq On : 06 Apr 2023 18:57
 Operator : CG/JU
 Sample : 02194-06
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BHDW4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	15.457	2082	2086	2091	rVB2	29894	42968	0.87%	0.100%
38	15.633	2109	2116	2132	rBV	2367844	3576192	72.35%	8.354%
39	15.763	2132	2138	2150	rVV	845079	1343965	27.19%	3.140%
40	15.875	2153	2157	2160	rVB4	18118	29006	0.59%	0.068%
41	15.998	2172	2178	2190	rBV	441314	654271	13.24%	1.528%
42	16.328	2230	2234	2244	rVB	50183	85671	1.73%	0.200%
43	16.563	2269	2274	2280	rBV	80790	117057	2.37%	0.273%
44	17.128	2366	2370	2374	rBV	60526	75552	1.53%	0.176%
45	17.175	2375	2378	2382	rVV5	17442	25059	0.51%	0.059%
46	17.398	2409	2416	2425	rBV	1676557	2452447	49.62%	5.729%
47	17.498	2427	2433	2446	rVV	2924432	4179507	84.56%	9.764%
48	17.663	2459	2461	2467	rBV7	12056	19434	0.39%	0.045%
49	17.863	2492	2495	2501	rVB2	56610	70786	1.43%	0.165%
50	18.039	2522	2525	2530	rVB	49606	65197	1.32%	0.152%
51	18.263	2559	2563	2572	rBV2	89761	154774	3.13%	0.362%
52	18.533	2606	2609	2614	rBV	48147	53745	1.09%	0.126%
53	19.139	2709	2712	2716	rBV	34215	46627	0.94%	0.109%
54	19.304	2736	2740	2746	rBV4	49564	73106	1.48%	0.171%
55	19.374	2749	2752	2759	rVB	41601	71488	1.45%	0.167%
56	19.492	2768	2772	2781	rBV4	70081	115222	2.33%	0.269%
57	19.727	2806	2812	2822	rBV	3662262	4942907	100.00%	11.547%
58	21.163	3053	3056	3062	rBV5	85518	142831	2.89%	0.334%
59	21.480	3105	3110	3124	rBV	1637549	2523223	51.05%	5.894%
60	23.821	3501	3508	3520	rVB2	1854170	3824256	77.37%	8.934%
61	23.980	3529	3535	3548	rVB2	903614	1964673	39.75%	4.590%




Sum of corrected areas: 42807299

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014594.D
Acq On : 06 Apr 2023 18:57
Operator : CG/JU
Sample : 02194-06
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

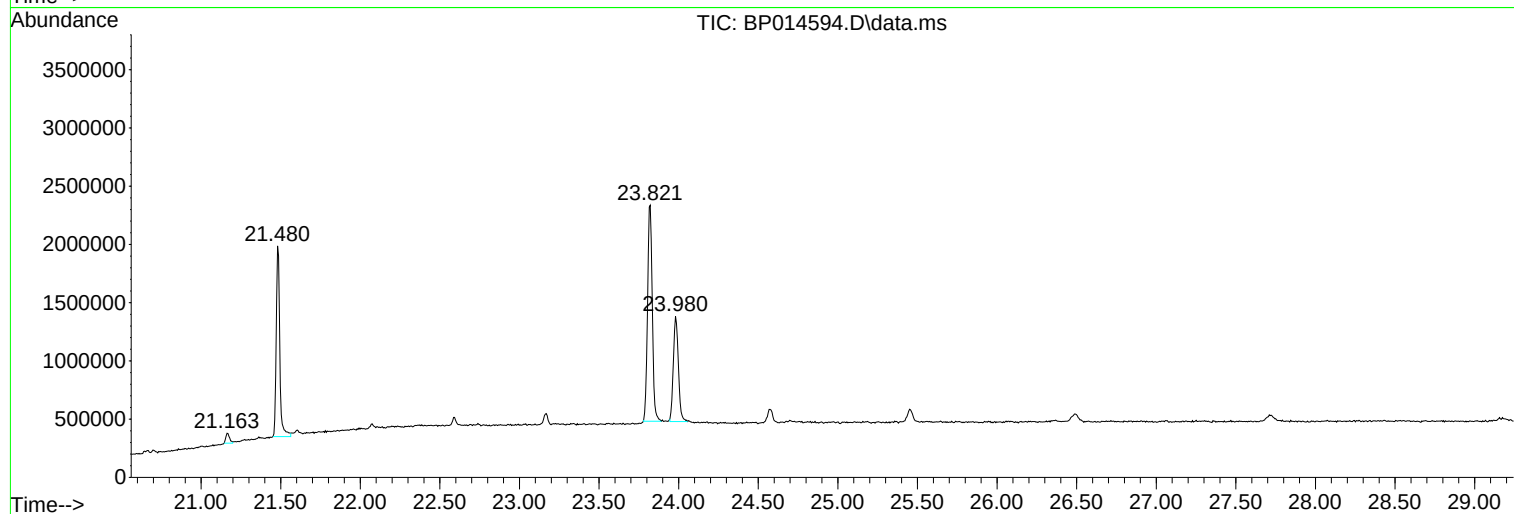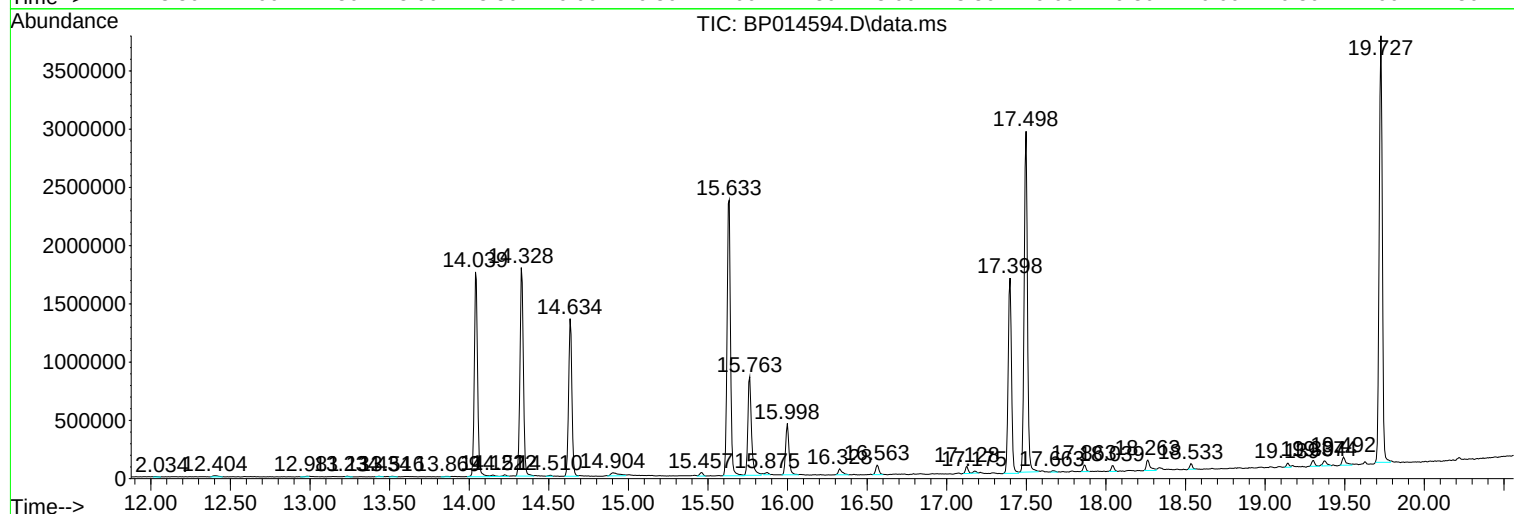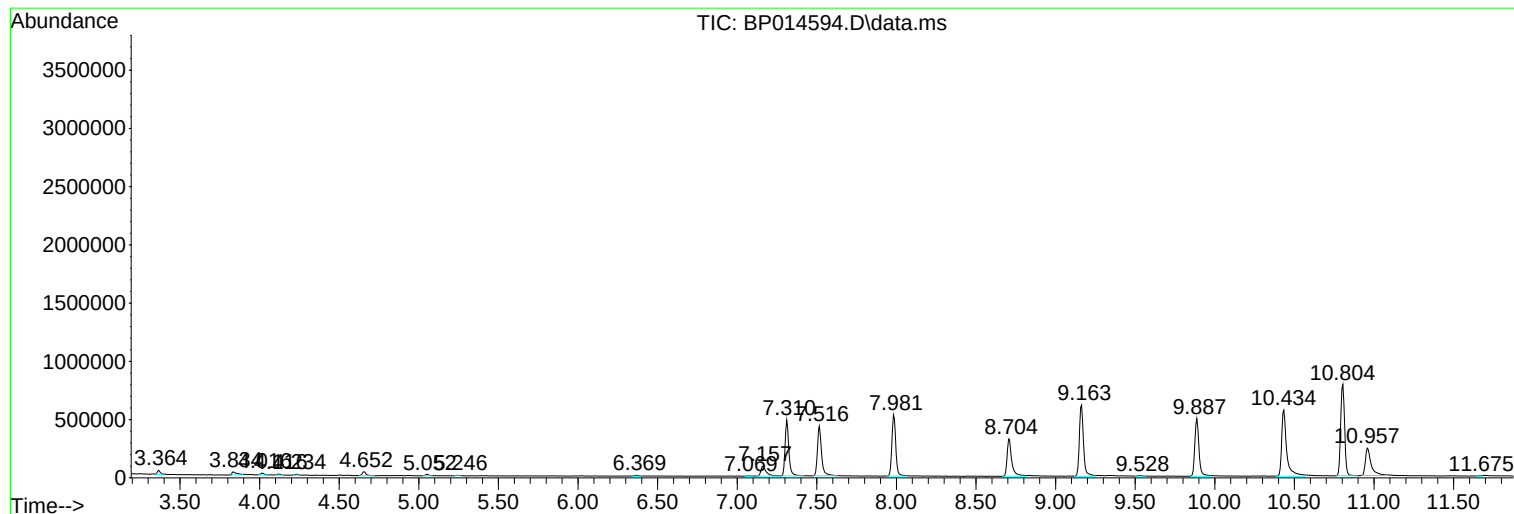

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014594.D
Acq On : 06 Apr 2023 18:57
Operator : CG/JU
Sample : 02194-06
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDW4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.998	6.72 ng/ul	654271	Acenaphthene-d10	14.634

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	97
2			Benzophenone	182	C13H10O	000119-61-9	96
3			Benzophenone	182	C13H10O	000119-61-9	96
4			Benzophenone	182	C13H10O	000119-61-9	95
5			Benzophenone	182	C13H10O	000119-61-9	91

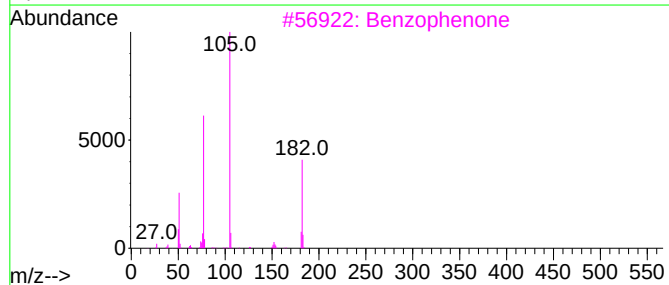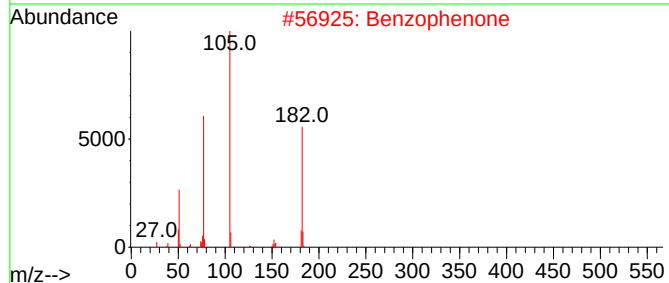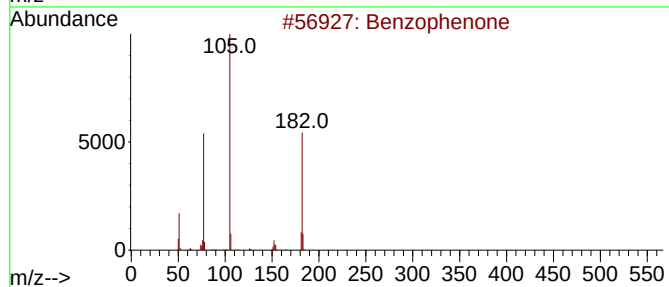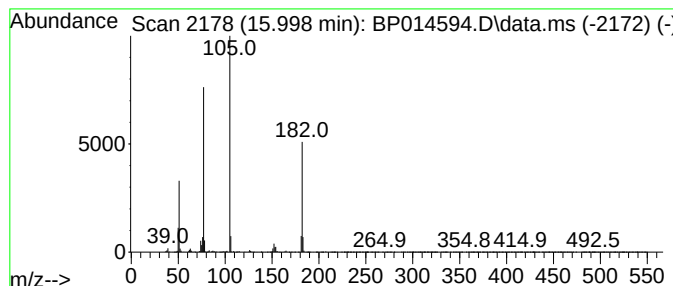

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014594.D
Acq On : 06 Apr 2023 18:57
Operator : CG/JU
Sample : 02194-06
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BHDW4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	15.998	6.7	ng/u1	654271	3	14.634	1947340	20.0