

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014600.D
 Acq On : 06 Apr 2023 22:21
 Operator : CG/JU
 Sample : 02225-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014600.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.364	27	30	38	rVB	32614	43596	0.83%	0.094%
2	3.811	105	106	128	rBV	76446	170830	3.27%	0.368%
3	4.016	137	141	145	rVB	16179	22875	0.44%	0.049%
4	4.122	155	159	164	rVB2	11736	19496	0.37%	0.042%
5	4.228	175	177	183	rVB5	7258	9328	0.18%	0.020%
6	4.499	220	223	229	rBV8	2848	6037	0.12%	0.013%
7	5.052	313	317	323	rVB3	9591	15921	0.30%	0.034%
8	6.363	536	540	547	rVB4	7873	12420	0.24%	0.027%
9	7.069	656	660	667	rVB6	5771	9060	0.17%	0.020%
10	7.157	667	675	689	rBV2	84610	196959	3.77%	0.424%
11	7.310	695	701	715	rBV	552843	911546	17.44%	1.963%
12	7.510	728	735	751	rBV	483635	875176	16.74%	1.885%
13	7.687	764	765	774	rVB9	3113	5290	0.10%	0.011%
14	7.981	807	815	831	rBV	663312	1102527	21.09%	2.375%
15	8.704	931	938	952	rBV	327029	637592	12.20%	1.373%
16	9.157	1008	1015	1030	rBV	700256	1255178	24.01%	2.704%
17	9.528	1072	1078	1083	rVB	25874	38330	0.73%	0.083%
18	9.887	1130	1139	1160	rBV	585891	1080020	20.66%	2.326%
19	10.428	1224	1231	1255	rBV	631129	1365698	26.13%	2.942%
20	10.745	1281	1285	1287	rBV5	4241	5627	0.11%	0.012%
21	10.798	1287	1294	1309	rVB	977479	1697675	32.48%	3.657%
22	10.951	1313	1320	1350	rBV	412539	1024328	19.60%	2.206%
23	12.028	1492	1503	1510	rVB2	22830	39884	0.76%	0.086%
24	12.204	1529	1533	1544	rVB6	8551	16886	0.32%	0.036%
25	12.398	1561	1566	1576	rVV3	10414	23750	0.45%	0.051%
26	13.434	1735	1742	1747	rBV3	14676	24925	0.48%	0.054%
27	13.604	1766	1771	1777	rVB10	3133	5497	0.11%	0.012%
28	14.039	1835	1845	1858	rBV	1793720	2664904	50.98%	5.740%
29	14.328	1884	1894	1913	rBV	1998554	2980219	57.01%	6.419%
30	14.504	1921	1924	1929	rVB	18384	23849	0.46%	0.051%
31	14.634	1938	1946	1956	rBV	1669009	2450332	46.88%	5.278%
32	14.922	1990	1995	1996	rBV3	16918	28158	0.54%	0.061%
33	15.463	2081	2087	2091	rBV2	17617	27090	0.52%	0.058%
34	15.569	2101	2105	2108	rBV6	5677	9190	0.18%	0.020%
35	15.628	2109	2115	2130	rBV	2546101	3819453	73.07%	8.227%
36	15.763	2130	2138	2151	rBV	862646	1418945	27.15%	3.056%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
 Data File : BP014600.D
 Acq On : 06 Apr 2023 22:21
 Operator : CG/JU
 Sample : 02225-02
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AB8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Title : SVOA CALIBRATION

37	16.004	2174	2179	2188	rVB	39910	72219	1.38%	0.156%
38	16.328	2228	2234	2240	rBV	18572	31820	0.61%	0.069%
39	17.069	2356	2360	2366	rBV7	3448	6189	0.12%	0.013%
40	17.128	2366	2370	2373	rVV2	11593	12861	0.25%	0.028%
41	17.180	2376	2379	2383	rVB6	5705	8344	0.16%	0.018%
42	17.392	2409	2415	2426	rBV	2096139	3036227	58.09%	6.540%
43	17.492	2426	2432	2448	rVV	3012442	4604512	88.09%	9.918%
44	17.869	2492	2496	2498	rBV5	8399	11309	0.22%	0.024%
45	18.045	2524	2526	2530	rVB5	8532	9791	0.19%	0.021%
46	18.269	2560	2564	2572	rBV3	33330	71865	1.37%	0.155%
47	18.533	2607	2609	2612	rBV3	5835	6396	0.12%	0.014%
48	19.139	2709	2712	2715	rBV5	13155	16834	0.32%	0.036%
49	19.304	2736	2740	2746	rBV	38554	53728	1.03%	0.116%
50	19.374	2748	2752	2759	rVV3	31760	59449	1.14%	0.128%
51	19.627	2793	2795	2799	rVB5	21206	18486	0.35%	0.040%
52	19.727	2805	2812	2821	rBV	3794267	5227209	100.00%	11.259%
53	21.480	3105	3110	3125	rBV	1970285	2965684	56.74%	6.388%
54	23.815	3500	3507	3519	rBV	1882467	3866394	73.97%	8.328%
55	23.980	3529	3535	3548	rVB2	1073261	2306984	44.13%	4.969%




Sum of corrected areas: 46424892

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014600.D
Acq On : 06 Apr 2023 22:21
Operator : CG/JU
Sample : 02225-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

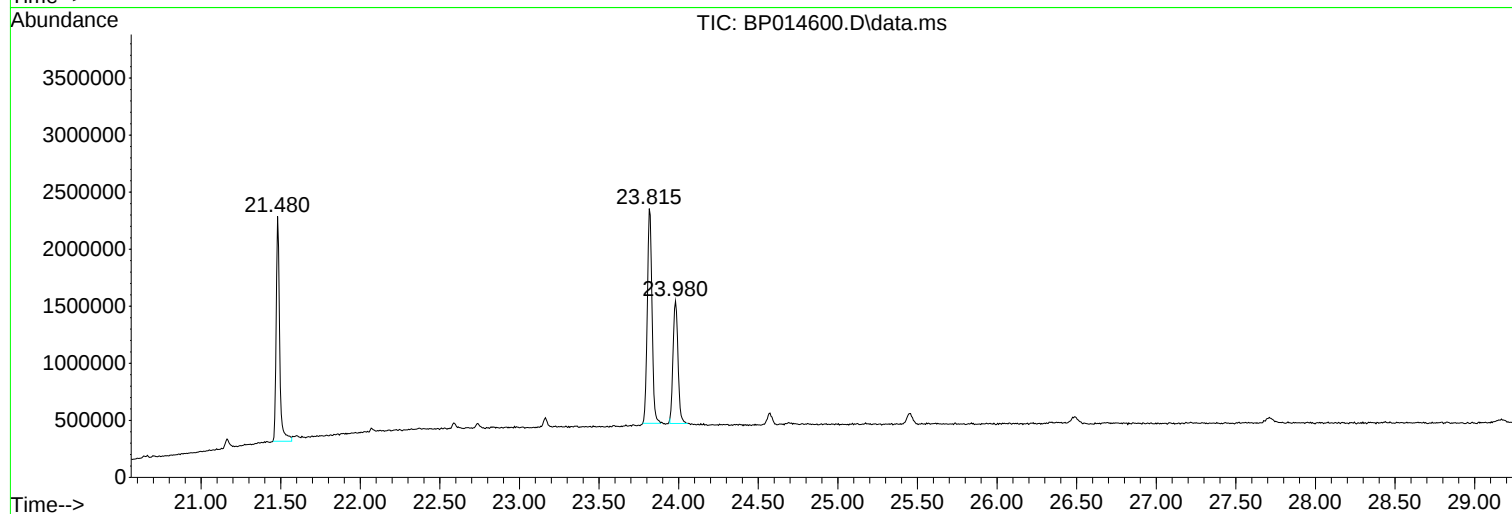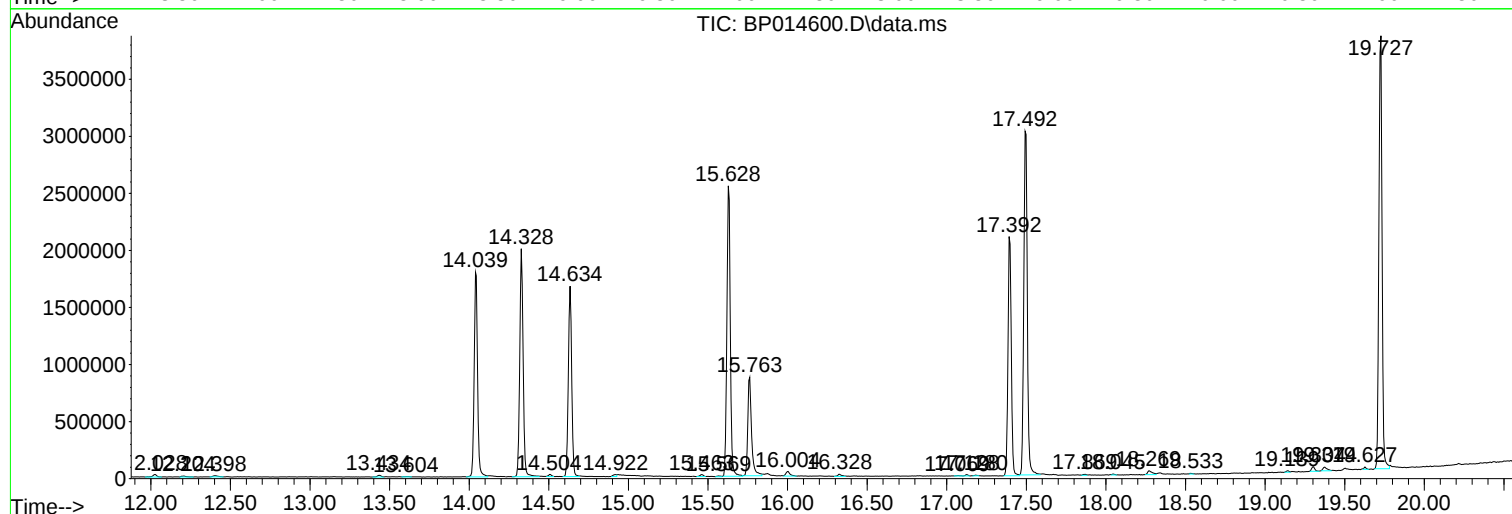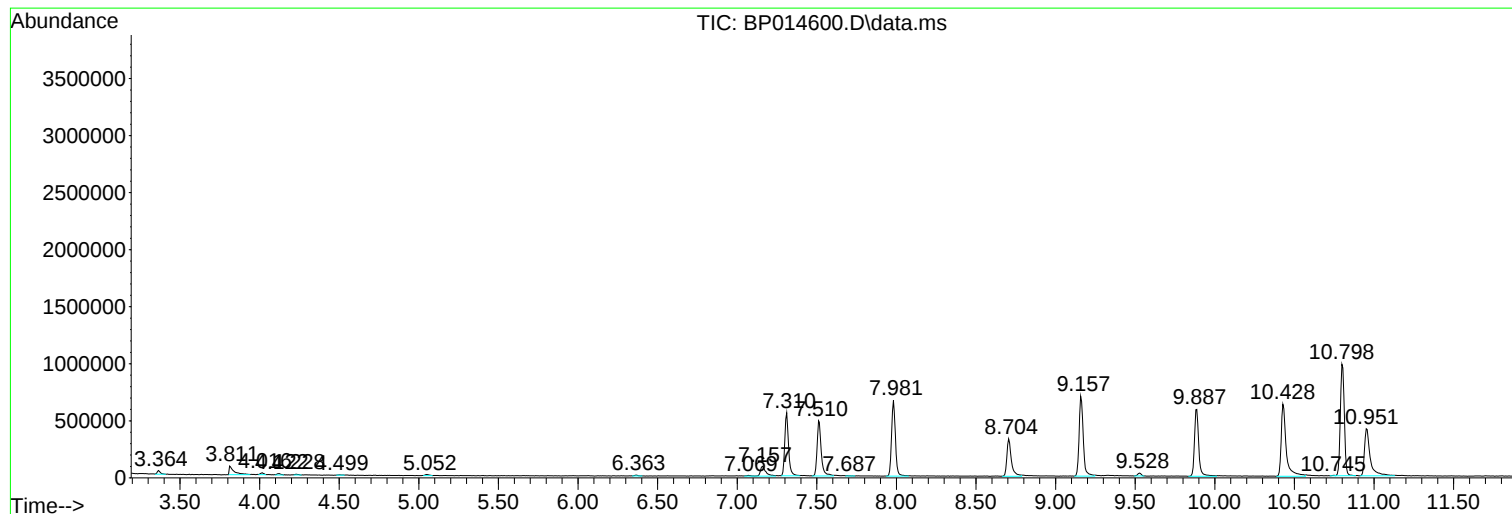

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014600.D
Acq On : 06 Apr 2023 22:21
Operator : CG/JU
Sample : 02225-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040523\
Data File : BP014600.D
Acq On : 06 Apr 2023 22:21
Operator : CG/JU
Sample : 02225-02
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AB8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc