
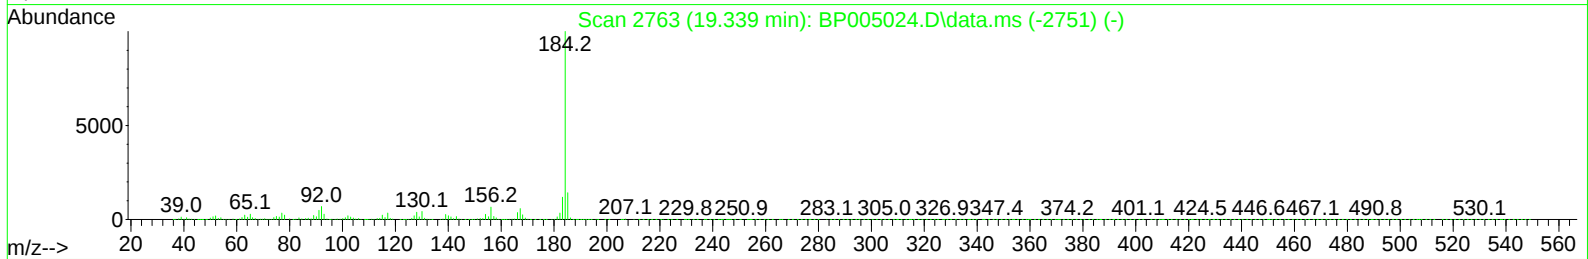
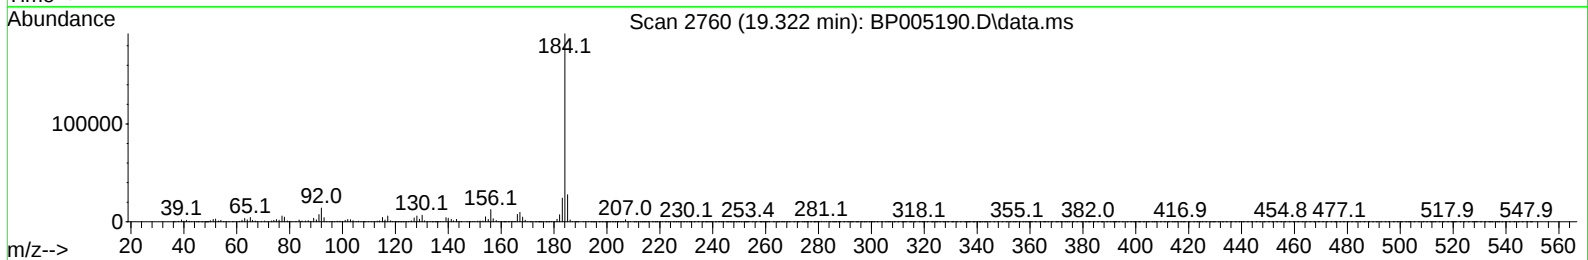


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040621\
 Data File : BP005190.D
 Acq On : 06 Apr 2021 10:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 12:04:24 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 12:23:57 2021
 Response via : Initial Calibration

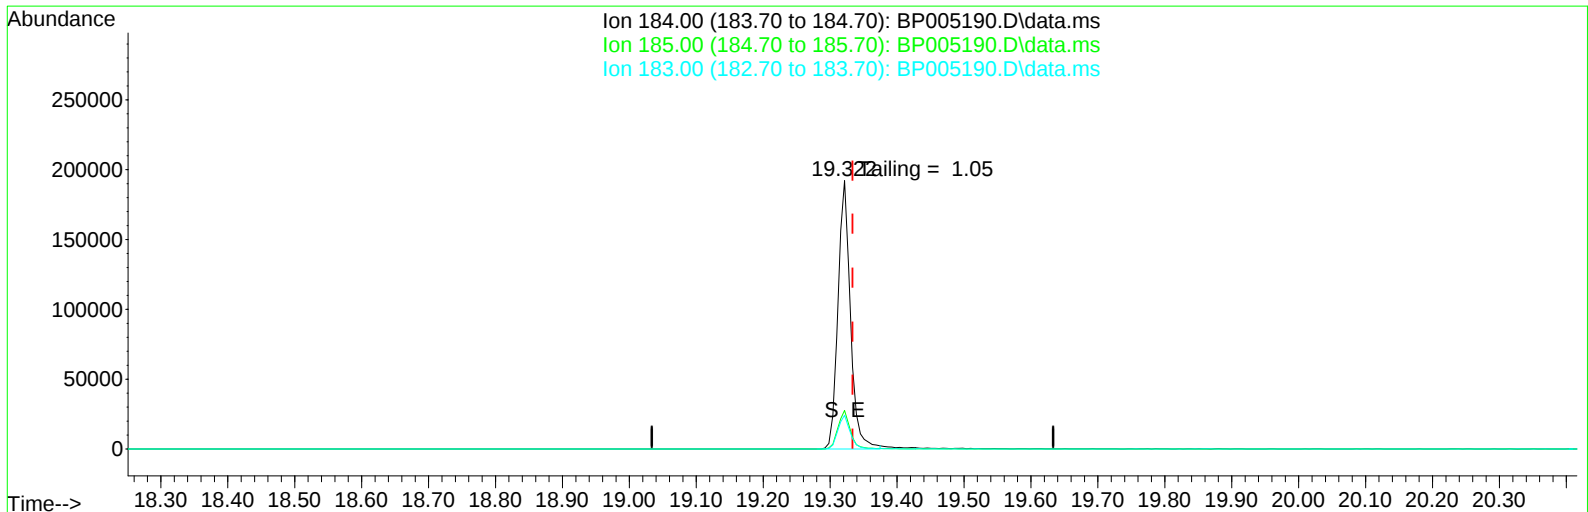




TIC: BP005190.D\data.ms

(77) Benzidine**19.322min (-0.012) 197562.52 ng****response 251405**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.39
183.00	12.00	12.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040621\
 Data File : BP005190.D
 Acq On : 06 Apr 2021 10:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 12:04:24 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 12:23:57 2021
 Response via : Initial Calibration

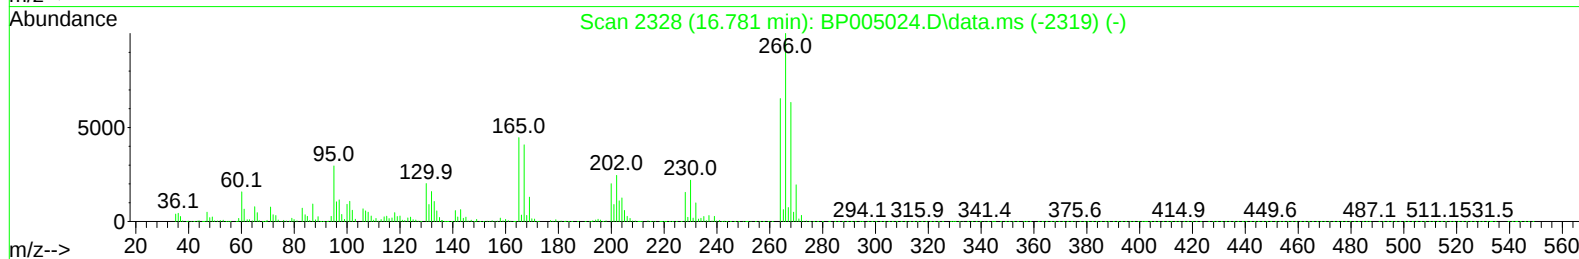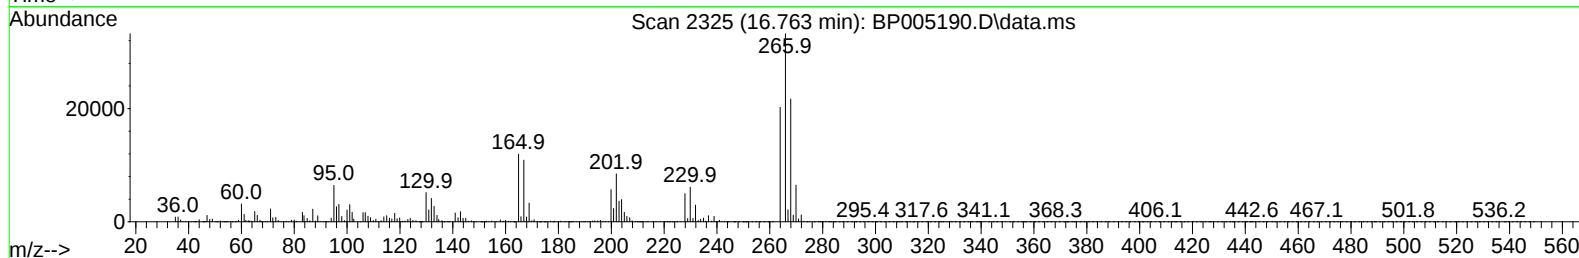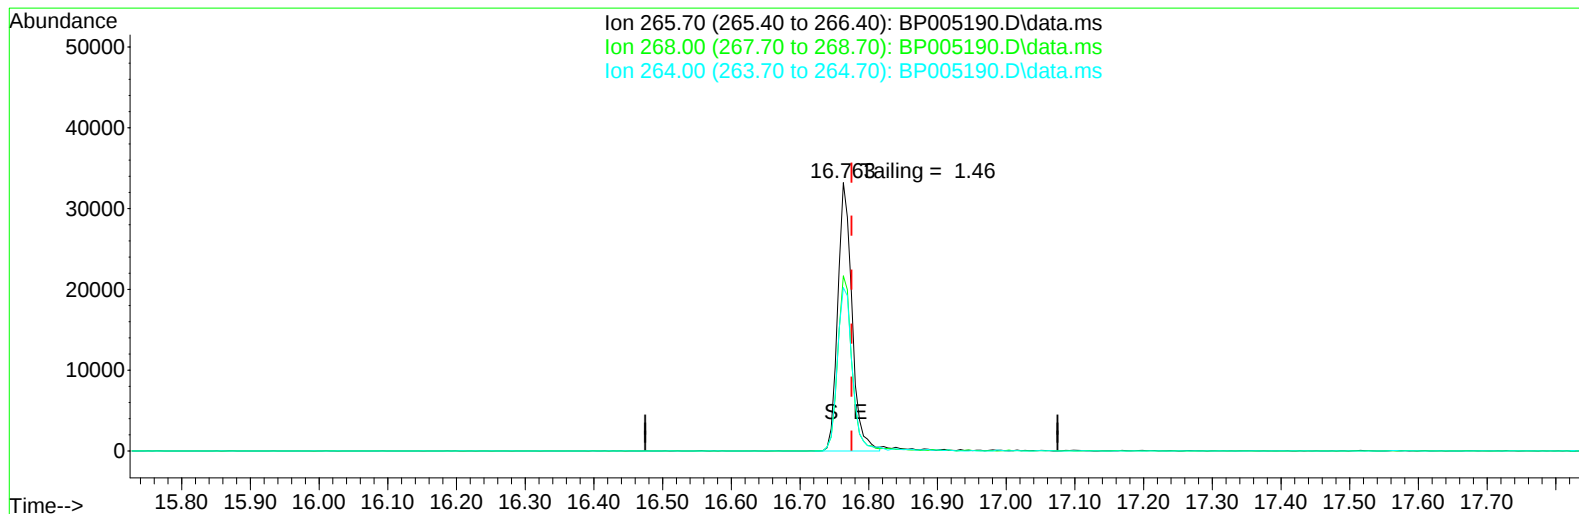

TIC: BP005190.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.012) 224097.01 ng

response 48197

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	65.29
264.00	63.30	60.89
0.00	0.00	0.00