

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040621\
 Data File : BP005194.D
 Acq On : 06 Apr 2021 13:46
 Operator : CG/JU
 Sample : M1874-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FS-SB16(45-46)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005194.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.299	369	376	385	rVB	329088	479792	8.87%	1.951%
2	6.881	638	645	661	rVB	317890	514838	9.52%	2.093%
3	7.693	777	783	792	rVB	80685	127882	2.36%	0.520%
4	8.858	972	981	988	rBV	199315	327810	6.06%	1.333%
5	10.487	1250	1258	1267	rBV	102891	169538	3.13%	0.689%
6	12.969	1673	1680	1689	rVB	478311	673421	12.45%	2.738%
7	14.351	1910	1915	1922	rVB2	140831	208247	3.85%	0.847%
8	15.745	2147	2152	2158	rBV	58472	85572	1.58%	0.348%
9	15.857	2165	2171	2176	rBV	325235	472588	8.74%	1.921%
10	16.151	2218	2221	2231	rVB5	38571	81727	1.51%	0.332%
11	16.516	2277	2283	2291	rVB6	31334	61059	1.13%	0.248%
12	17.116	2379	2385	2390	rBV	170940	239170	4.42%	0.972%
13	17.798	2486	2501	2503	rBV	425214	937767	17.34%	3.813%
14	17.992	2520	2534	2536	rBV	523901	1565098	28.94%	6.363%
15	18.022	2536	2539	2546	rVV	744099	1298637	24.01%	5.280%
16	18.157	2546	2562	2571	rVB	1539815	5408343	100.00%	21.989%
17	18.334	2580	2592	2602	rVB3	165161	513355	9.49%	2.087%
18	18.539	2621	2627	2636	rVB3	38853	98309	1.82%	0.400%
19	18.904	2684	2689	2692	rBV	577586	655026	12.11%	2.663%
20	18.933	2692	2694	2699	rVB2	414160	435249	8.05%	1.770%
21	19.063	2713	2716	2720	rVB	91721	94515	1.75%	0.384%
22	19.163	2721	2733	2746	rBV	1564175	3646025	67.41%	14.824%
23	19.269	2747	2751	2763	rVB	636191	868841	16.06%	3.533%
24	19.692	2818	2823	2828	rBV	849916	987836	18.27%	4.016%
25	20.033	2876	2881	2889	rVB	176467	316720	5.86%	1.288%
26	20.316	2925	2929	2933	rBV	264419	324486	6.00%	1.319%
27	20.369	2936	2938	2944	rVB2	60448	70353	1.30%	0.286%
28	20.780	3003	3008	3013	rVB	229488	347019	6.42%	1.411%
29	20.869	3017	3023	3026	rBV2	181085	271079	5.01%	1.102%
30	20.933	3030	3034	3041	rVV2	136268	248580	4.60%	1.011%
31	20.998	3042	3045	3049	rVB	69744	76528	1.41%	0.311%
32	21.216	3077	3082	3086	rVB	232044	294330	5.44%	1.197%
33	21.416	3111	3116	3127	rBV	300573	442751	8.19%	1.800%
34	22.086	3224	3230	3236	rVB	249989	423867	7.84%	1.723%
35	22.269	3257	3261	3269	rVB	93489	130686	2.42%	0.531%
36	22.822	3347	3355	3363	rVB2	203429	462263	8.55%	1.879%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040621\
Data File : BP005194.D
Acq On : 06 Apr 2021 13:46
Operator : CG/JU
Sample : M1874-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FS-SB16(45-46)

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	23.092	3397	3401	3409	rVB6	72563	144513	2.67%	0.588%
38	23.498	3464	3470	3483	rVB	162729	366959	6.79%	1.492%
39	23.663	3491	3498	3505	rVB	133769	305802	5.65%	1.243%
40	25.468	3798	3805	3818	rVB6	131165	418628	7.74%	1.702%




Sum of corrected areas: 24595209

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040621\
Data File : BP005194.D
Acq On : 06 Apr 2021 13:46
Operator : CG/JU
Sample : M1874-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FS-SB16(45-46)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

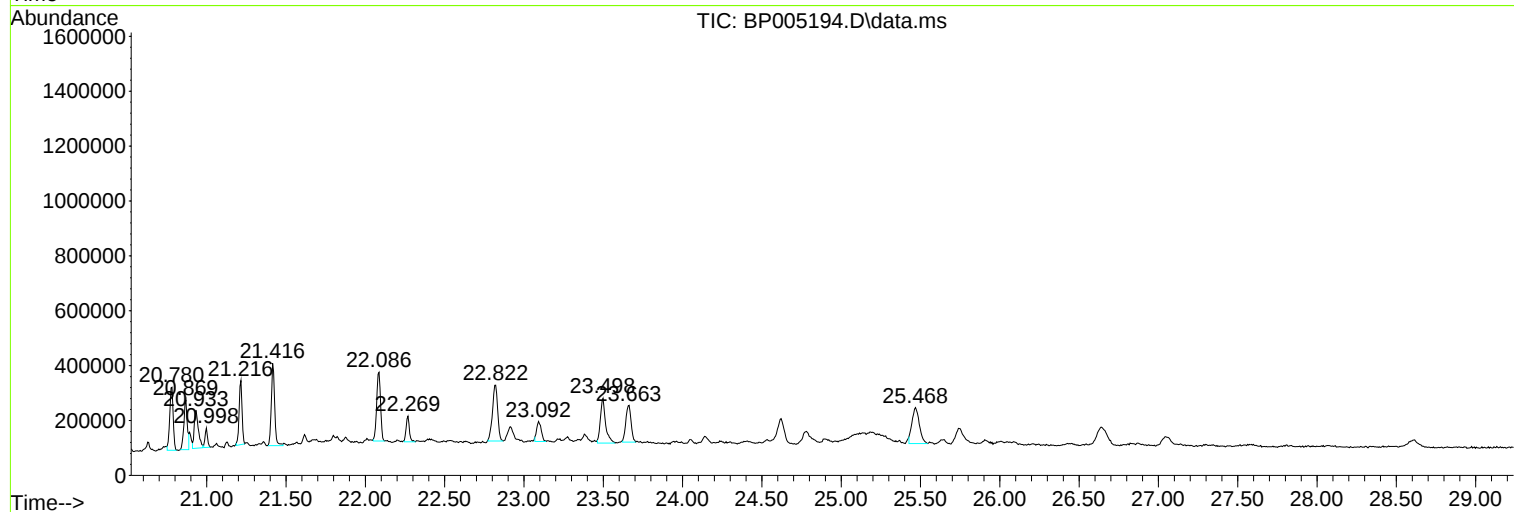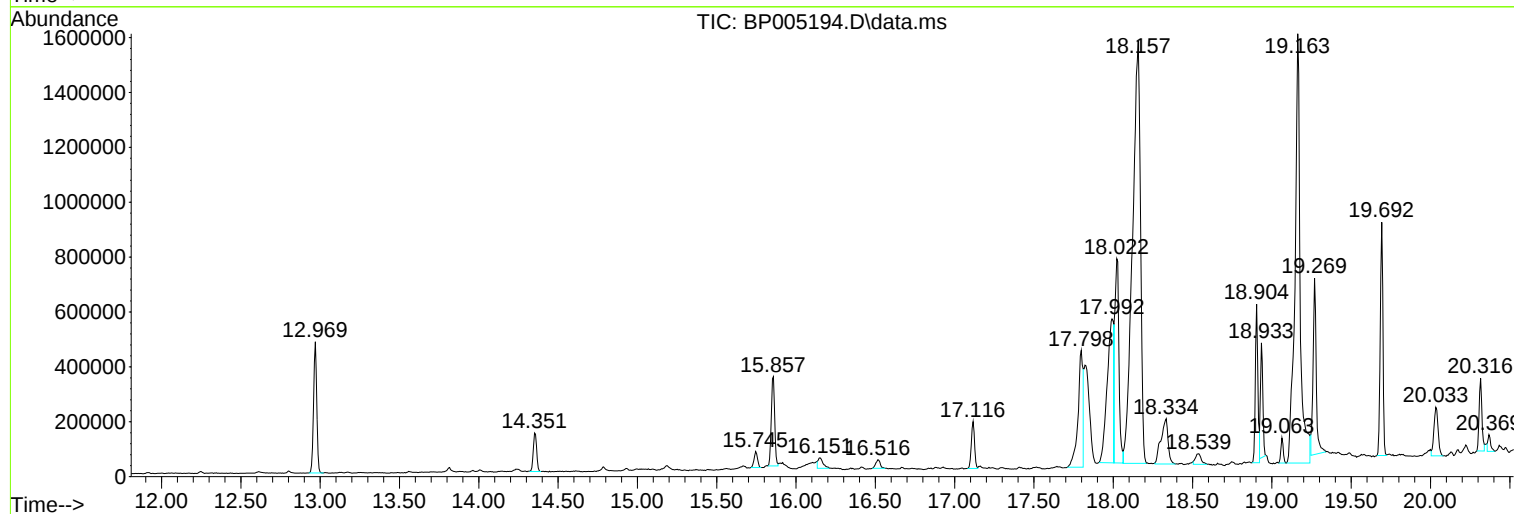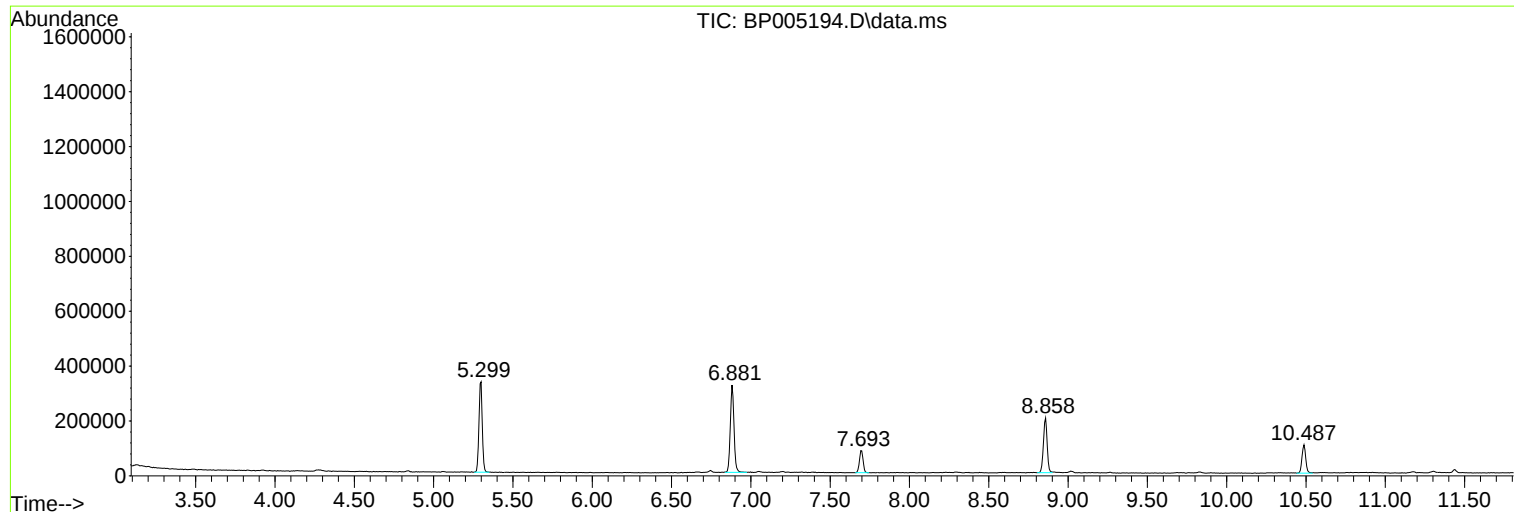

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040621\
Data File : BP005194.D
Acq On : 06 Apr 2021 13:46
Operator : CG/JU
Sample : M1874-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FS-SB16(45-46)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040621\
Data File : BP005194.D
Acq On : 06 Apr 2021 13:46
Operator : CG/JU
Sample : M1874-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FS-SB16(45-46)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc