
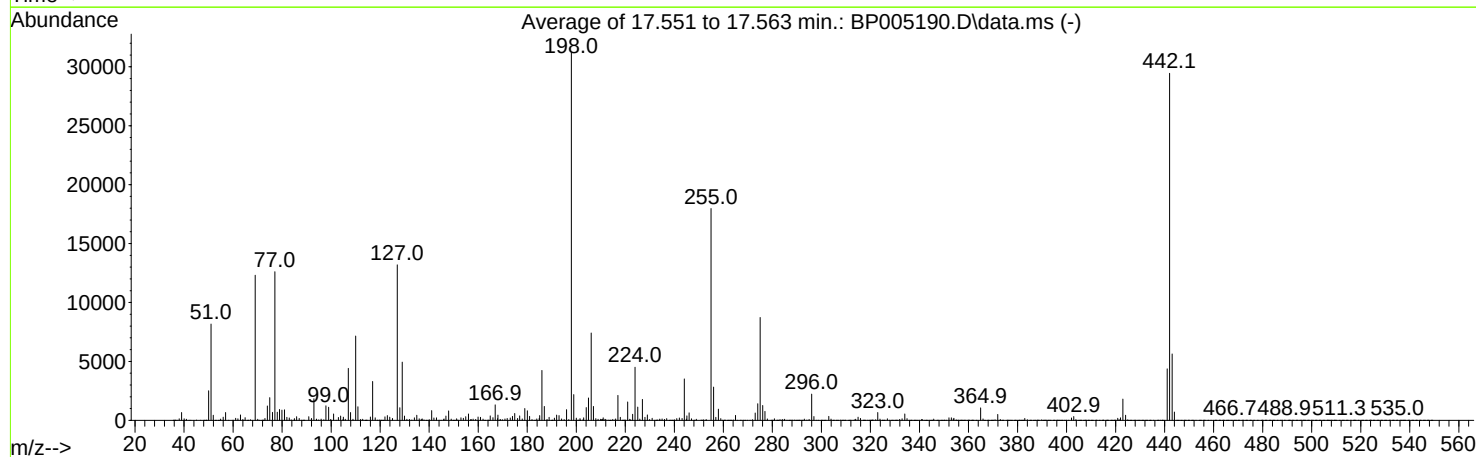


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040621\
 Data File : BP005190.D
 Acq On : 06 Apr 2021 10:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 06 12:33:08 2021

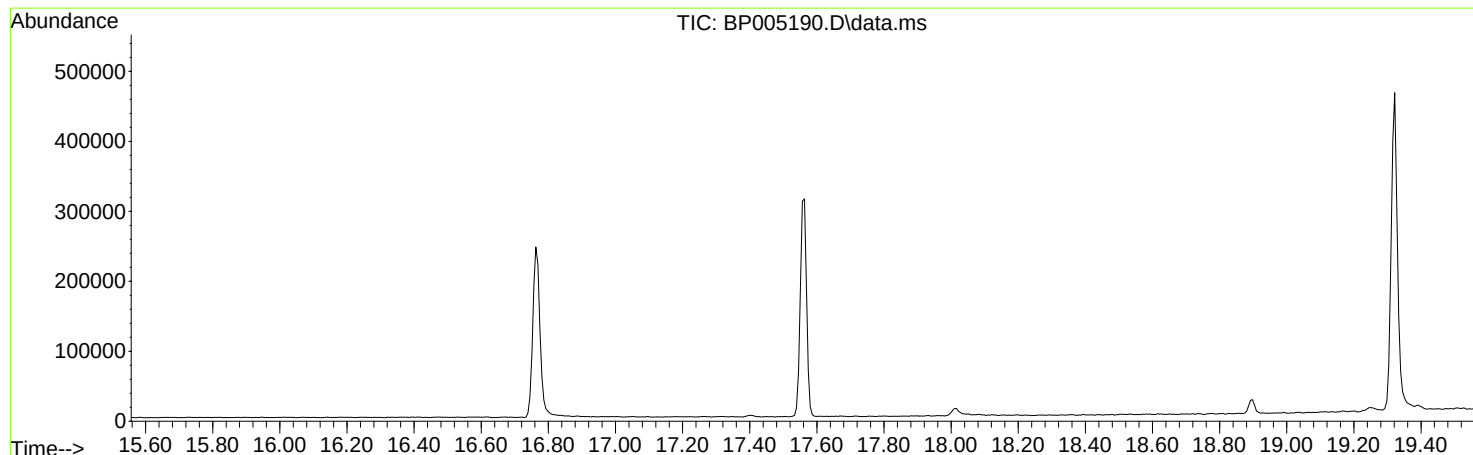

AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2449

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.2	8177	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.5	12321	PASS
70	69	0.00	2	0.8	94	PASS
127	198	10	80	42.3	13193	PASS
197	198	0.00	2	0.2	68	PASS
198	198	100	100	100.0	31211	PASS
199	198	5	9	7.0	2185	PASS
275	198	10	60	28.0	8730	PASS
365	198	1	100	3.4	1064	PASS
441	198	0.01	100	14.0	4378	PASS
442	442	100	100	100.0	29446	PASS
443	442	15	24	19.2	5640	PASS

Instrument :
BNA_P
ClientSampleId :
DFTPP

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/6/2021	BNA_P	<u>BP005190.D</u>
Compound Name	Response	Retention Time
DDT	131735	20.52
DDD	4996	20.09
DDE	442	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5438	137173	3.96

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040621\
Data File : BP005190.D
Acq On : 06 Apr 2021 10:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 06 12:04:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 01 12:23:57 2021
Response via : Initial Calibration

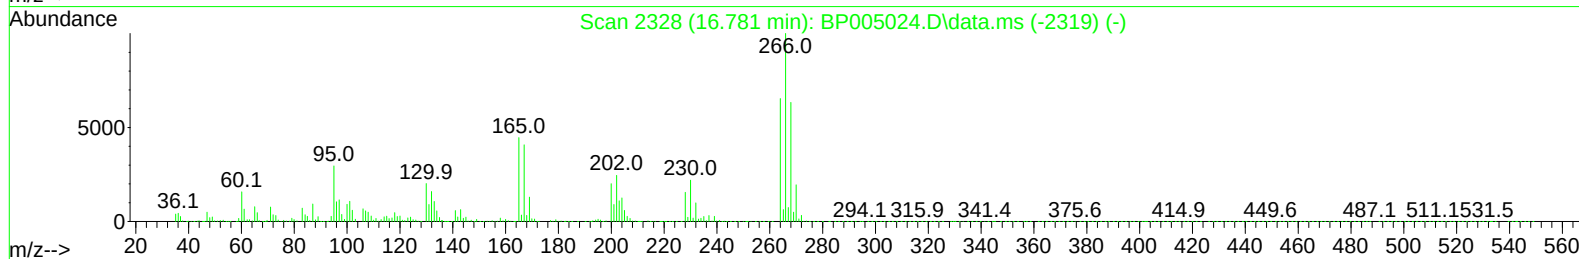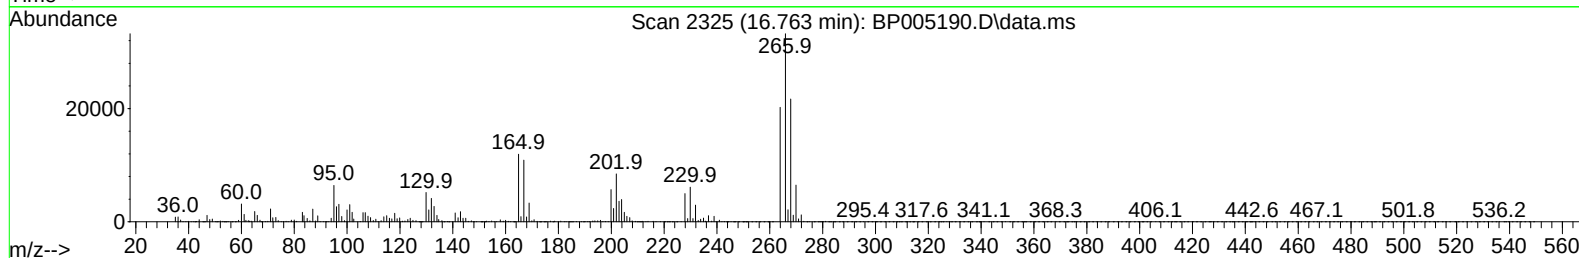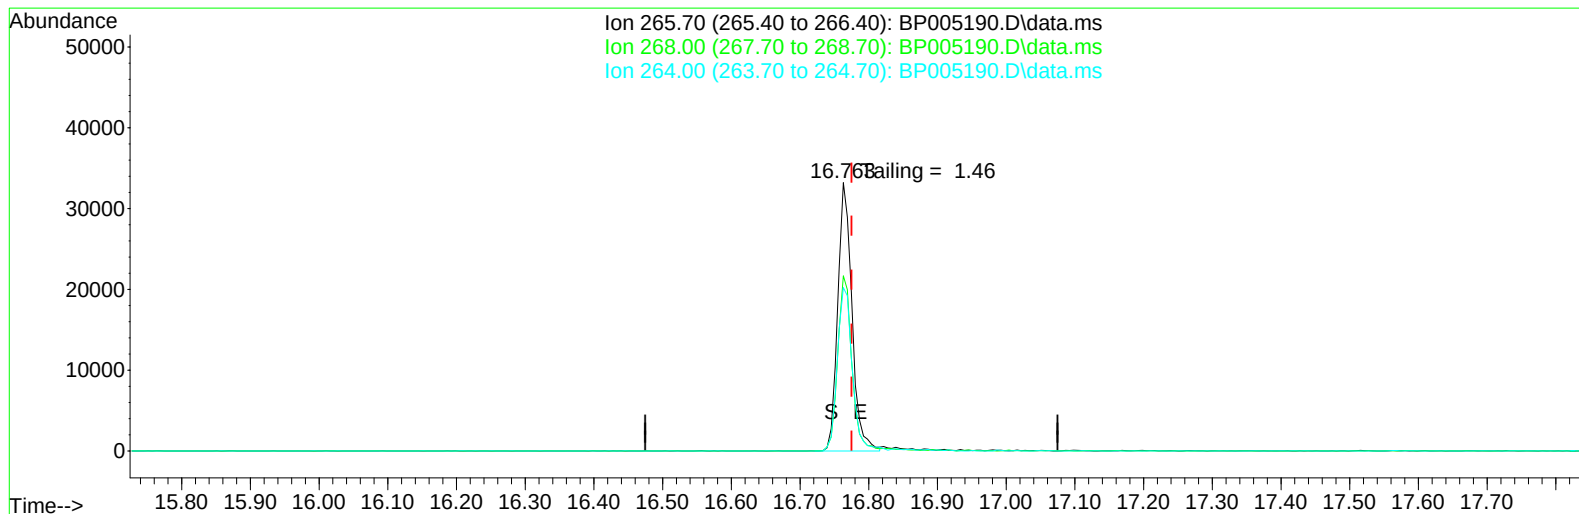

TIC: BP005190.D\data.ms

(70) Pentachlorophenol (C)

16.763min (-0.012) 224097.01 ng




response 48197

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	65.29
264.00	63.30	60.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040621\
 Data File : BP005190.D
 Acq On : 06 Apr 2021 10:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 06 12:04:24 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 01 12:23:57 2021
 Response via : Initial Calibration

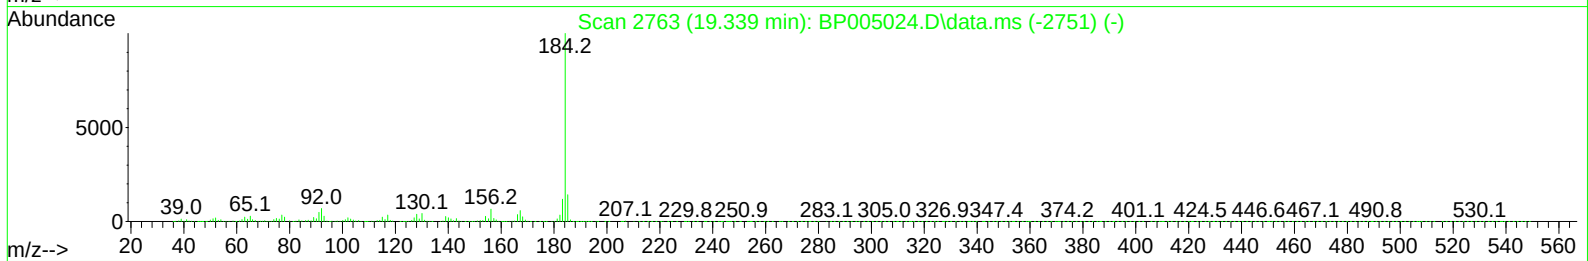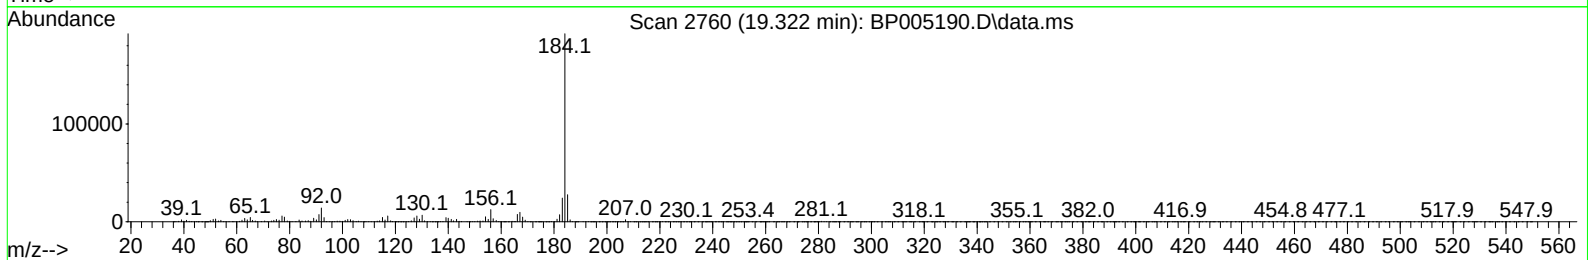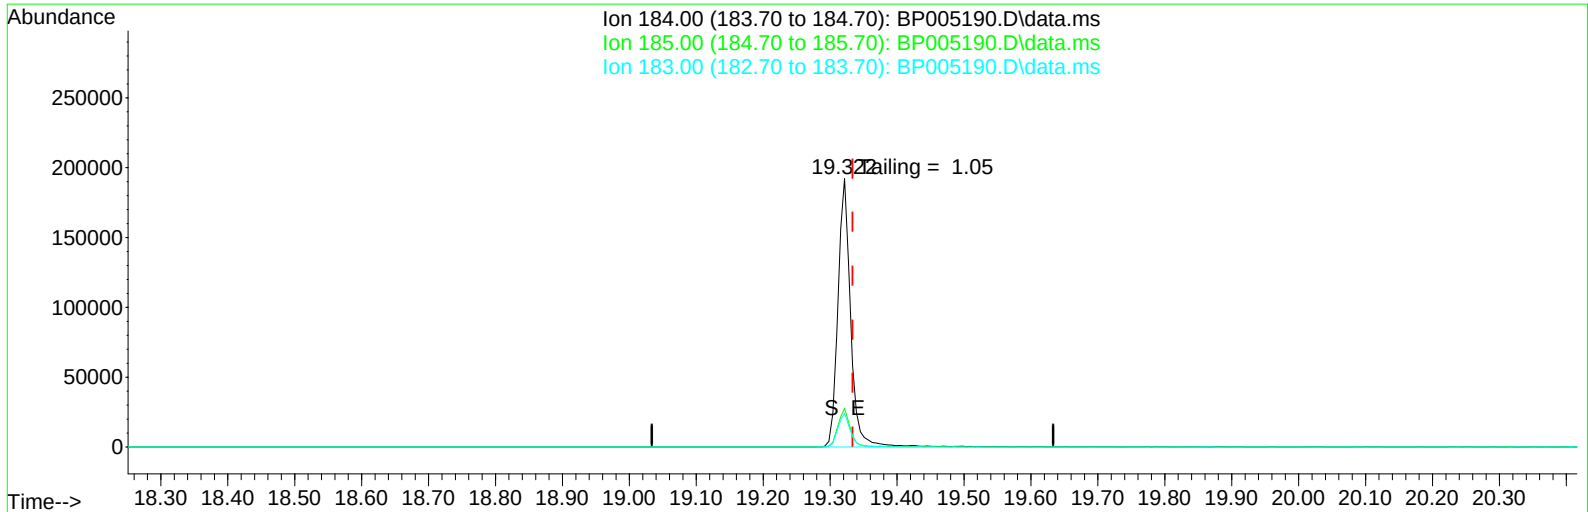

TIC: BP005190.D\data.ms

(77) Benzidine

19.322min (-0.012) 197562.52 ng

response 251405

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.39
183.00	12.00	12.61
0.00	0.00	0.00