
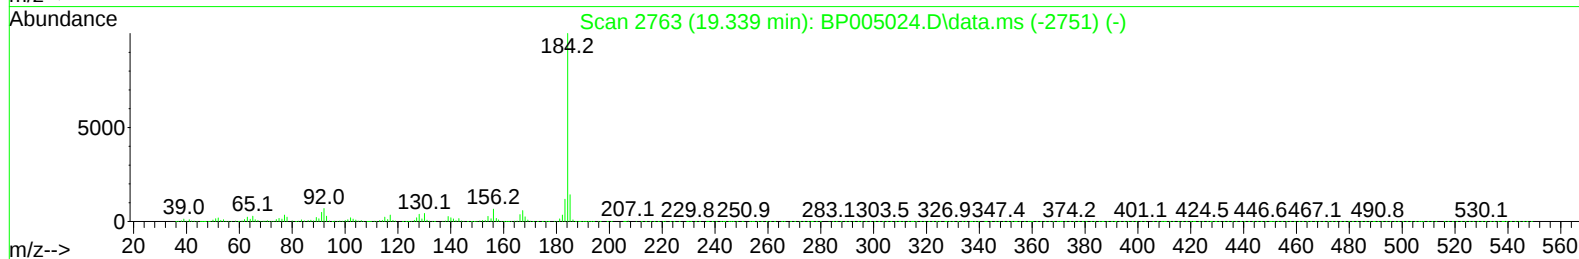
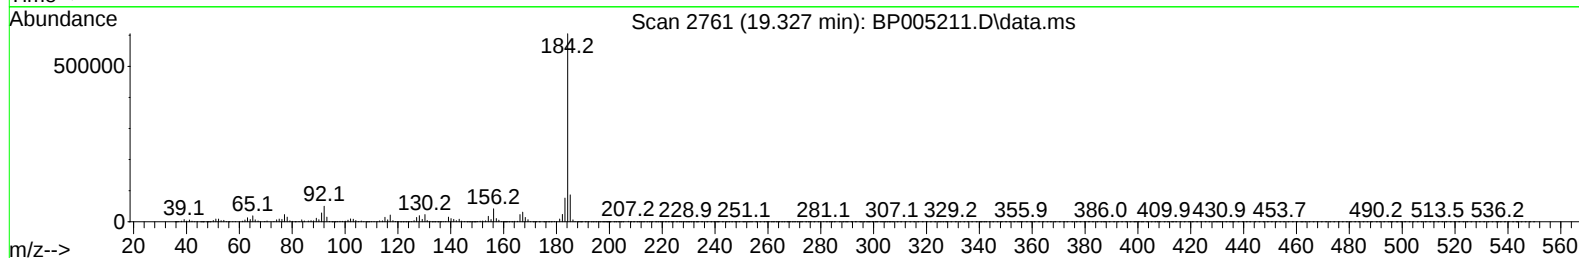


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040721\
Data File : BP005211.D
Acq On : 07 Apr 2021 09:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 10:59:55 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 06 12:33:08 2021
Response via : Initial Calibration



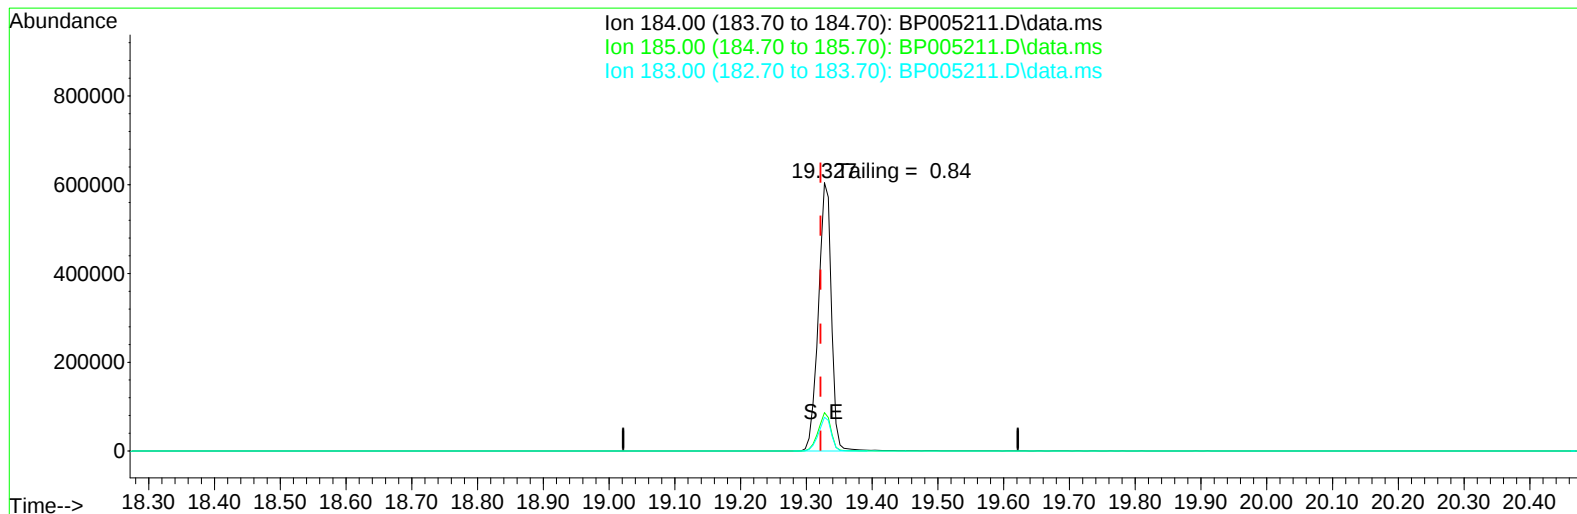


TIC: BP005211.D\data.ms

(77) Benzidine**19.327min (+ 0.006) 1122464.84 ng****response 837323**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.30
183.00	12.00	12.58
0.00	0.00	0.00

Quant Time: Apr 07 10:59:55 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 06 12:33:08 2021
Response via : Initial Calibration

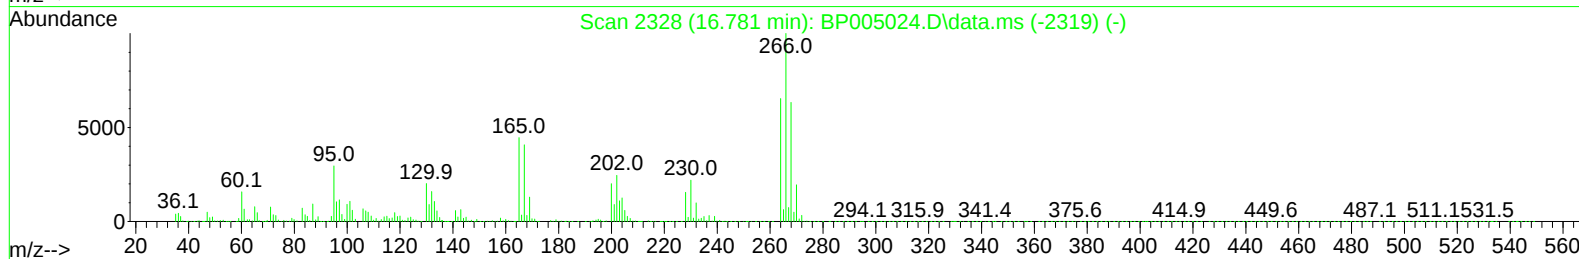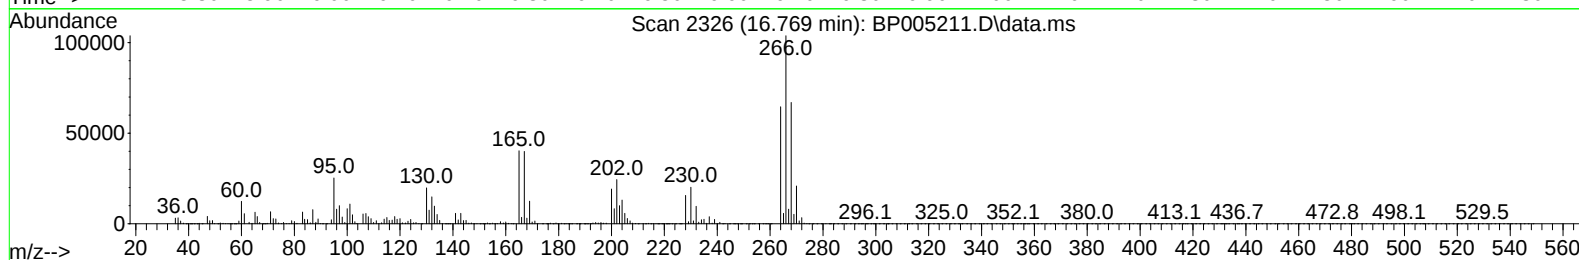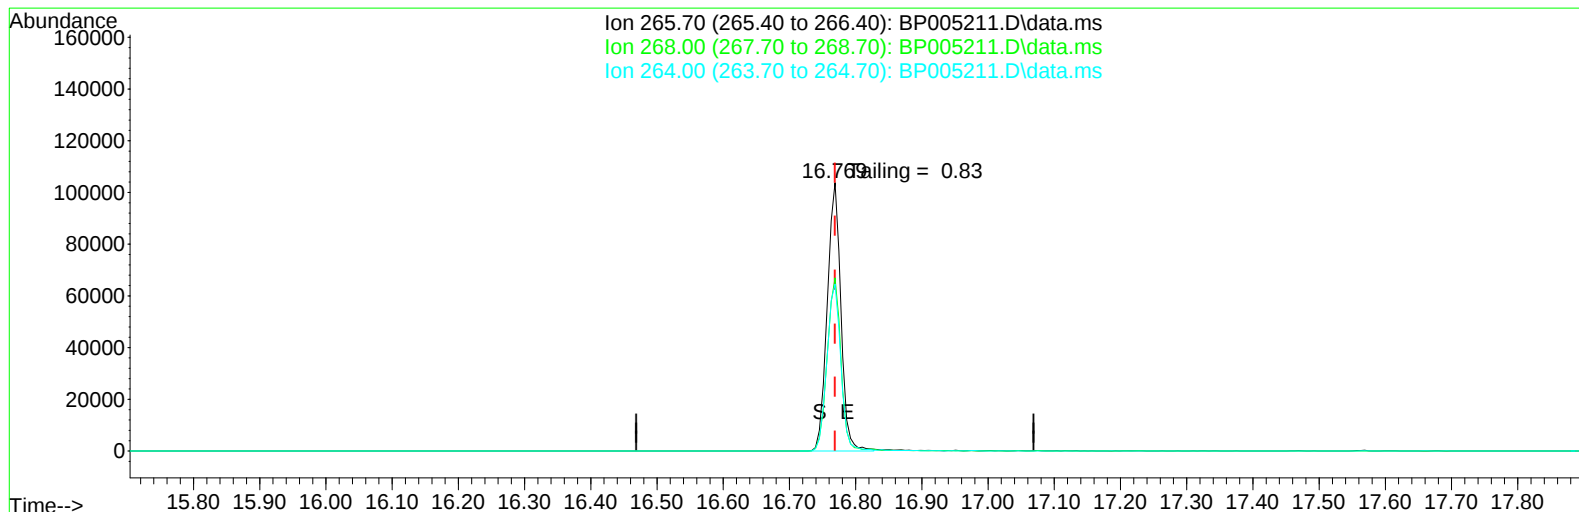

TIC: BP005211.D\data.ms

(70) Pentachlorophenol (C)

16.769min (+ 0.000) 2190995.59 ng

response **150791**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.51
264.00	63.30	62.22
0.00	0.00	0.00