

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040721\
 Data File : BP005222.D
 Acq On : 07 Apr 2021 16:01
 Operator : CG/JU
 Sample : M1961-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 TR2-A-D-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	33	rVB	58163	66836	4.31%	1.024%
2	4.352	211	215	220	rVB	59732	70623	4.55%	1.082%
3	4.799	287	291	295	rBV	31692	41157	2.65%	0.630%
4	4.840	295	298	304	rVB	17321	24387	1.57%	0.374%
5	5.293	369	375	383	rVB	433128	595437	38.40%	9.120%
6	6.875	637	644	657	rBV	327826	509818	32.88%	7.808%
7	7.693	775	783	790	rBV	76936	122609	7.91%	1.878%
8	8.852	971	980	998	rBV	273355	440202	28.39%	6.742%
9	10.481	1250	1257	1264	rBV	88312	149080	9.61%	2.283%
10	12.963	1672	1679	1691	rBV	577809	851631	54.92%	13.044%
11	13.245	1720	1727	1733	rBV2	9395	16299	1.05%	0.250%
12	13.810	1817	1823	1834	rBV	24524	36487	2.35%	0.559%
13	14.345	1908	1914	1928	rVB	137226	209240	13.49%	3.205%
14	15.845	2163	2169	2179	rBV	526144	782697	50.47%	11.988%
15	17.104	2377	2383	2390	rBV	159866	238259	15.36%	3.649%
16	18.010	2532	2537	2546	rBV3	36750	61434	3.96%	0.941%
17	19.245	2743	2747	2753	rBV2	16048	23226	1.50%	0.356%
18	19.680	2816	2821	2828	rBV	1235774	1550723	100.00%	23.751%
19	20.921	3028	3032	3038	rVB4	42906	59315	3.82%	0.908%
20	21.204	3076	3080	3085	rBV2	257356	311798	20.11%	4.776%
21	23.486	3462	3468	3478	rVB2	191977	367757	23.72%	5.633%




Sum of corrected areas: 6529015

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040721\
Data File : BP005222.D
Acq On : 07 Apr 2021 16:01
Operator : CG/JU
Sample : M1961-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TR2-A-D-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

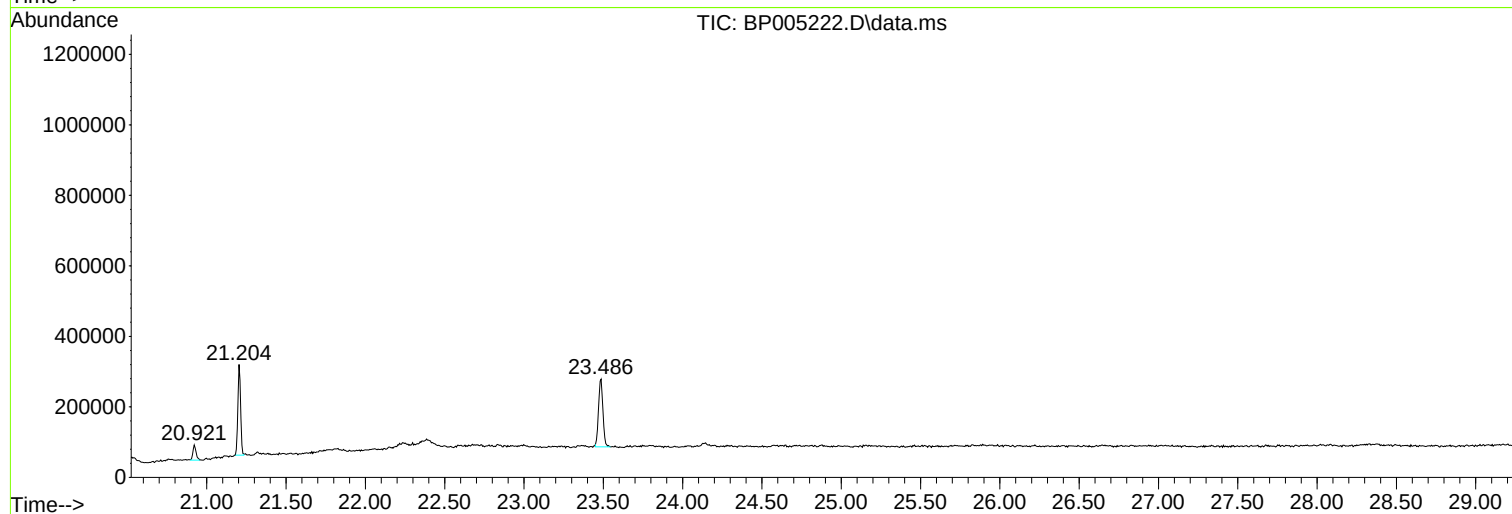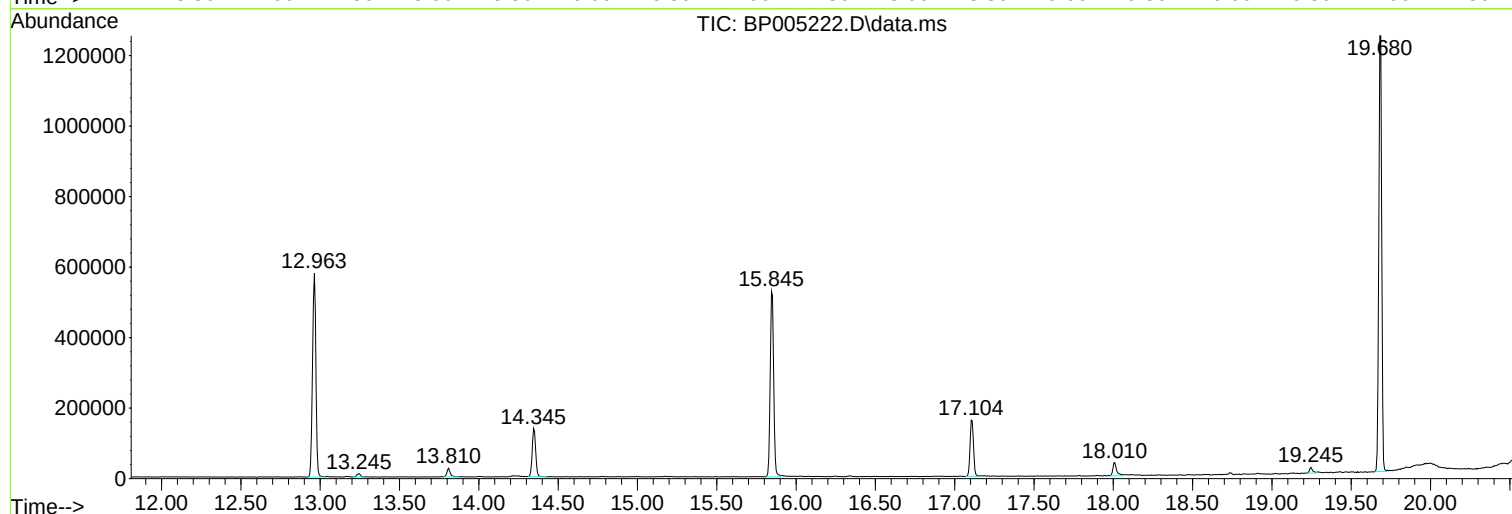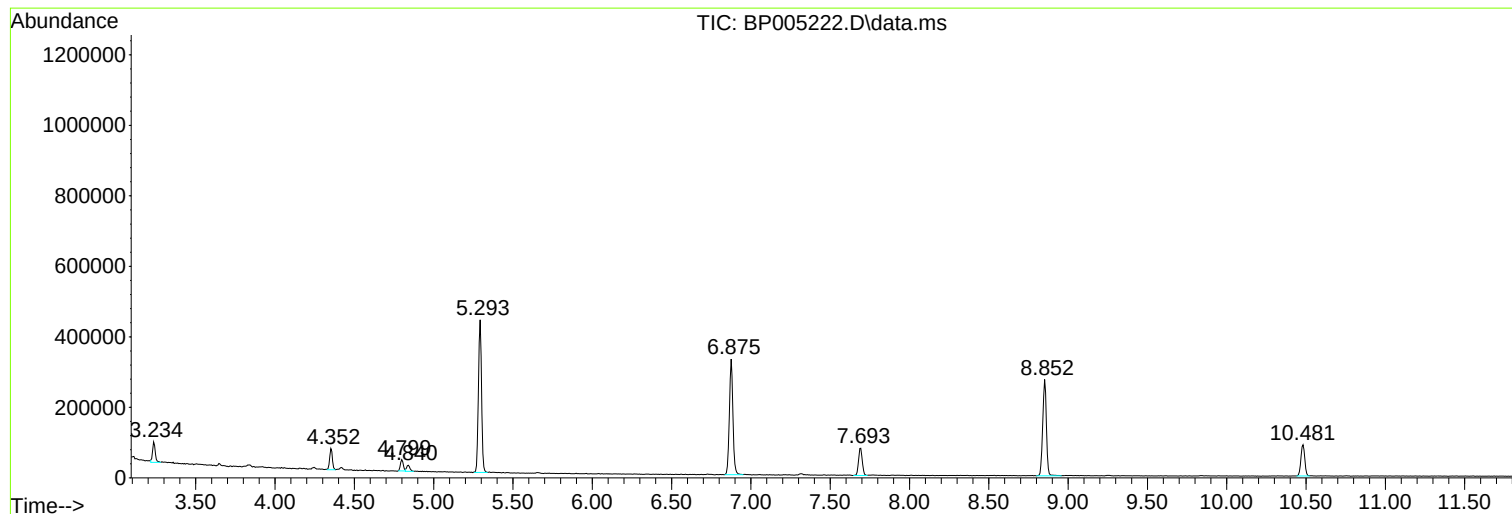

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040721\
Data File : BP005222.D
Acq On : 07 Apr 2021 16:01
Operator : CG/JU
Sample : M1961-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TR2-A-D-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040721\
Data File : BP005222.D
Acq On : 07 Apr 2021 16:01
Operator : CG/JU
Sample : M1961-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
TR2-A-D-COMP

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------