
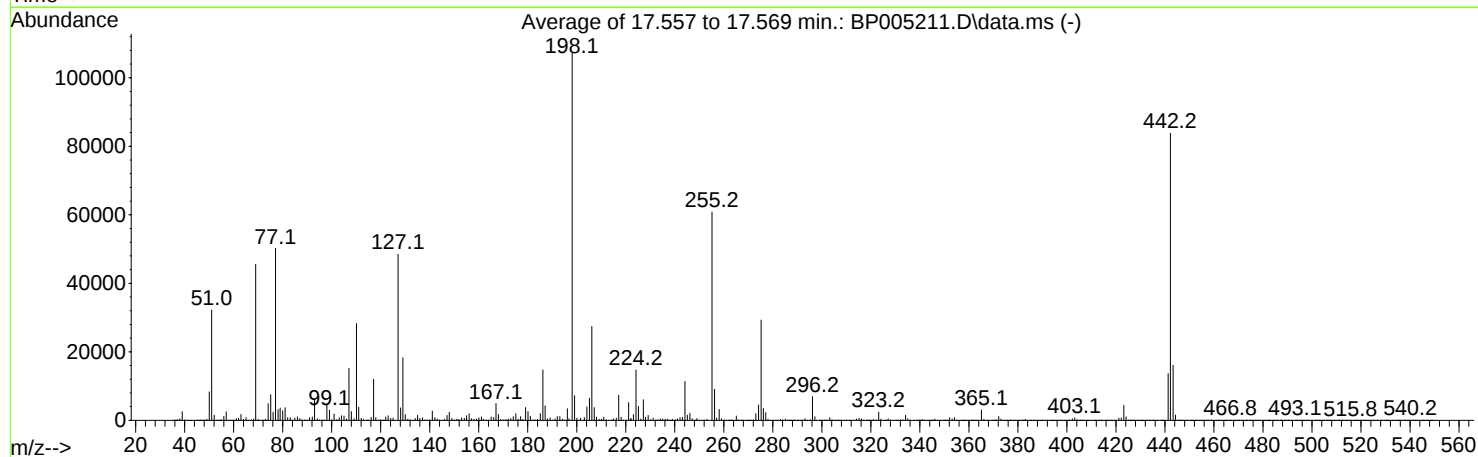


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040721\
 Data File : BP005211.D
 Acq On : 07 Apr 2021 09:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 06 12:33:08 2021

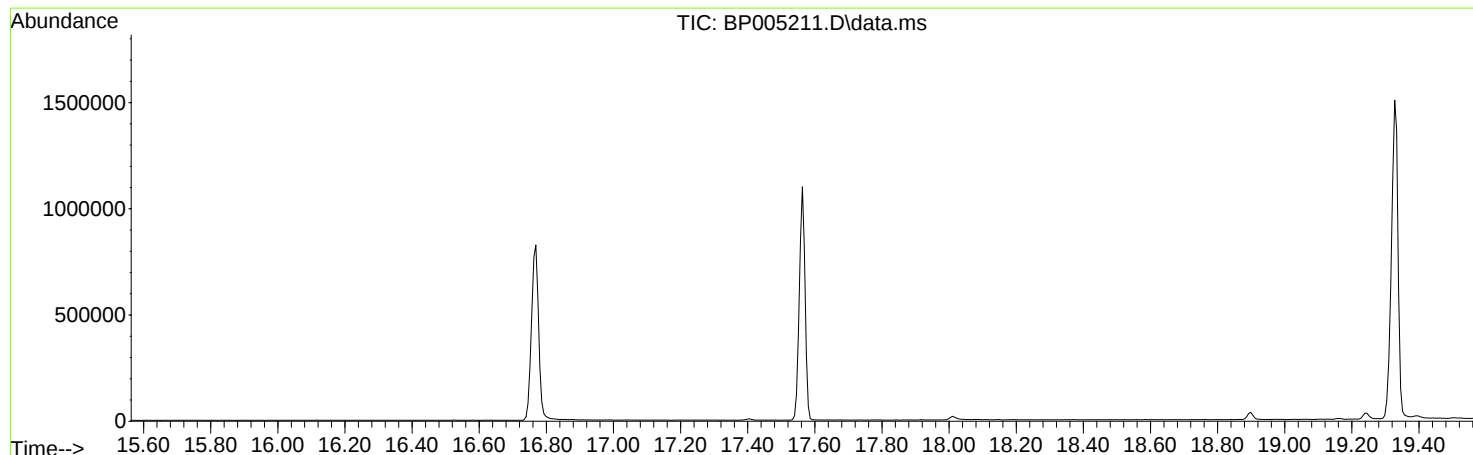

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.0	32219	PASS
68	69	0.00	2	0.8	362	PASS
69	198	0.00	100	42.4	45541	PASS
70	69	0.00	2	0.7	339	PASS
127	198	10	80	45.2	48501	PASS
197	198	0.00	2	0.4	463	PASS
198	198	100	100	100.0	107375	PASS
199	198	5	9	6.7	7213	PASS
275	198	10	60	27.3	29276	PASS
365	198	1	100	2.9	3061	PASS
441	198	0.01	100	12.7	13623	PASS
442	442	100	100	100.0	83809	PASS
443	442	15	24	19.2	16085	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/7/2021	BNA_P	<u>BP005211.D</u>
Compound Name	Response	Retention Time
DDT	414808	20.52
DDD	7258	20.09
DDE	757	19.59
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8015	422823	1.90

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040721\
Data File : BP005211.D
Acq On : 07 Apr 2021 09:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Apr 07 10:59:55 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 06 12:33:08 2021
Response via : Initial Calibration

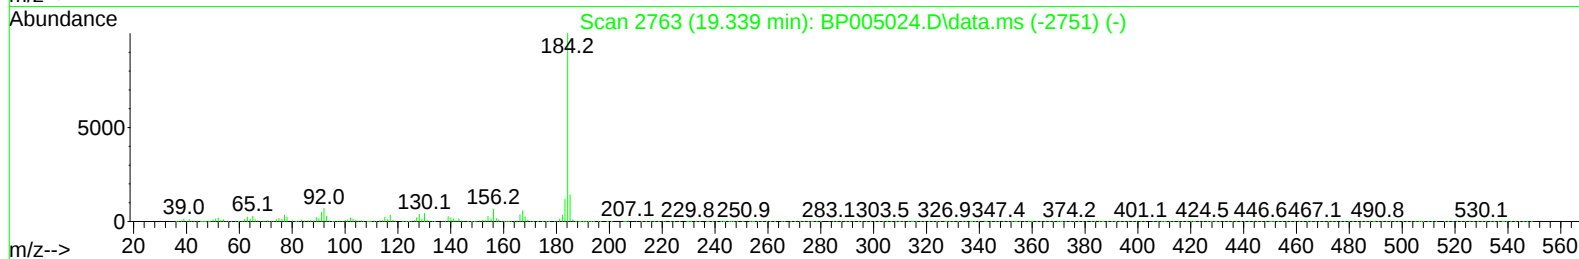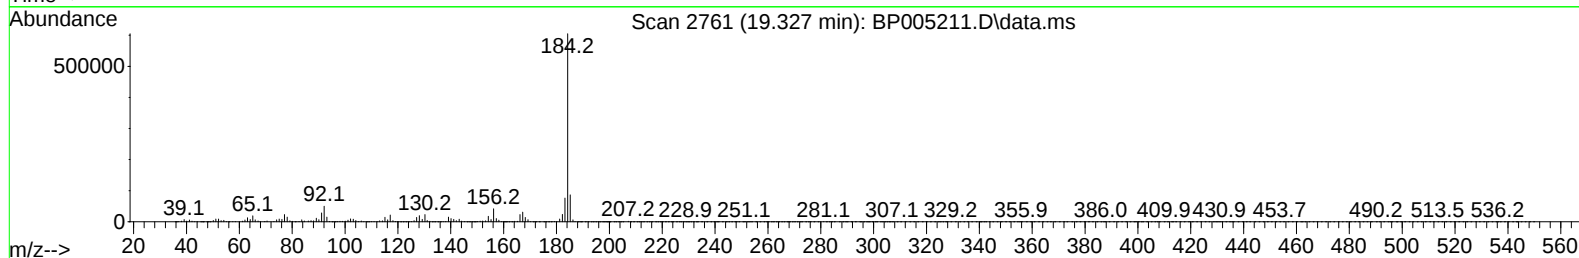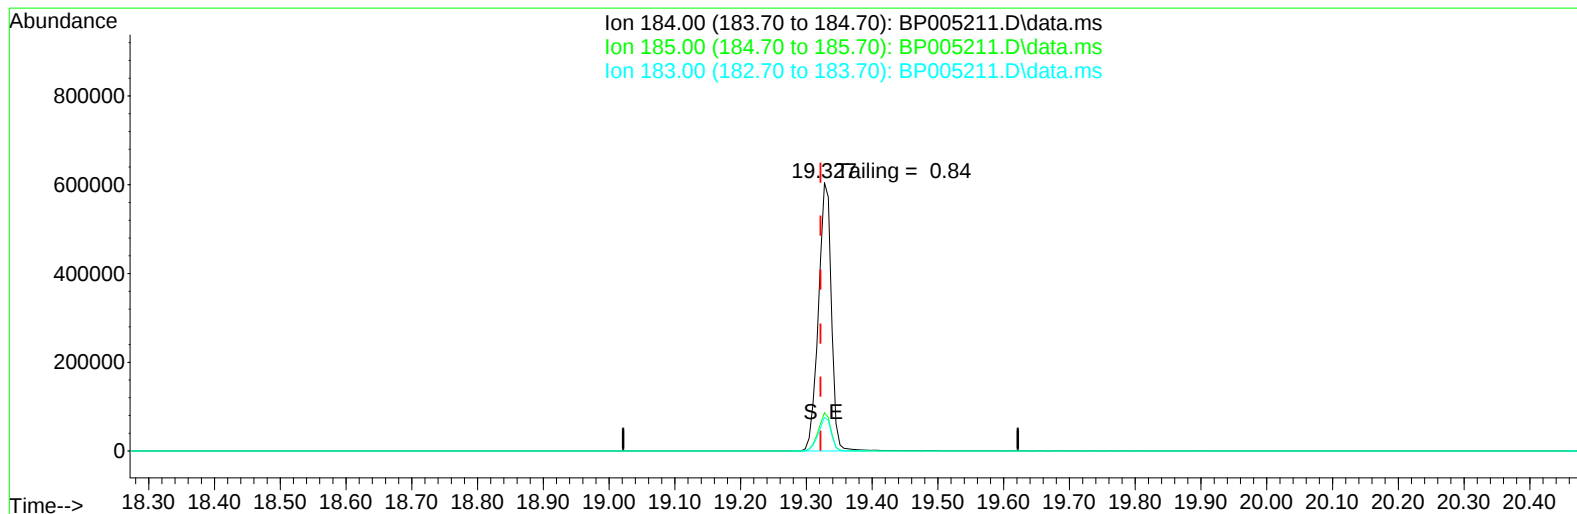

TIC: BP005211.D\data.ms

(77) Benzidine

19.327min (+ 0.006) 1122464.84 ng




response 837323

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.30
183.00	12.00	12.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040721\
 Data File : BP005211.D
 Acq On : 07 Apr 2021 09:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Apr 07 10:59:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 06 12:33:08 2021
 Response via : Initial Calibration

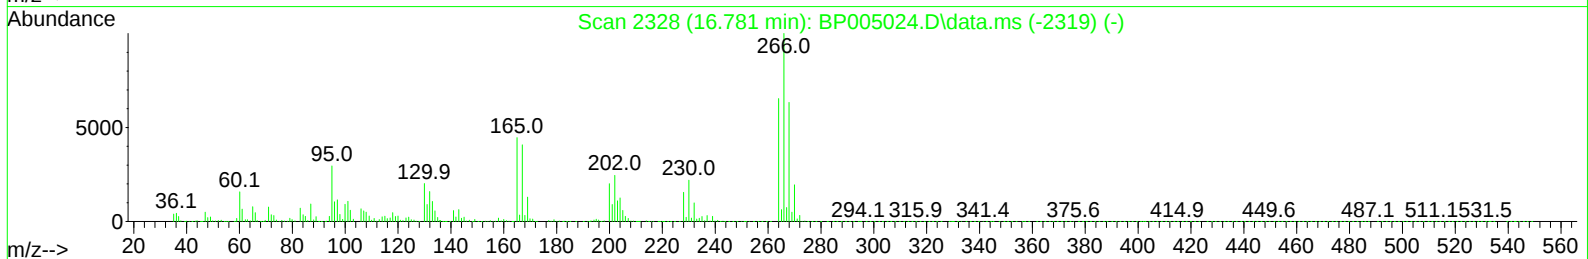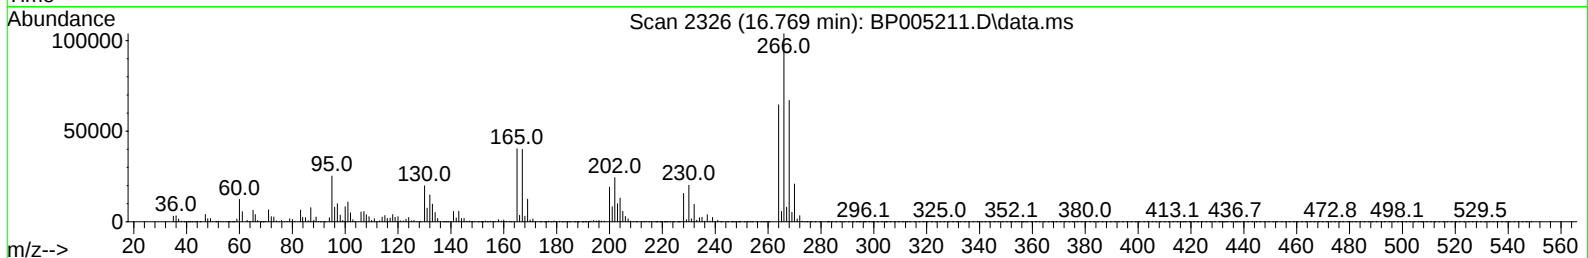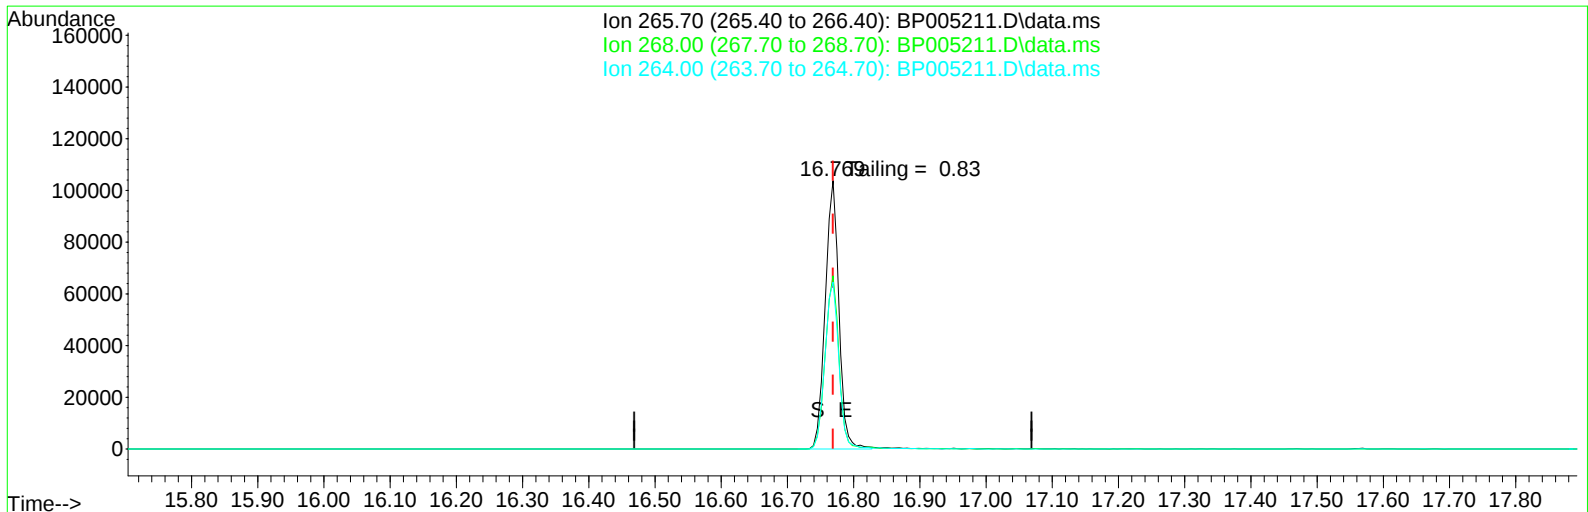

TIC: BP005211.D\data.ms

(70) Pentachlorophenol (C)

16.769min (+ 0.000) 2190995.59 ng

response 150791

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.51
264.00	63.30	62.22
0.00	0.00	0.00