
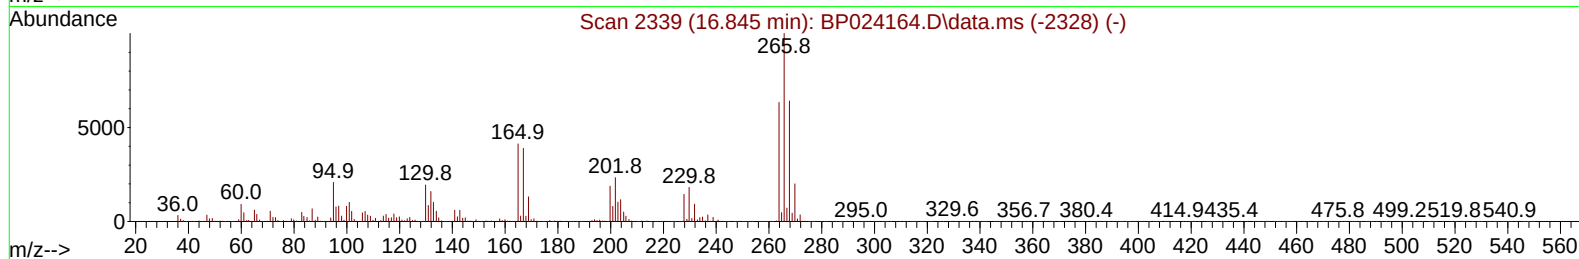
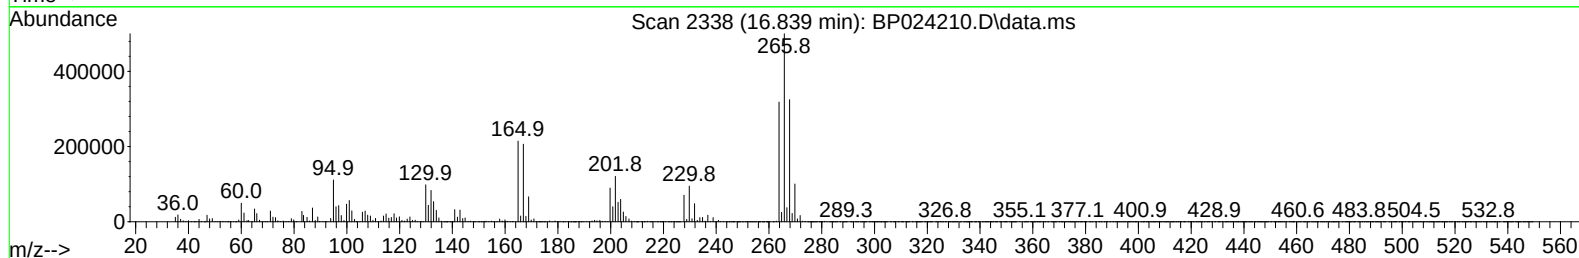


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024210.D
Acq On : 08 Apr 2025 13:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 18:25:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

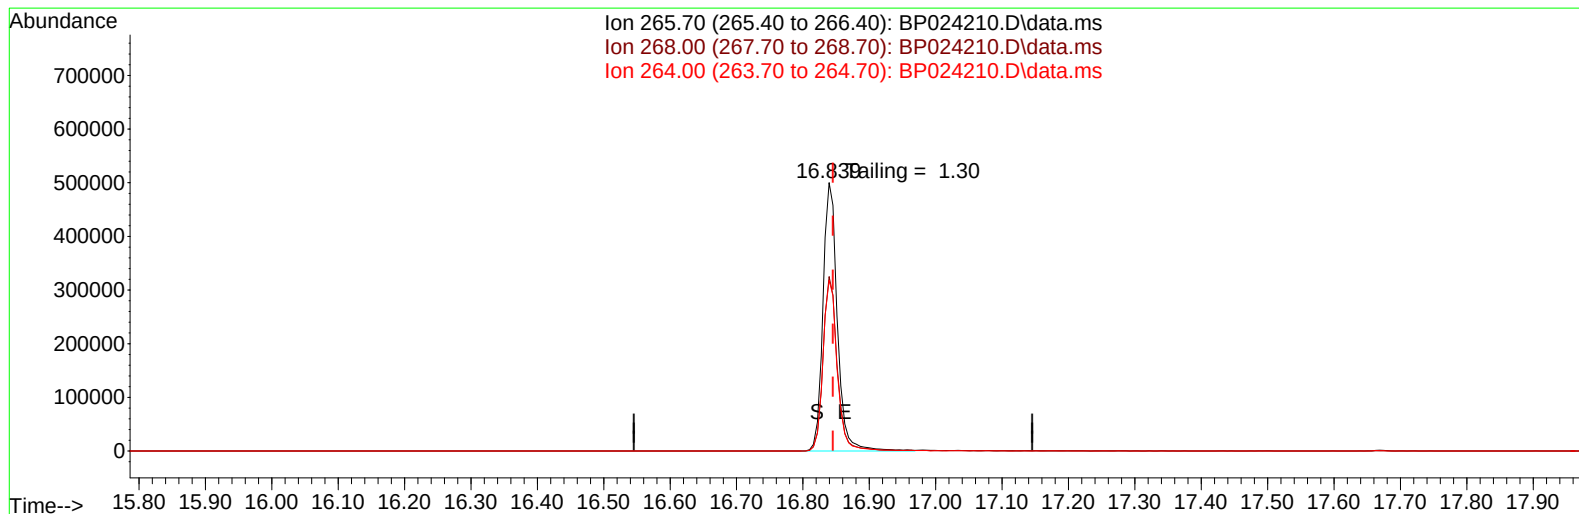

TIC: BP024210.D\data.ms

(70) Pentachlorophenol (C)




16.839min (-0.006) 277531.82 ng

response 753321

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.97
264.00	63.30	63.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024210.D
Acq On : 08 Apr 2025 13:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 18:25:29 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

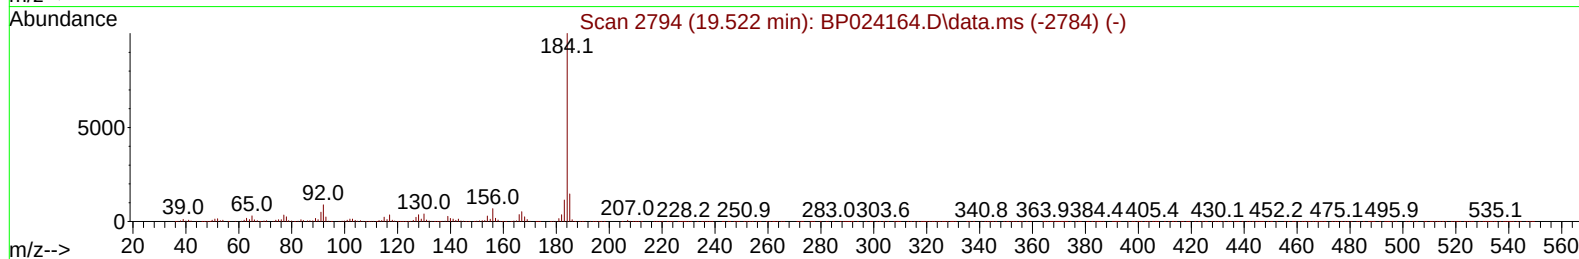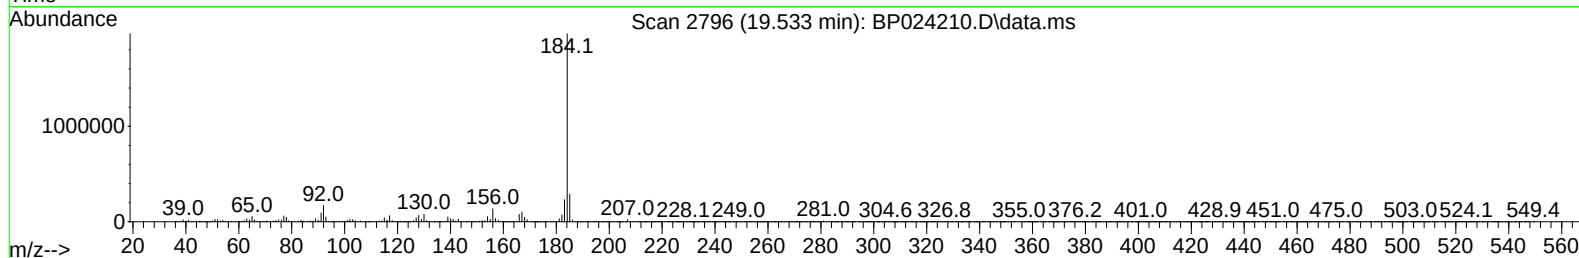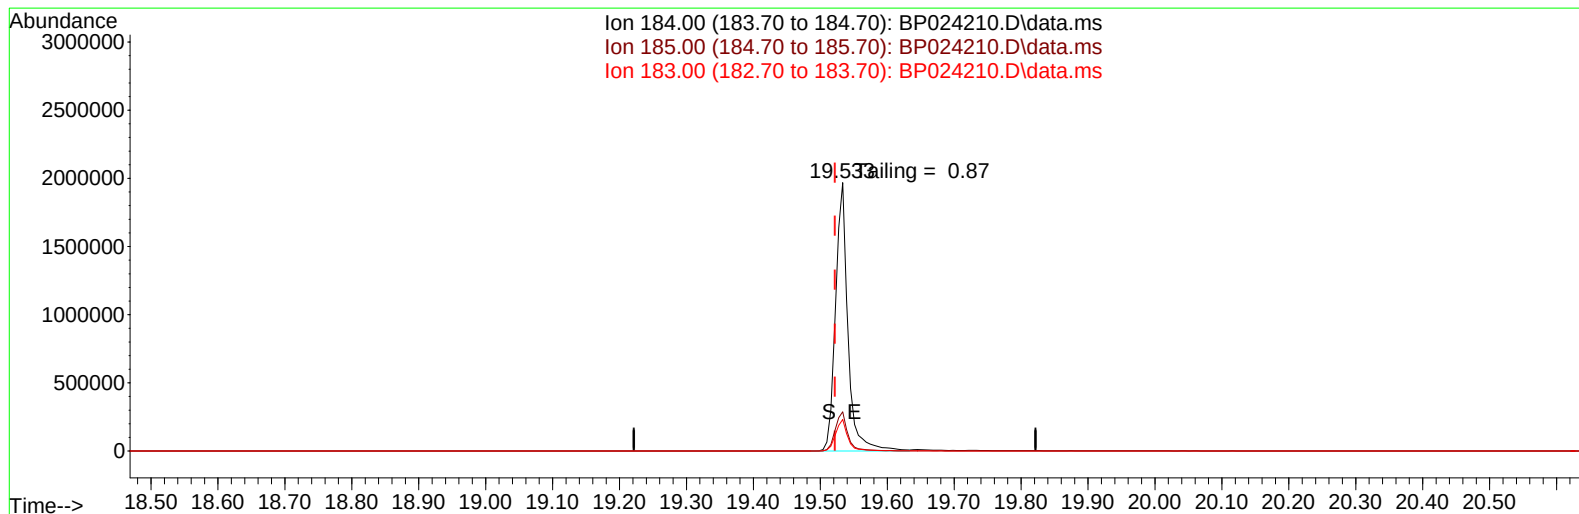

TIC: BP024210.D\data.ms

(77) Benzidine**19.533min (+ 0.012) 6521.01 ng****response 2548937**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.65
183.00	11.40	11.76
0.00	0.00	0.00