

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
 Data File : BP024214.D
 Acq On : 08 Apr 2025 15:45
 Operator : RC/JU
 Sample : Q1730-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-VSL-15-040325

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.899	302	308	322	rVB	831703	1141604	4.53%	1.078%
2	5.358	379	386	399	rBV	5611502	7631013	30.29%	7.208%
3	6.922	644	652	674	rBV	5546355	8676089	34.44%	8.195%
4	7.740	784	791	798	rBV	1294964	1999585	7.94%	1.889%
5	8.887	977	986	998	rBV	3222391	5500204	21.84%	5.196%
6	10.522	1255	1264	1275	rBV	1778178	2957791	11.74%	2.794%
7	12.992	1676	1684	1700	rBV	9777152	14471748	57.45%	13.670%
8	14.381	1913	1920	1936	rBV	2619171	4279346	16.99%	4.042%
9	15.775	2150	2157	2167	rBV	2479830	3184394	12.64%	3.008%
10	15.904	2172	2179	2198	rBV	7350003	10169409	40.37%	9.606%
11	16.351	2250	2255	2265	rVB	316413	397540	1.58%	0.376%
12	17.192	2391	2398	2412	rBV2	3577423	5398393	21.43%	5.099%
13	18.133	2553	2558	2566	rBV	281439	377622	1.50%	0.357%
14	19.927	2856	2863	2868	rBV	19599691	25189292	100.00%	23.794%
15	21.327	3096	3101	3116	rBV	662917	1553940	6.17%	1.468%
16	21.651	3150	3156	3164	rBV	4114315	6526531	25.91%	6.165%
17	25.033	3723	3731	3746	rVB	2436031	6410028	25.45%	6.055%




Sum of corrected areas: 105864529

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024214.D
Acq On : 08 Apr 2025 15:45
Operator : RC/JU
Sample : Q1730-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-VSL-15-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

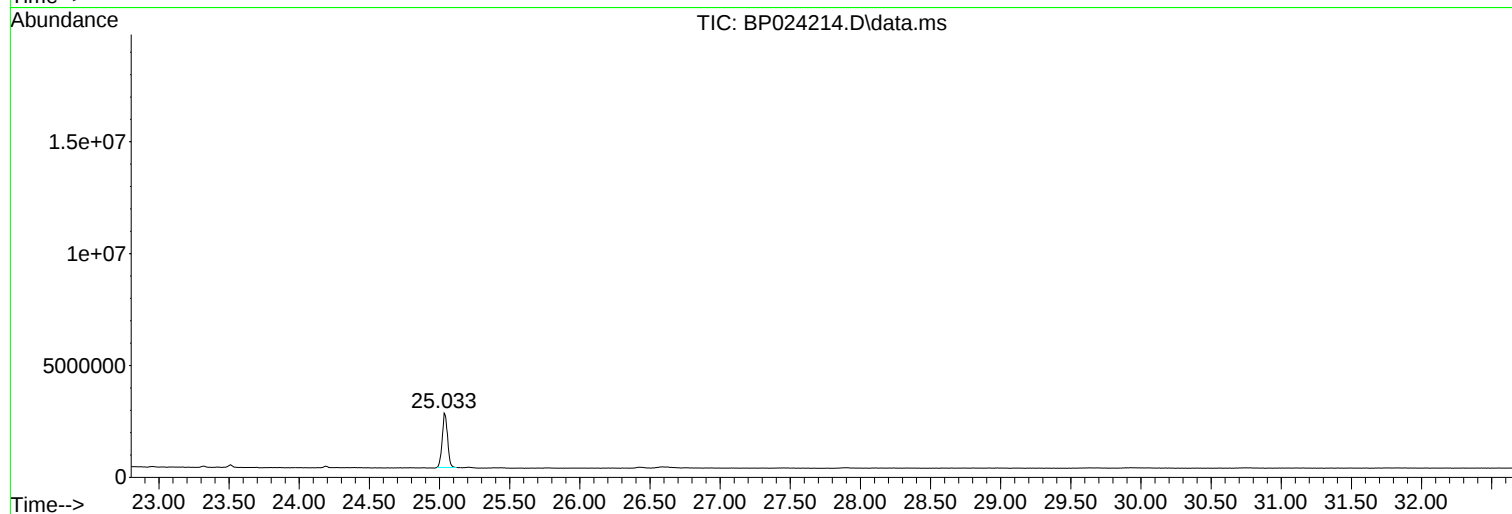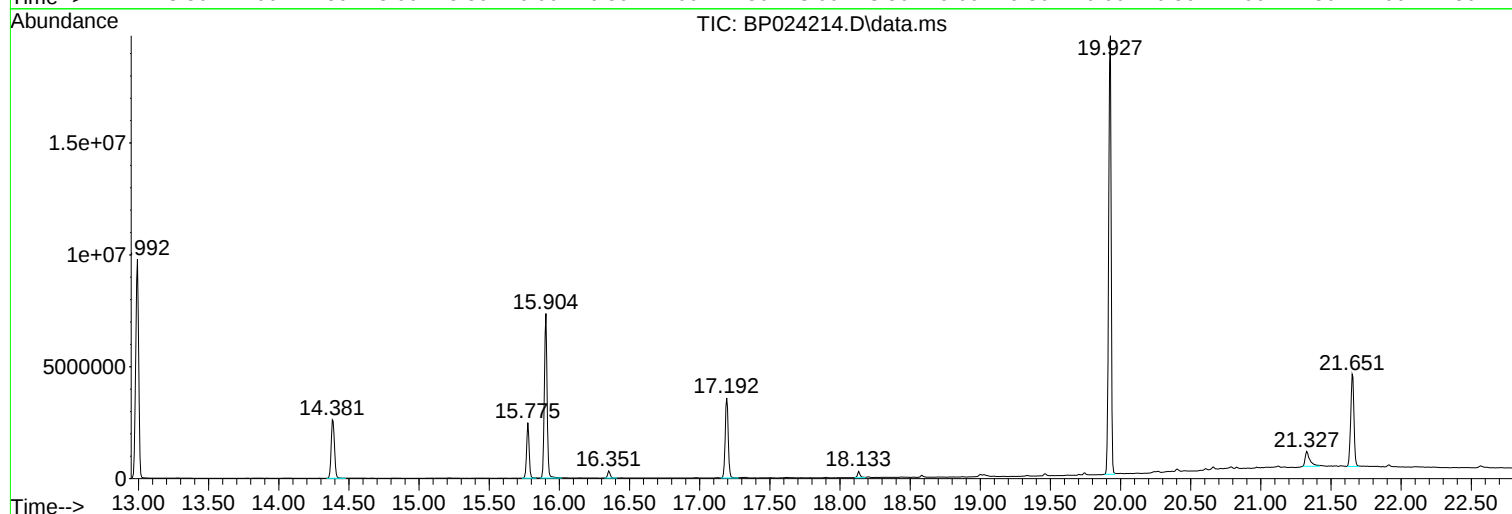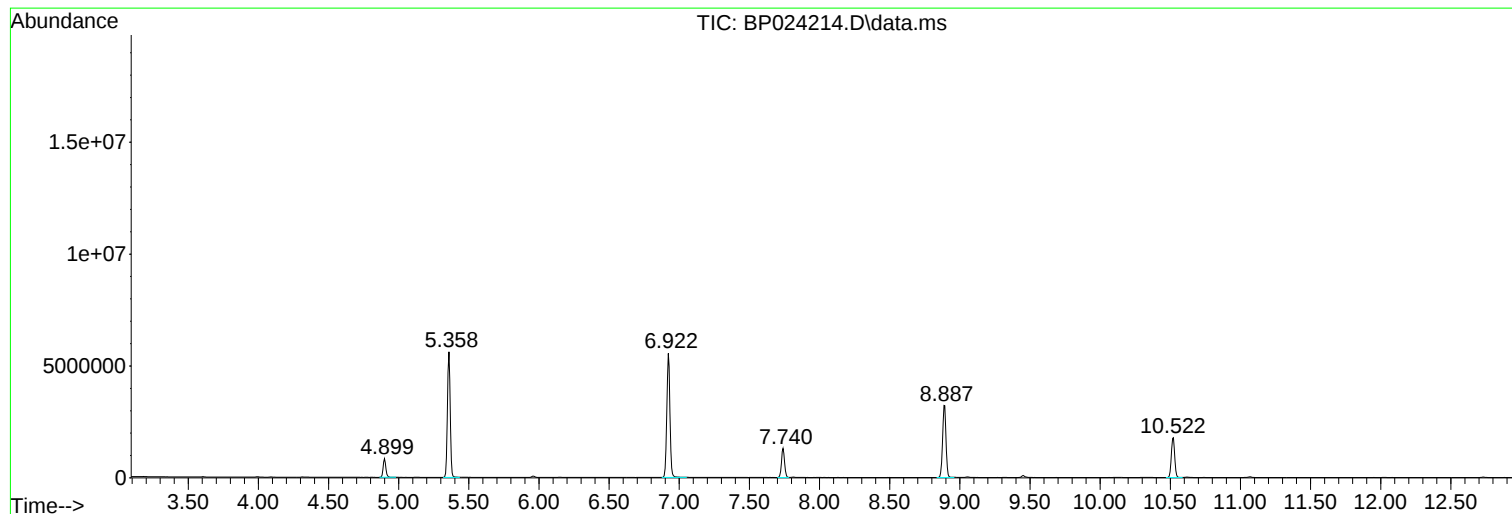

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024214.D
Acq On : 08 Apr 2025 15:45
Operator : RC/JU
Sample : Q1730-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-VSL-15-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024214.D
Acq On : 08 Apr 2025 15:45
Operator : RC/JU
Sample : Q1730-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-VSL-15-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------