

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
 Data File : BP024217.D
 Acq On : 08 Apr 2025 17:47
 Operator : RC/JU
 Sample : Q1730-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-VSL-16-040325

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024217.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.899	302	308	319	rBV	557422	751482	3.77%	0.826%
2	5.358	379	386	403	rBV	4376981	6365543	31.94%	6.998%
3	6.922	643	652	674	rBV	4400410	6974339	34.99%	7.667%
4	7.740	783	791	799	rBV	1394145	2069812	10.38%	2.275%
5	8.887	978	986	998	rBV	2722404	4396676	22.06%	4.833%
6	10.516	1253	1263	1275	rBV	1859617	3079448	15.45%	3.385%
7	12.993	1675	1684	1700	rBV	7563117	11437106	57.38%	12.573%
8	14.387	1911	1921	1929	rBV	3132998	4540638	22.78%	4.992%
9	15.769	2149	2156	2163	rBV	650345	903890	4.54%	0.994%
10	15.904	2171	2179	2201	rBV	6192226	9498655	47.66%	10.442%
11	17.187	2390	2397	2408	rBV2	4015171	5614408	28.17%	6.172%
12	18.128	2552	2557	2566	rBV	929477	1290063	6.47%	1.418%
13	19.457	2779	2783	2790	rBV	212607	278772	1.40%	0.306%
14	19.910	2854	2860	2870	rBV	14854708	19931098	100.00%	21.911%
15	21.316	3095	3099	3118	rVB2	385463	958055	4.81%	1.053%
16	21.645	3149	3155	3162	rBV	4399301	6486978	32.55%	7.131%
17	25.016	3719	3728	3744	rVB	2536446	6387414	32.05%	7.022%




Sum of corrected areas: 90964377

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024217.D
Acq On : 08 Apr 2025 17:47
Operator : RC/JU
Sample : Q1730-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-VSL-16-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

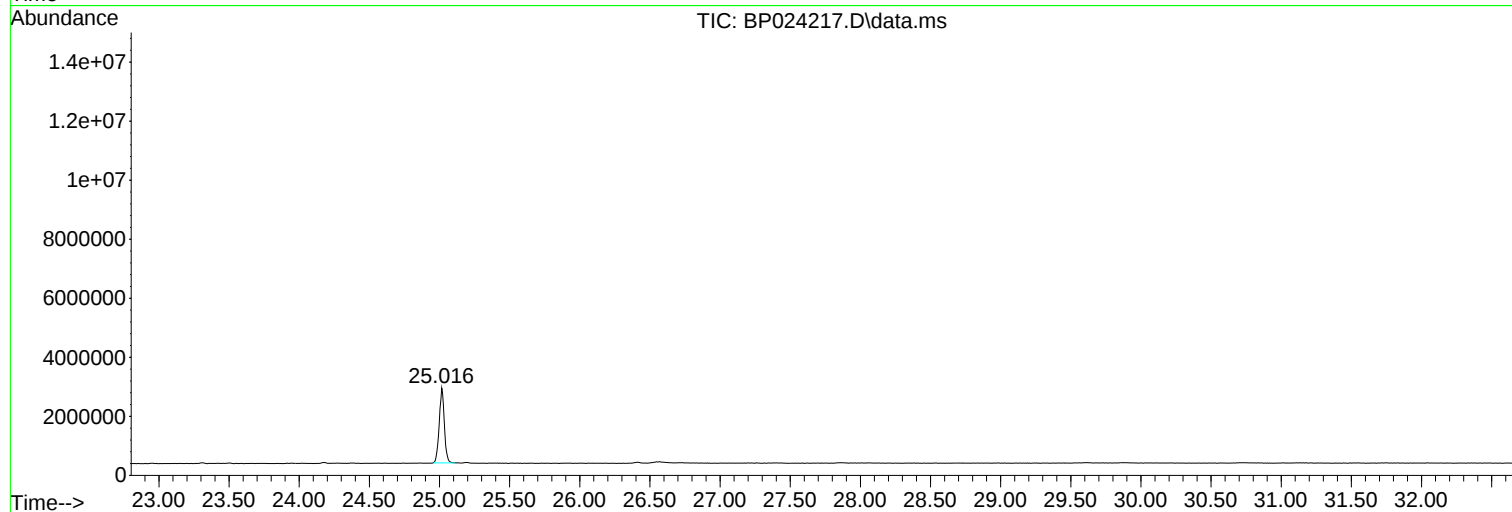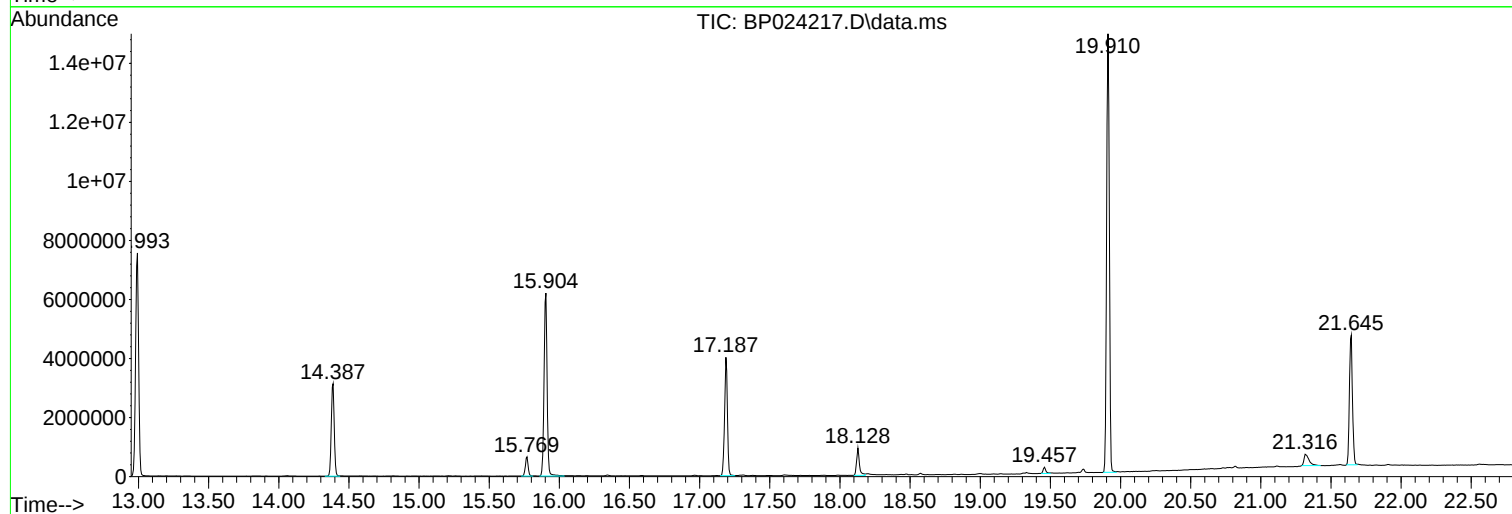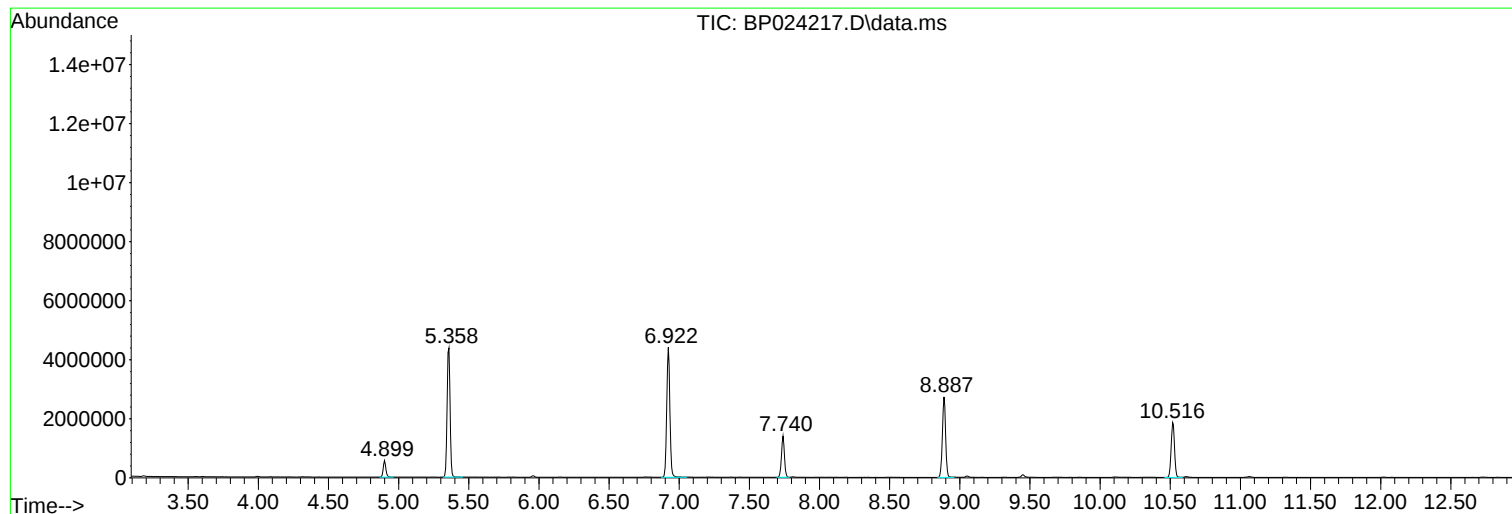

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024217.D
Acq On : 08 Apr 2025 17:47
Operator : RC/JU
Sample : Q1730-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-VSL-16-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024217.D
Acq On : 08 Apr 2025 17:47
Operator : RC/JU
Sample : Q1730-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-VSL-16-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------