

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
 Data File : BP024218.D
 Acq On : 08 Apr 2025 18:28
 Operator : RC/JU
 Sample : Q1730-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-VSL-17-040325

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024218.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.899	302	308	320	rBV	326871	480210	2.64%	0.654%
2	5.352	379	385	398	rBV	2856283	4282389	23.56%	5.835%
3	6.922	645	652	670	rBV	3048504	4812208	26.47%	6.557%
4	7.740	781	791	799	rBV	804801	1250705	6.88%	1.704%
5	8.887	978	986	997	rBV	1837048	2970653	16.34%	4.048%
6	10.522	1256	1264	1278	rBV	1133290	1956212	10.76%	2.666%
7	12.987	1676	1683	1704	rBV	5929017	8007028	44.05%	10.911%
8	14.381	1911	1920	1939	rBV	2064796	3142056	17.28%	4.282%
9	15.763	2148	2155	2162	rBV	531522	707669	3.89%	0.964%
10	15.892	2170	2177	2197	rBV	5642945	7774040	42.77%	10.593%
11	17.180	2389	2396	2410	rBV2	3148038	4502045	24.77%	6.135%
12	18.127	2551	2557	2566	rBV	764966	1092088	6.01%	1.488%
13	19.451	2778	2782	2787	rBV	165943	228396	1.26%	0.311%
14	19.910	2854	2860	2870	rBV	13478299	18178254	100.00%	24.771%
15	21.316	3094	3099	3115	rBV3	309455	846294	4.66%	1.153%
16	21.639	3147	3154	3171	rVB	3884389	6383130	35.11%	8.698%
17	25.021	3721	3729	3744	rVB	2755206	6772962	37.26%	9.229%




Sum of corrected areas: 73386339

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024218.D
Acq On : 08 Apr 2025 18:28
Operator : RC/JU
Sample : Q1730-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-VSL-17-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

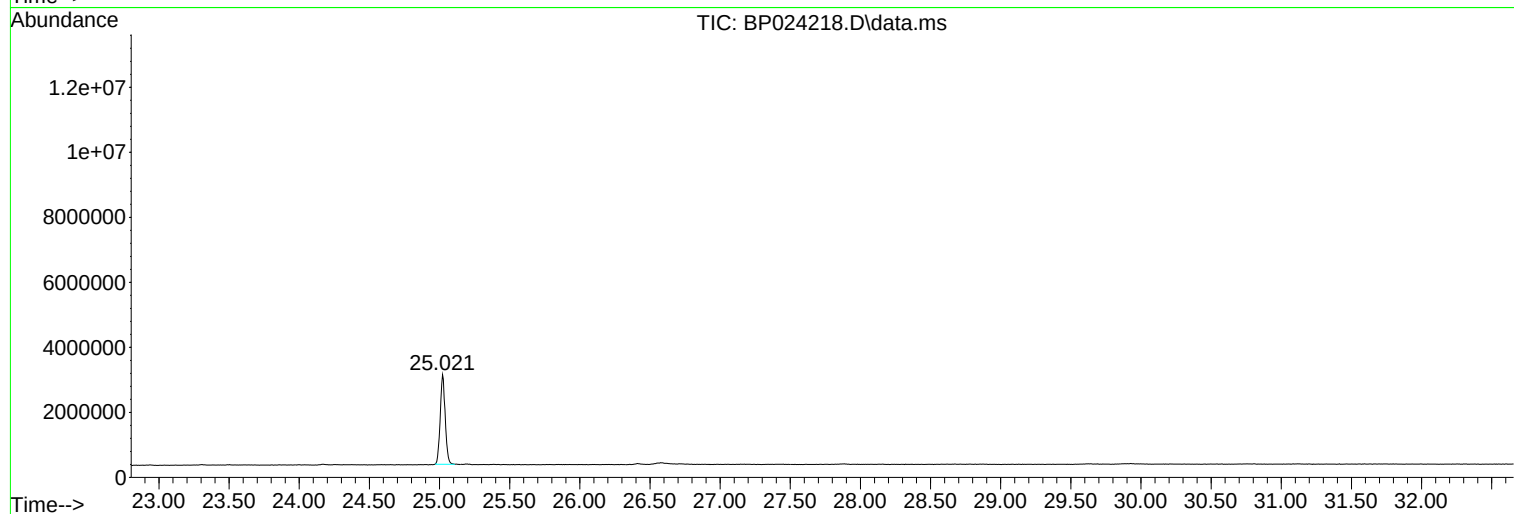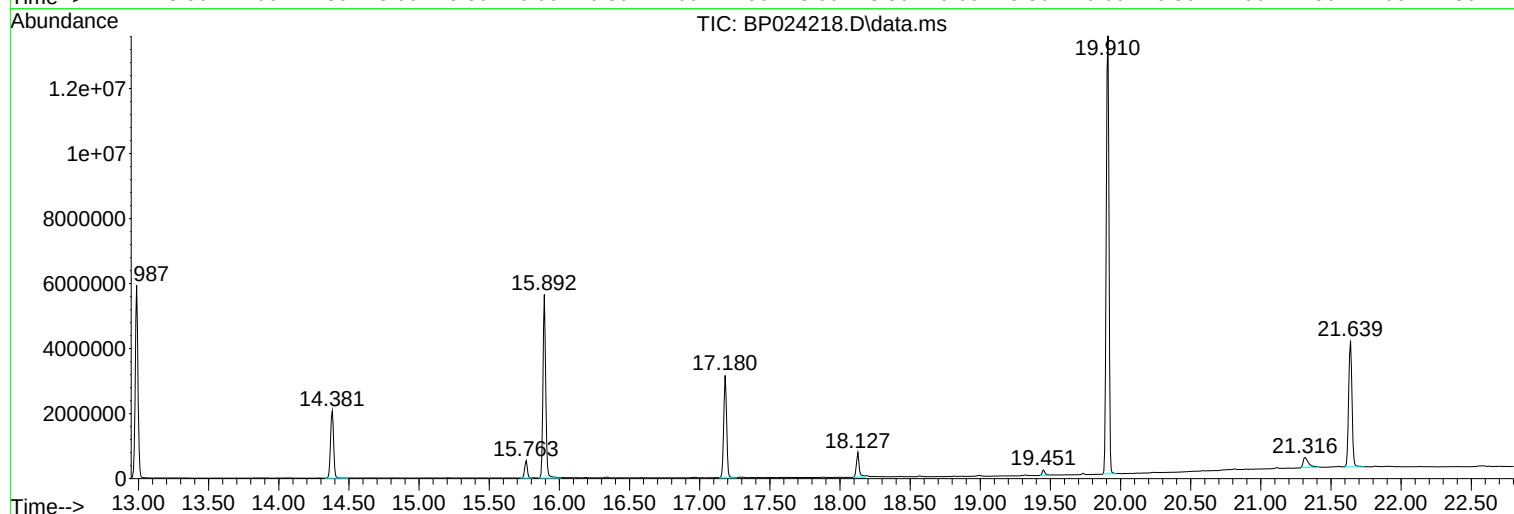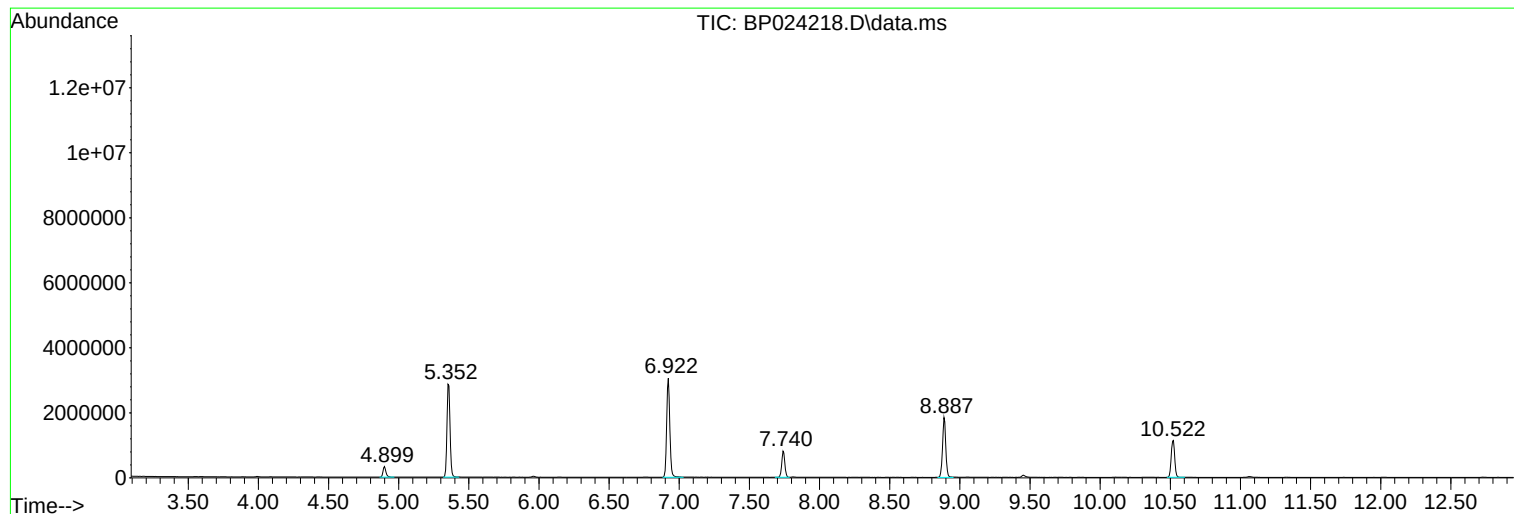

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024218.D
Acq On : 08 Apr 2025 18:28
Operator : RC/JU
Sample : Q1730-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-VSL-17-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024218.D
Acq On : 08 Apr 2025 18:28
Operator : RC/JU
Sample : Q1730-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-VSL-17-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------