

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
 Data File : BP024219.D
 Acq On : 08 Apr 2025 19:09
 Operator : RC/JU
 Sample : Q1730-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-PCS-TC-21-040325

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.899	303	308	320	rVB	502115	688942	5.41%	1.028%
2	5.358	379	386	403	rBV	4401057	5993612	47.07%	8.941%
3	6.922	644	652	672	rBV	3904118	6121762	48.08%	9.133%
4	7.740	783	791	798	rBV	1230749	1936852	15.21%	2.889%
5	8.887	976	986	996	rBV	2396312	3840285	30.16%	5.729%
6	9.452	1075	1082	1094	rBV2	73654	140208	1.10%	0.209%
7	10.516	1255	1263	1276	rBV	1621911	2621100	20.59%	3.910%
8	12.987	1675	1683	1699	rBV	5797527	8664687	68.05%	12.926%
9	14.375	1912	1919	1932	rBV	2253871	3294819	25.88%	4.915%
10	15.763	2148	2155	2164	rBV	429048	596404	4.68%	0.890%
11	15.892	2171	2177	2198	rBV	4472817	6227830	48.91%	9.291%
12	17.186	2390	2397	2411	rBV2	2585781	3676744	28.88%	5.485%
13	18.128	2552	2557	2566	rBV	504333	698045	5.48%	1.041%
14	19.457	2779	2783	2787	rBV	112436	141873	1.11%	0.212%
15	19.910	2854	2860	2873	rBV	10294769	12733007	100.00%	18.995%
16	21.304	3093	3097	3108	rBV2	207263	528185	4.15%	0.788%
17	21.633	3146	3153	3166	rBV	2737012	4484424	35.22%	6.690%
18	25.021	3719	3729	3744	rVB2	1508235	4643334	36.47%	6.927%




Sum of corrected areas: 67032113

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024219.D
Acq On : 08 Apr 2025 19:09
Operator : RC/JU
Sample : Q1730-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-21-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

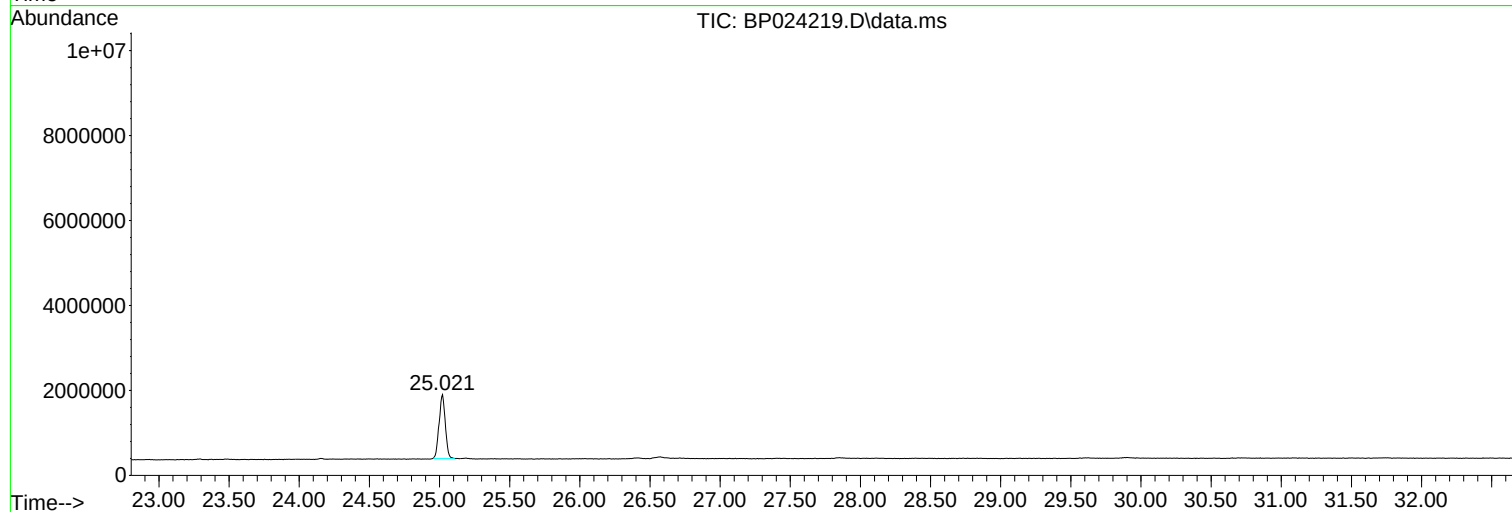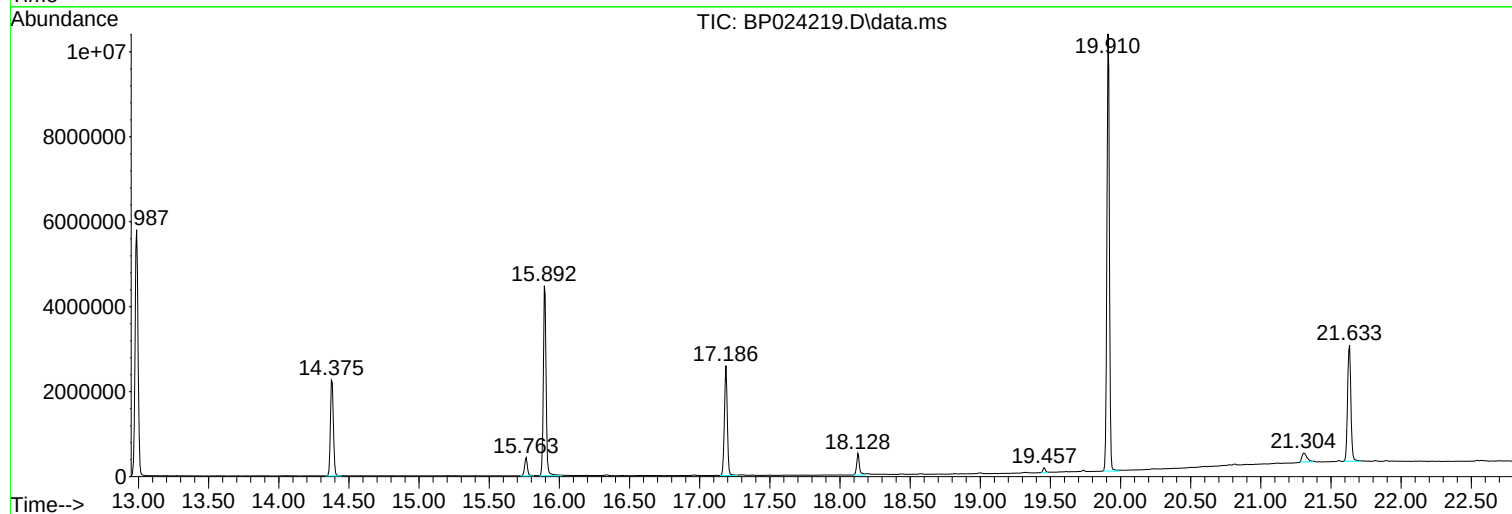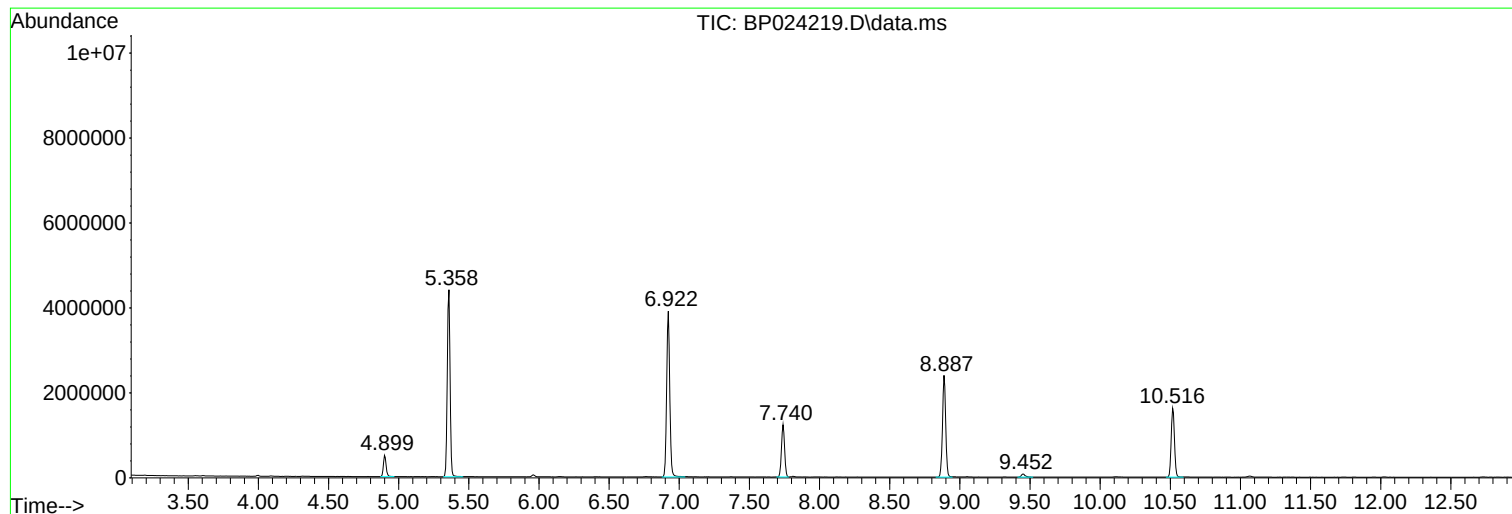

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024219.D
Acq On : 08 Apr 2025 19:09
Operator : RC/JU
Sample : Q1730-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-21-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024219.D
Acq On : 08 Apr 2025 19:09
Operator : RC/JU
Sample : Q1730-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-21-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------