

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
 Data File : BP024220.D
 Acq On : 08 Apr 2025 19:50
 Operator : RC/JU
 Sample : Q1730-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-PCS-TC-22-040325

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.899	303	308	321	rBV	561866	776905	4.85%	0.950%
2	5.357	379	386	399	rBV	4531267	6428441	40.10%	7.857%
3	6.922	644	652	669	rBV	4423566	6994999	43.64%	8.549%
4	7.740	783	791	799	rBV	1579142	2405399	15.01%	2.940%
5	8.887	975	986	1004	rBV	2574384	4228123	26.38%	5.168%
6	9.451	1075	1082	1094	rVB	96467	165931	1.04%	0.203%
7	10.522	1256	1264	1273	rBV	2156774	3428002	21.38%	4.190%
8	12.986	1676	1683	1706	rBV	7395401	10286676	64.17%	12.572%
9	14.375	1911	1919	1931	rBV	3376876	4649711	29.01%	5.683%
10	15.763	2148	2155	2162	rBV	753348	1032879	6.44%	1.262%
11	15.892	2169	2177	2197	rBV	5643918	8564928	53.43%	10.468%
12	17.180	2389	2396	2409	rBV2	3599163	5357207	33.42%	6.548%
13	18.127	2550	2557	2566	rBV	867932	1379820	8.61%	1.686%
14	19.451	2778	2782	2792	rBV	228168	363484	2.27%	0.444%
15	19.910	2854	2860	2868	rBV	11944735	16030018	100.00%	19.592%
16	21.315	3095	3099	3110	rBV	323311	725160	4.52%	0.886%
17	21.639	3148	3154	3162	rBV2	3041807	5056696	31.55%	6.180%
18	25.027	3722	3730	3743	rVB	1504531	3944856	24.61%	4.821%




Sum of corrected areas: 81819235

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024220.D
Acq On : 08 Apr 2025 19:50
Operator : RC/JU
Sample : Q1730-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-22-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

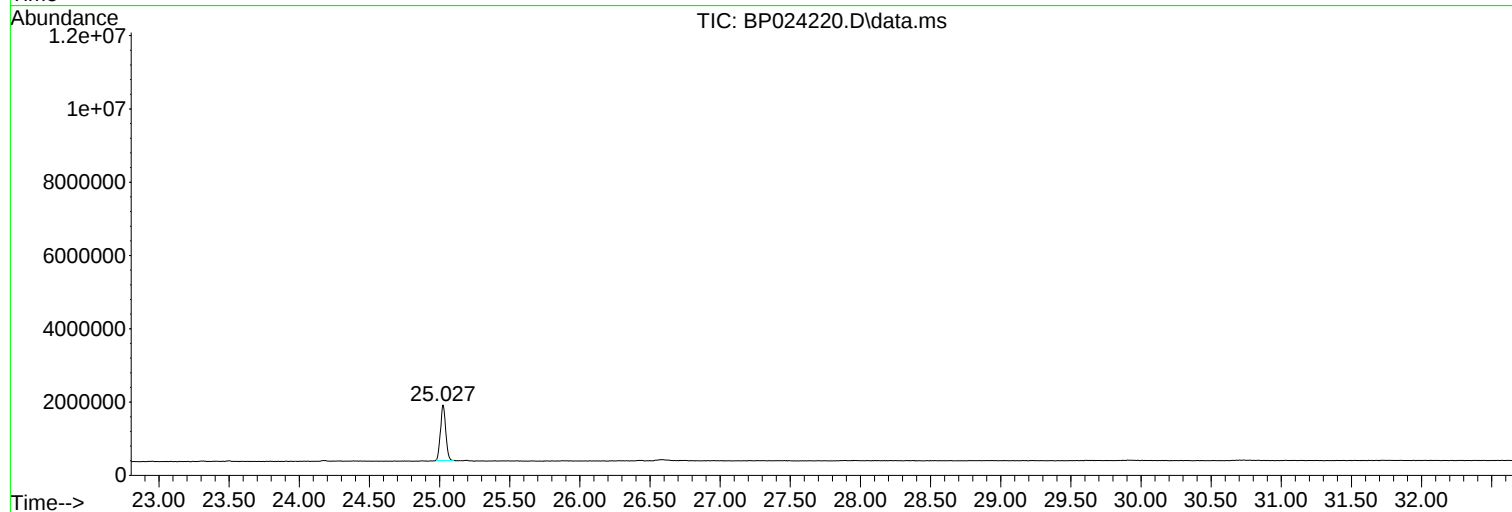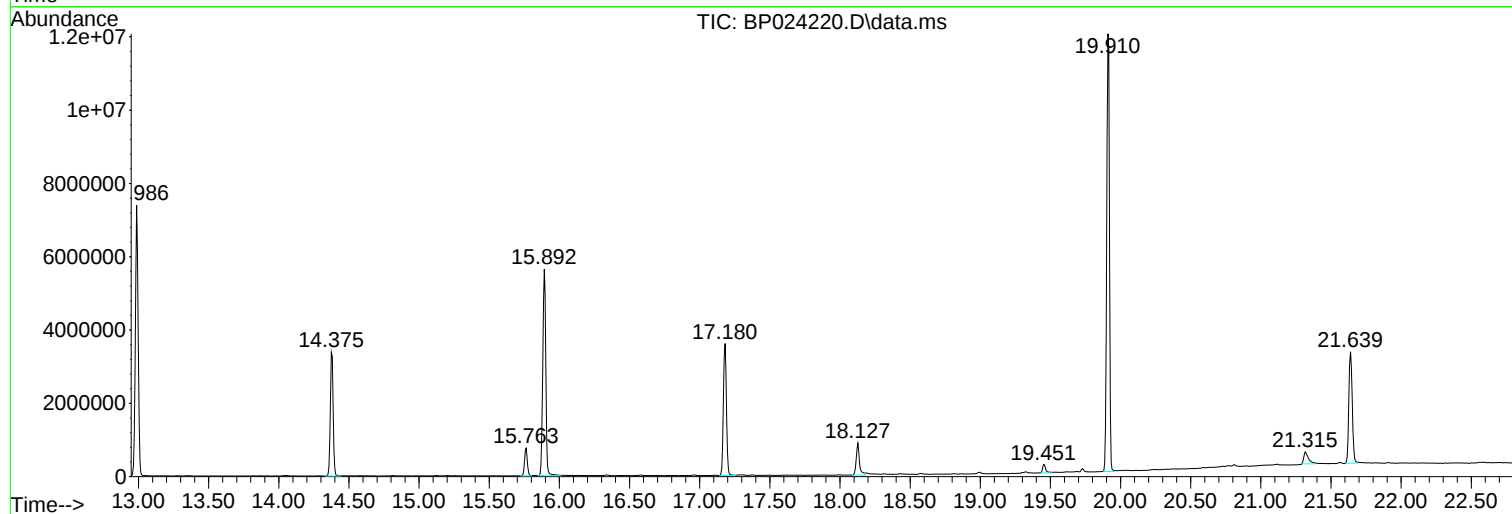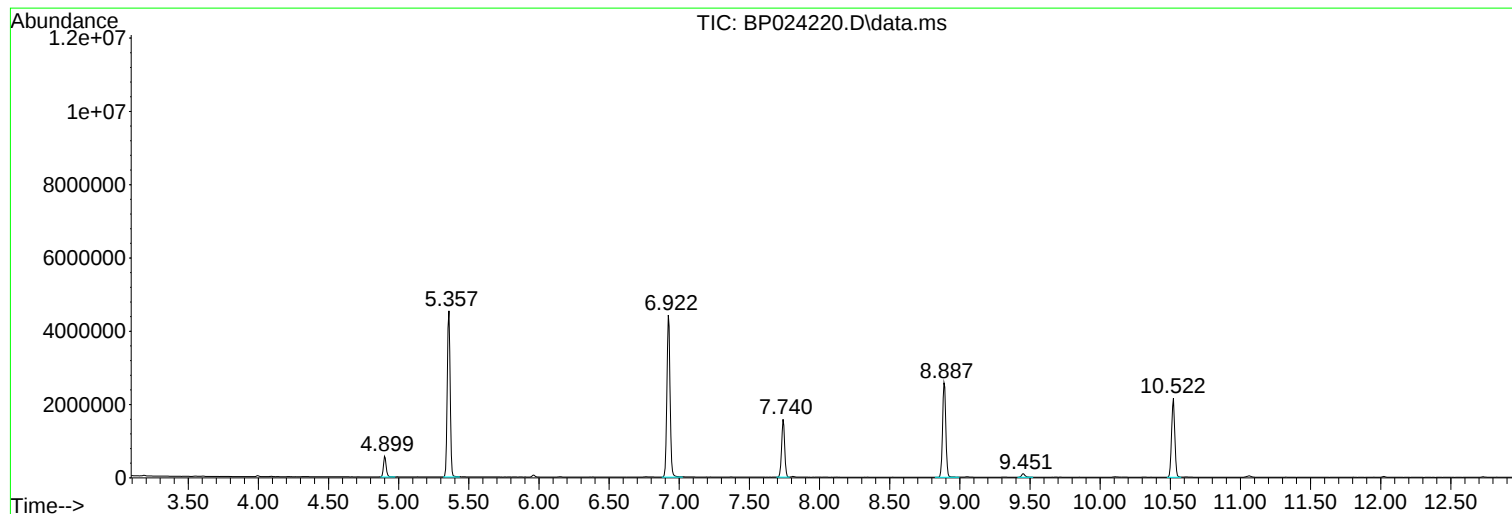

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024220.D
Acq On : 08 Apr 2025 19:50
Operator : RC/JU
Sample : Q1730-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-22-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP040825\
Data File : BP024220.D
Acq On : 08 Apr 2025 19:50
Operator : RC/JU
Sample : Q1730-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-PCS-TC-22-040325

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc